

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 22:38
Operator : SM/SJ
Sample : J4310-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
C-2

Manual Integrations
APPROVED

Sohil
8/6/2018 12:41:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:27:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.396	3.642	3811490	4676128	18.878m	19.031
2) SA Decachlor...	10.087	8.631	2432110	2505532	14.912	15.939

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 22:38
Operator : SM/SJ
Sample : J4310-03
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
C-2


Manual Integrations
APPROVED

Sohil
8/6/2018 12:41:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 04:27:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

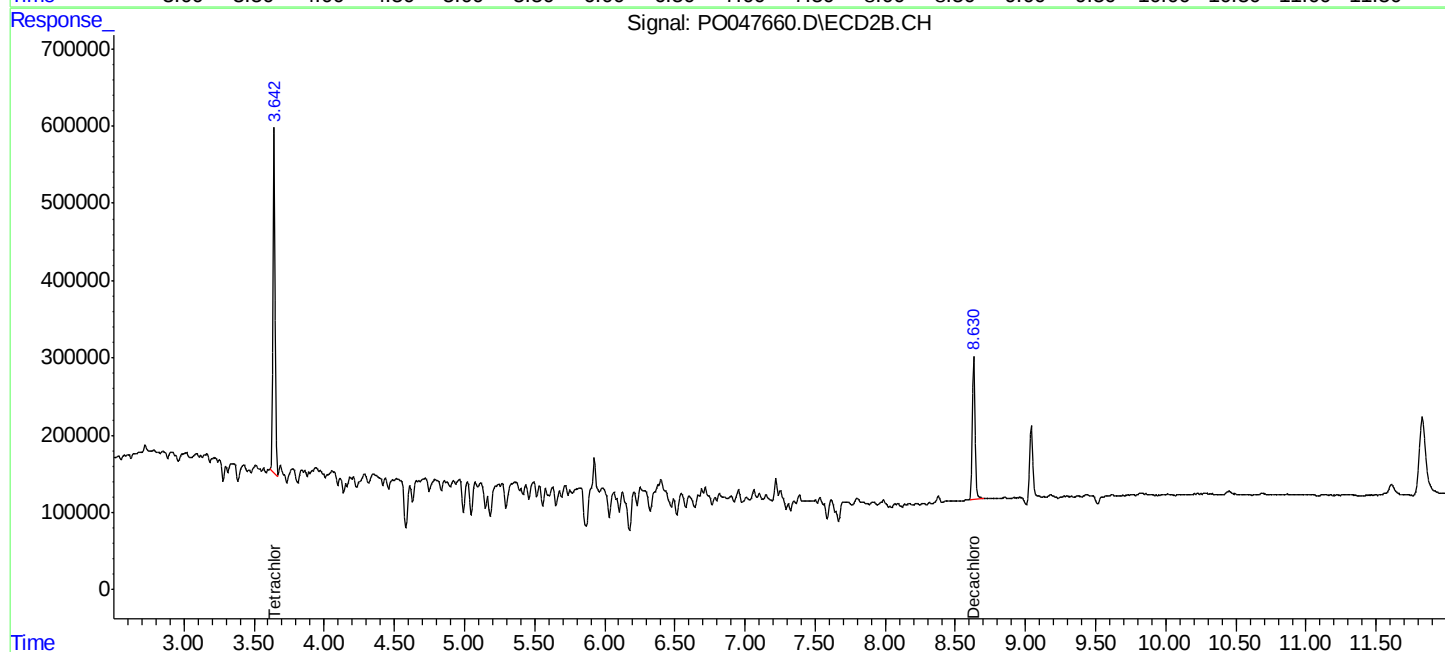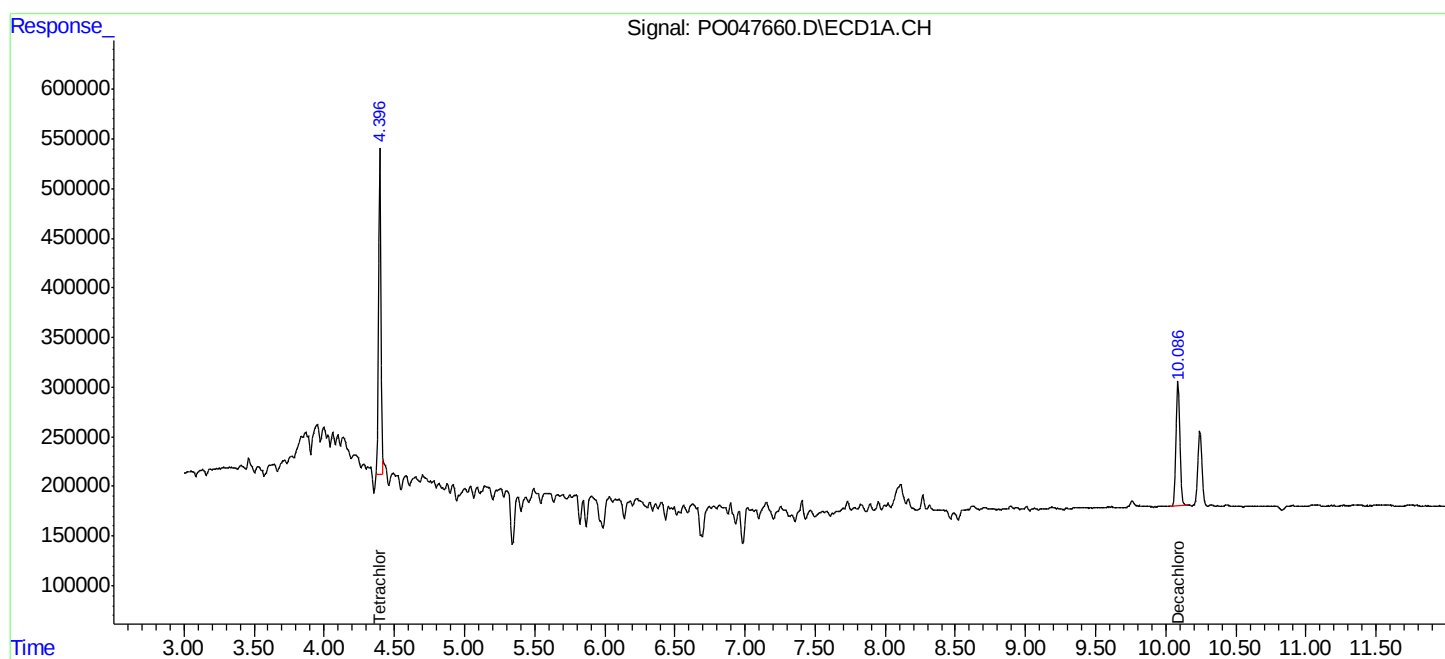

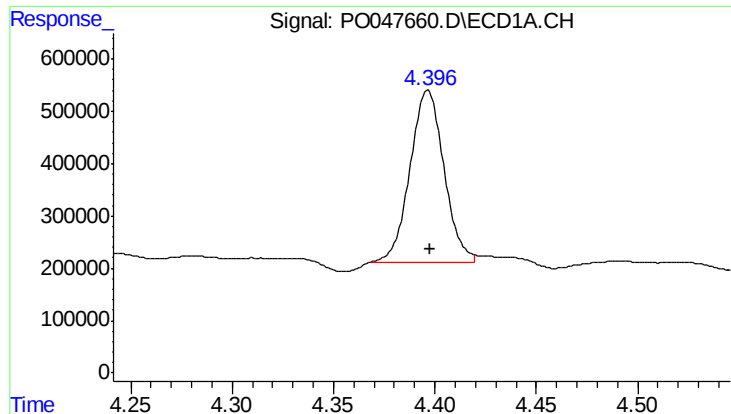


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: -0.001 min
Response: 3811490
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-2


Manual Integrations
APPROVED

Sohil
8/6/2018 12:41:10 PM

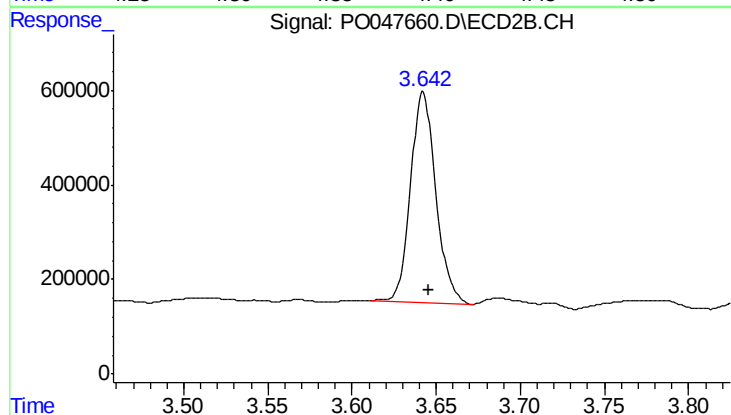


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 4676128
Conc: 19.03 ng/ml

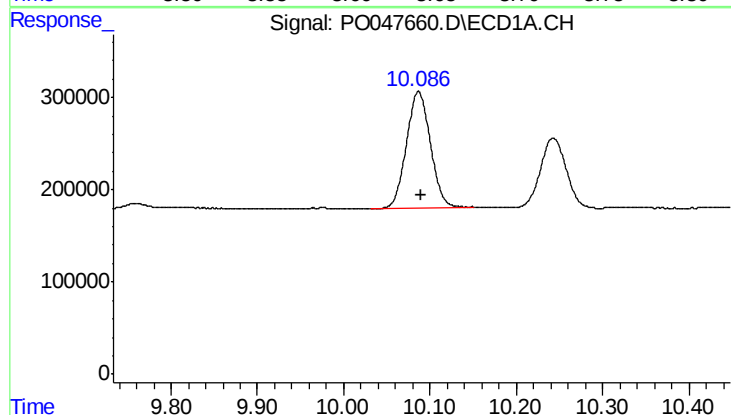

#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: -0.003 min
Response: 2432110
Conc: 14.91 ng/ml

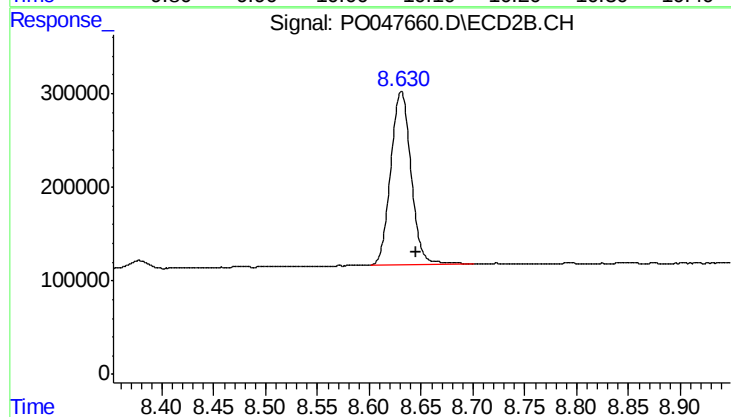

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: -0.014 min
Response: 2505532
Conc: 15.94 ng/ml