

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047665.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 23:57
Operator : SM/SJ
Sample : J4313-05
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
C-7

Manual Integrations
APPROVED

Sohil
8/6/2018 2:24:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:23:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.643	4369340	4981431	21.641	20.273
2) SA Decachlor...	10.086	8.628	4361435	3931412	26.741m	25.010

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047665.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2018 23:57
Operator : SM/SJ
Sample : J4313-05
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
C-7


Manual Integrations
APPROVED

Sohil
8/6/2018 2:24:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:23:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

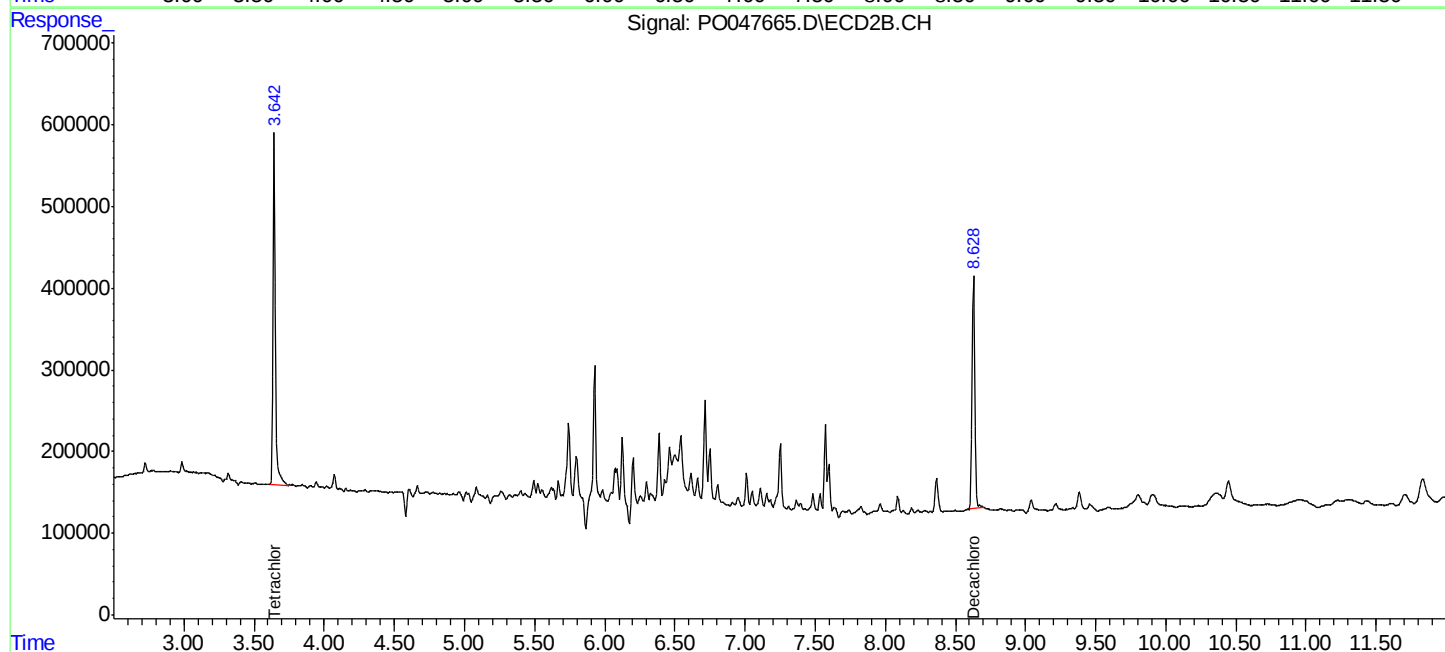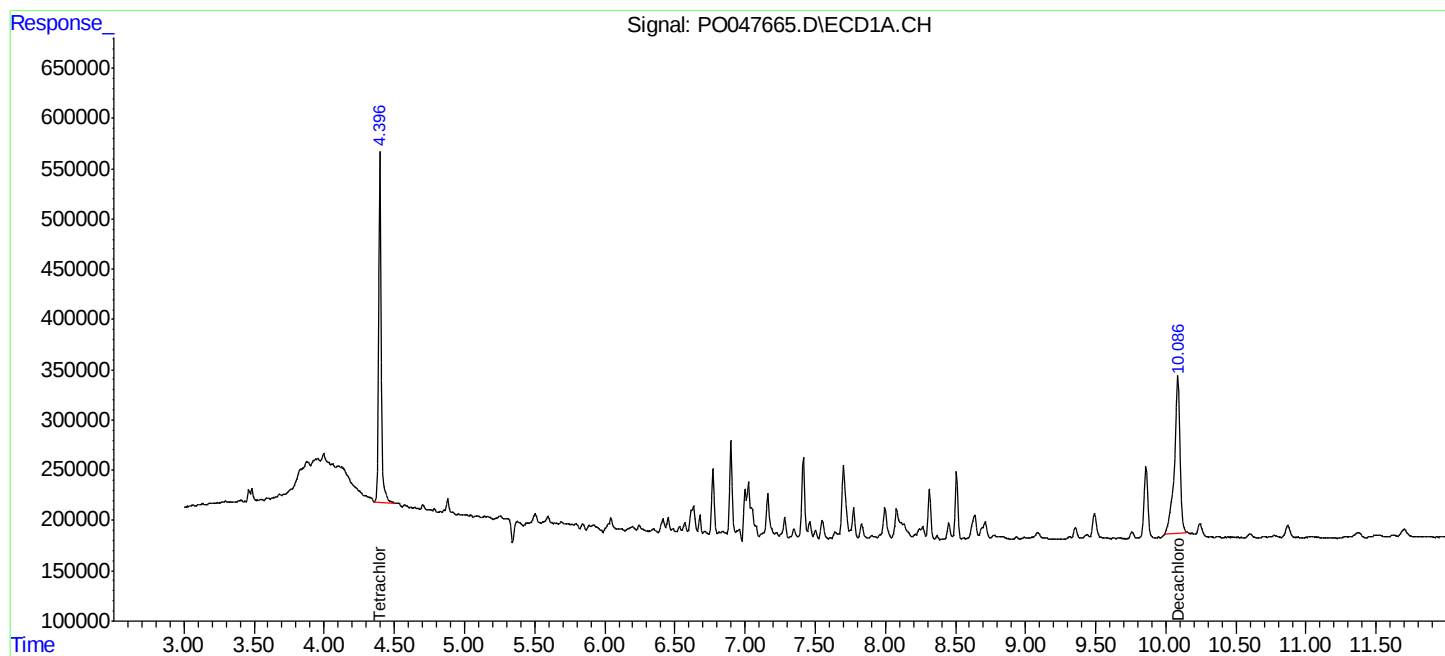

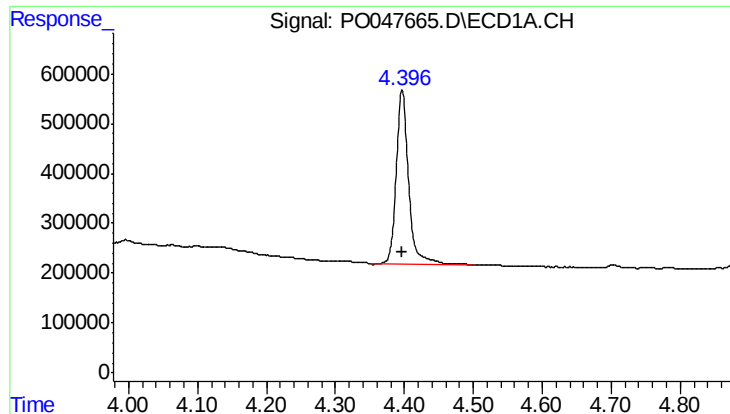


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 4369340
Conc: 21.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-7


Manual Integrations
APPROVED

Sohil
8/6/2018 2:24:52 PM

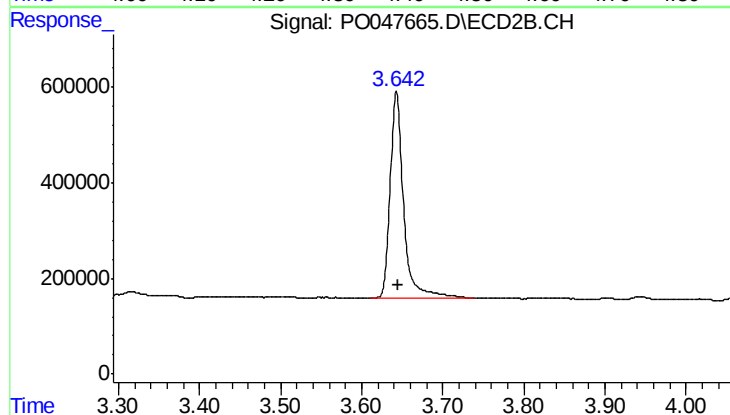


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.003 min
Response: 4981431
Conc: 20.27 ng/ml

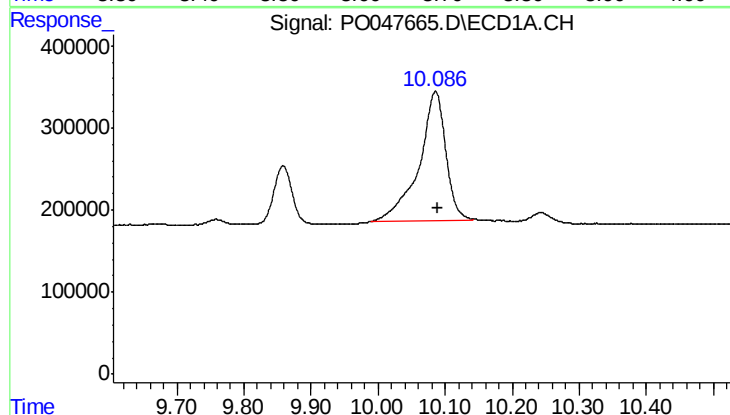

#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: -0.004 min
Response: 4361435
Conc: 26.74 ng/ml m

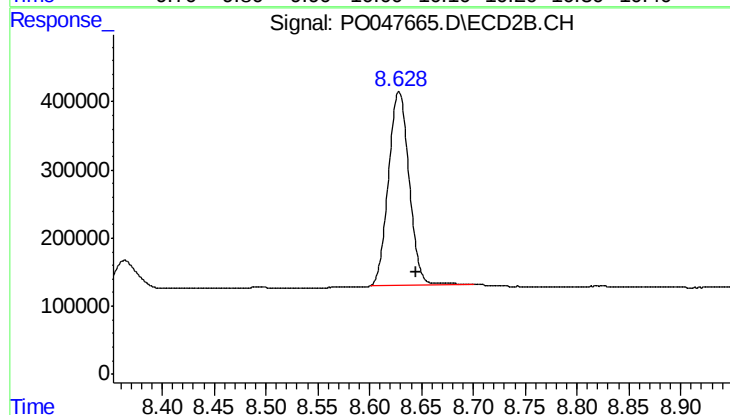

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.016 min
Response: 3931412
Conc: 25.01 ng/ml