

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047678.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2018 4:13
Operator : SM/SJ
Sample : J4313-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
C-14

Manual Integrations
APPROVED

Sohil
8/6/2018 2:25:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:36:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.397	3.643	5076343	5466627	25.143m	22.248m
2) SA Decachlor...	10.087	8.629	3058309	3247981	18.751	20.663

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047678.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2018 4:13
Operator : SM/SJ
Sample : J4313-19
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
C-14


Manual Integrations
APPROVED

Sohil
8/6/2018 2:25:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:36:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

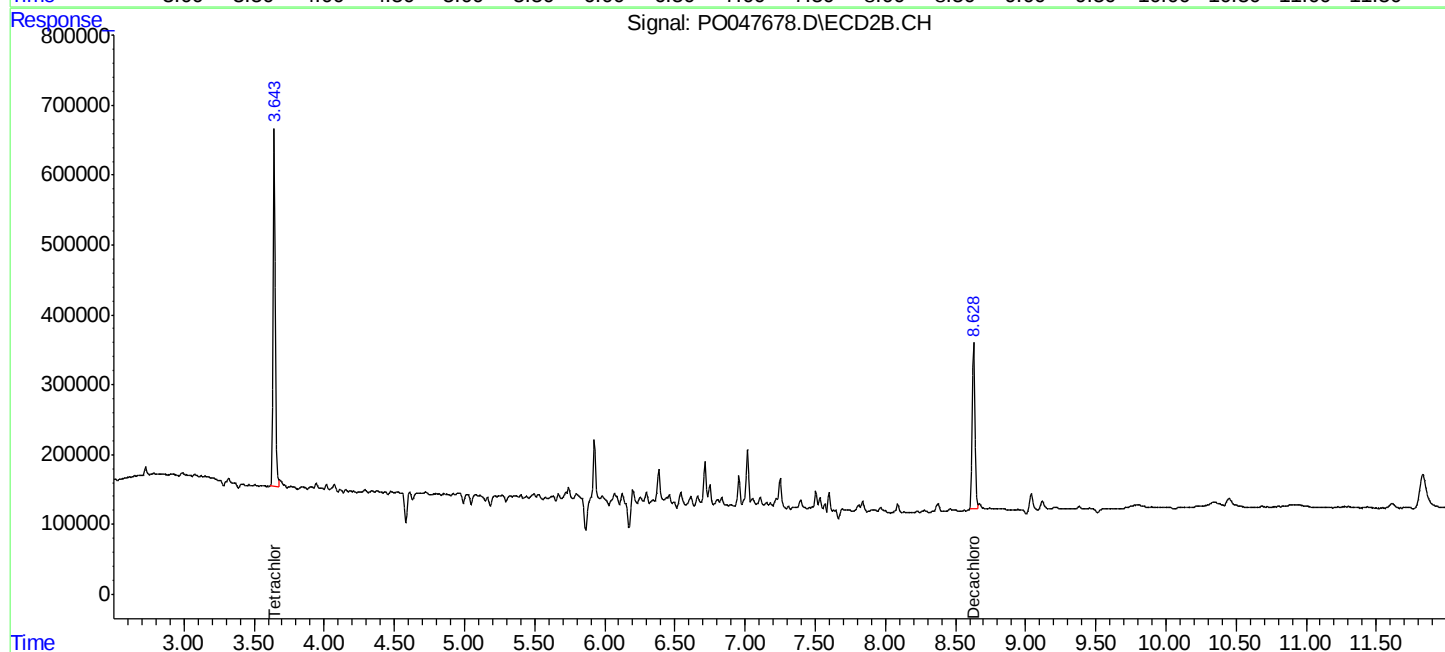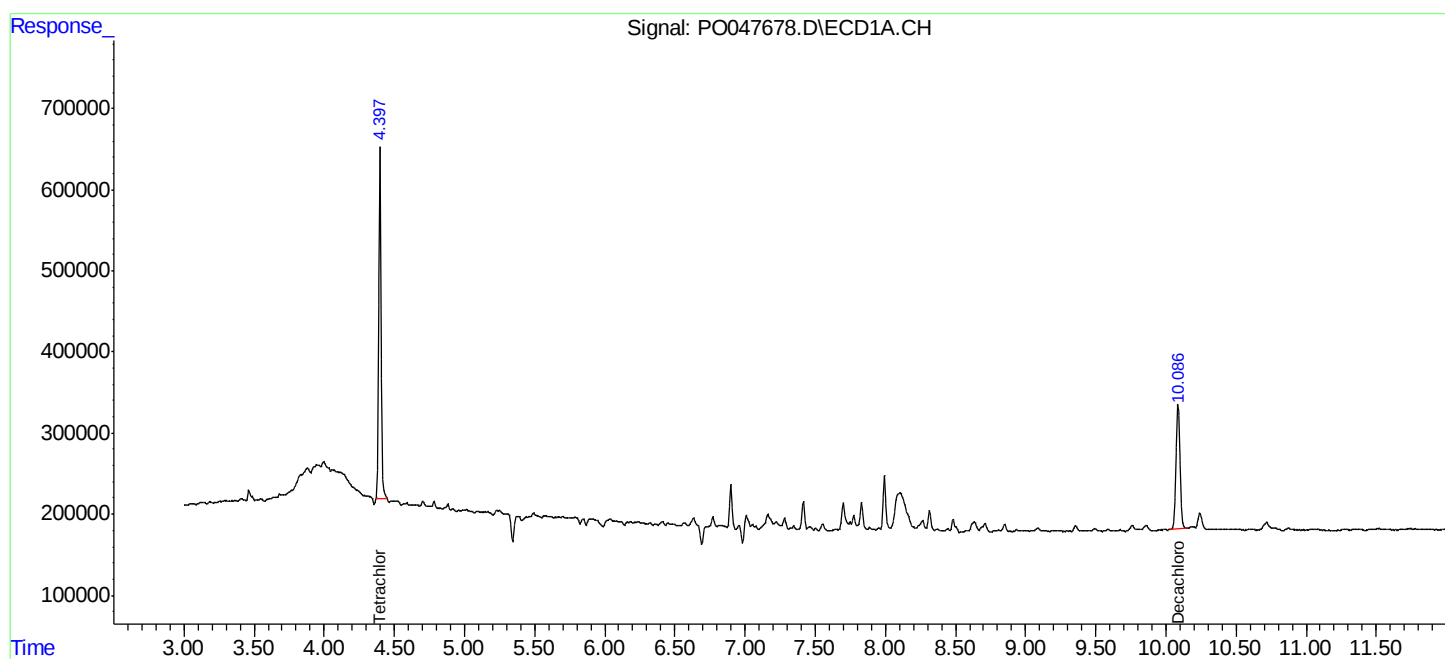

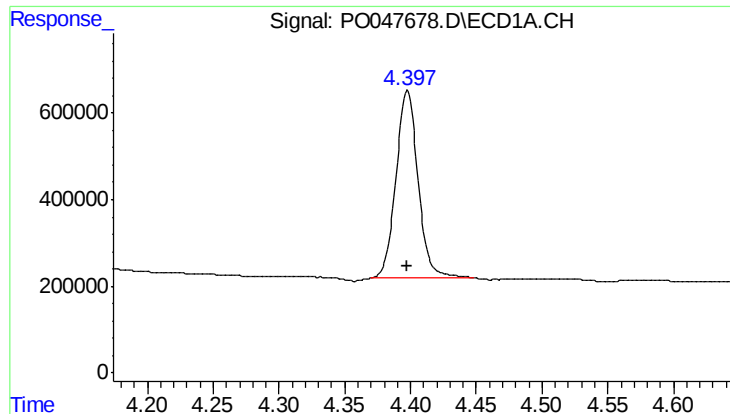


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 5076343
Conc: 25.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-14


Manual Integrations
APPROVED

Sohil
8/6/2018 2:25:04 PM

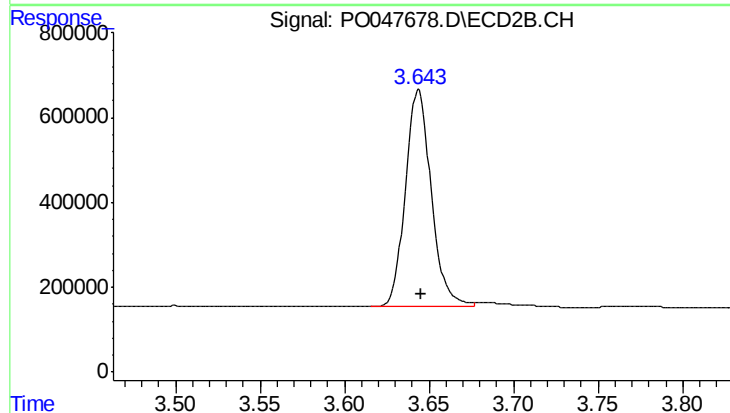


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 5466627
Conc: 22.25 ng/ml m

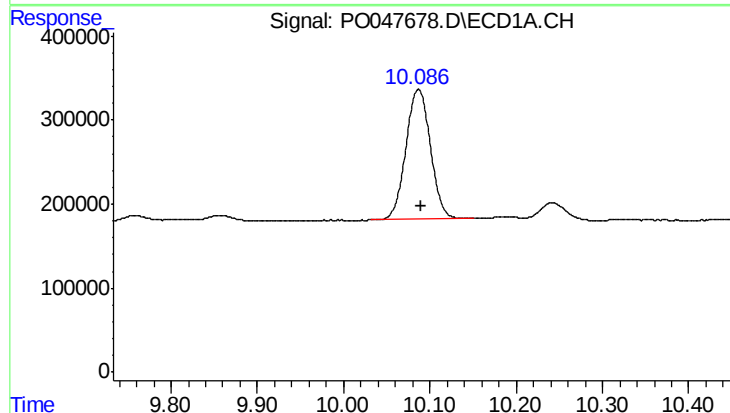

#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: -0.003 min
Response: 3058309
Conc: 18.75 ng/ml

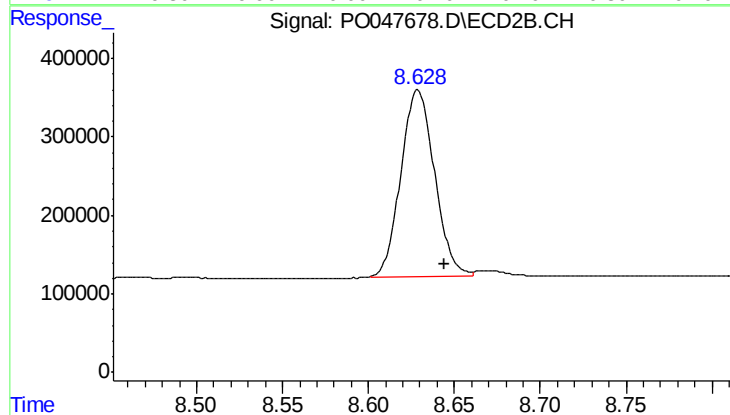

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.016 min
Response: 3247981
Conc: 20.66 ng/ml