

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
 Data File : P0047684.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Aug 2018 5:49
 Operator : SM/SJ
 Sample : J4318-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BEEBEE-SITE-DEMO-2A

Manual Integrations
 APPROVED

Sohil
 8/6/2018 2:25:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 13:37:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.644	5567359	5794340	27.575	23.581
2) SA Decachlor...	10.090	8.630	3554619	3351159	21.794	21.319

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080318\
Data File : P0047684.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2018 5:49
Operator : SM/SJ
Sample : J4318-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BEEBEE-SITE-DEMO-2A


Manual Integrations
APPROVED

Sohil
8/6/2018 2:25:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:37:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

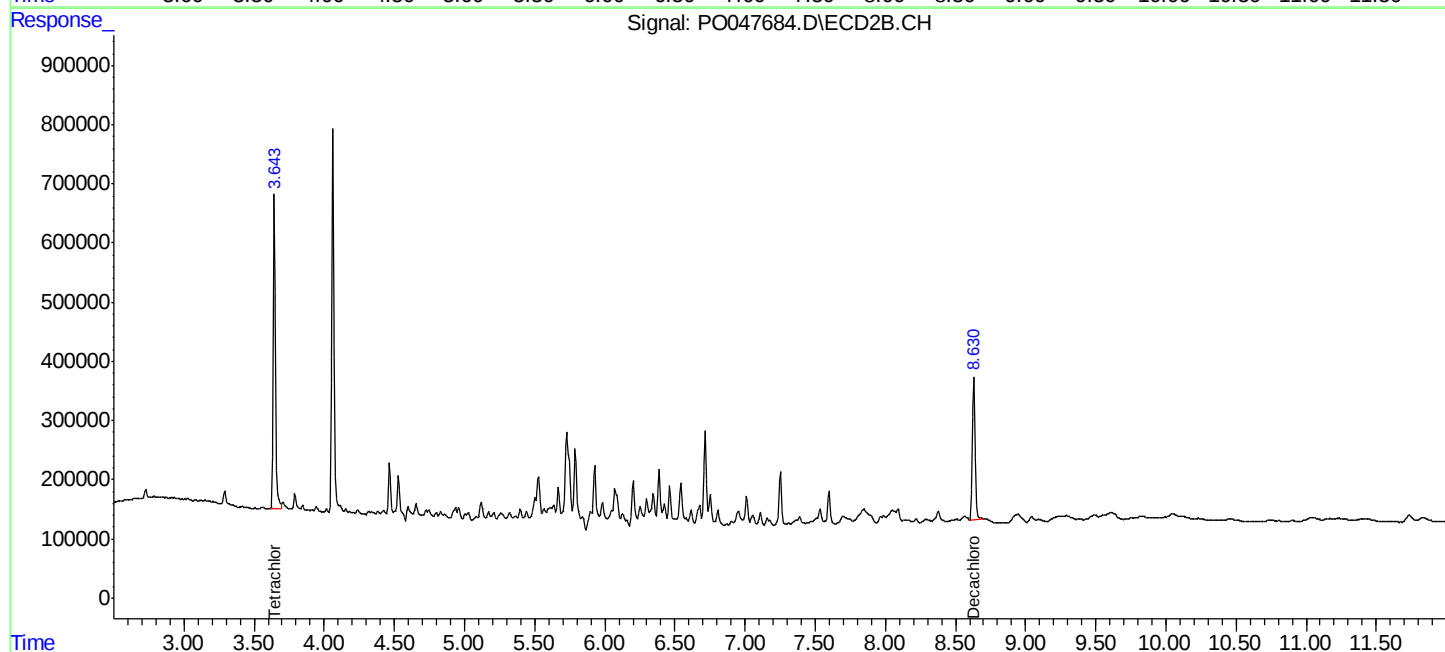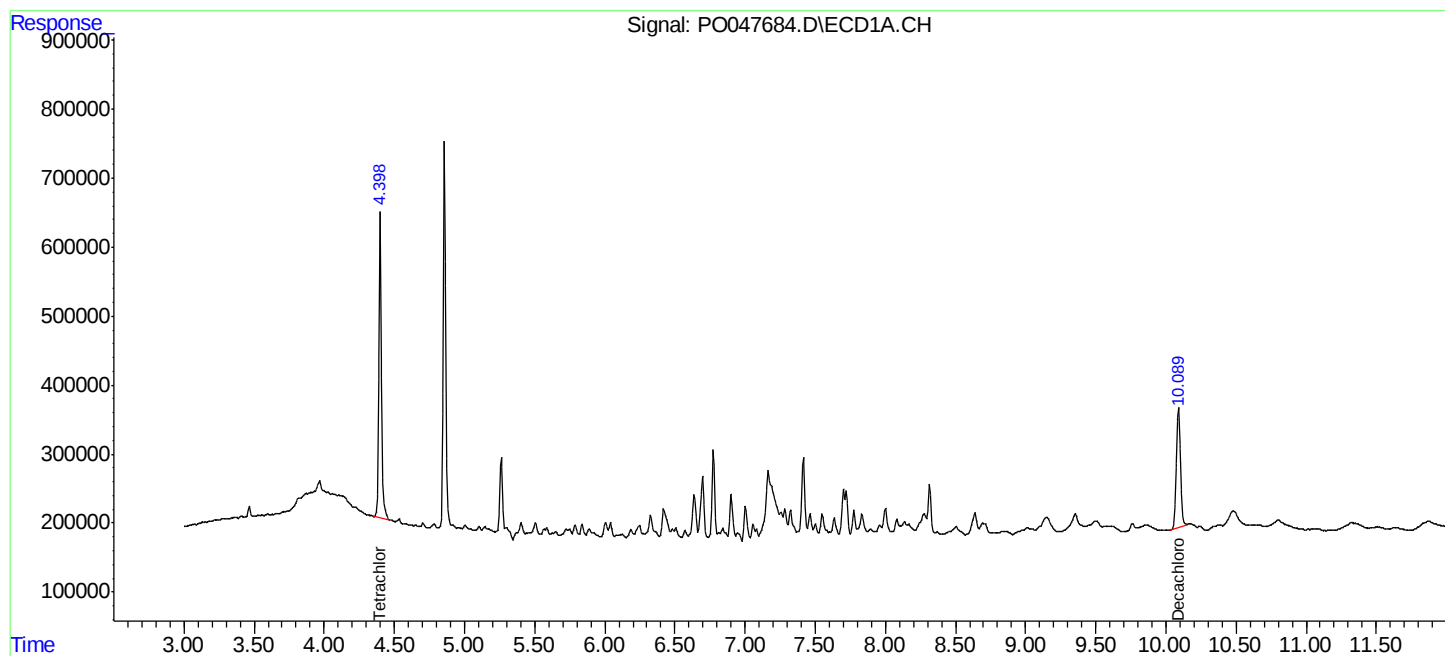

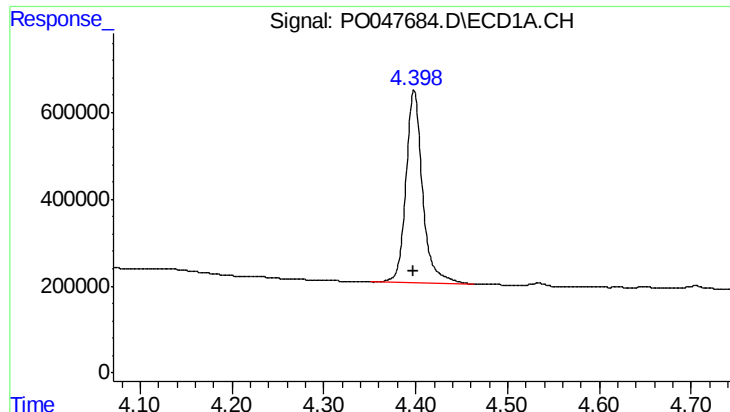


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 5567359
Conc: 27.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
BEEBEE-SITE-DEMO-2A


Manual Integrations
APPROVED

Sohil
8/6/2018 2:25:07 PM

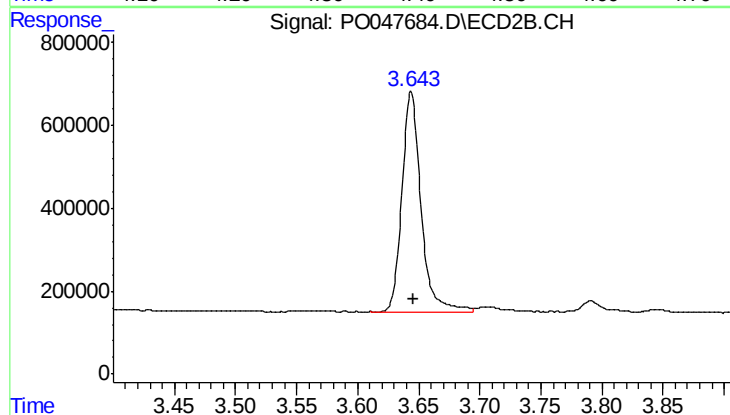


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.001 min
Response: 5794340
Conc: 23.58 ng/ml

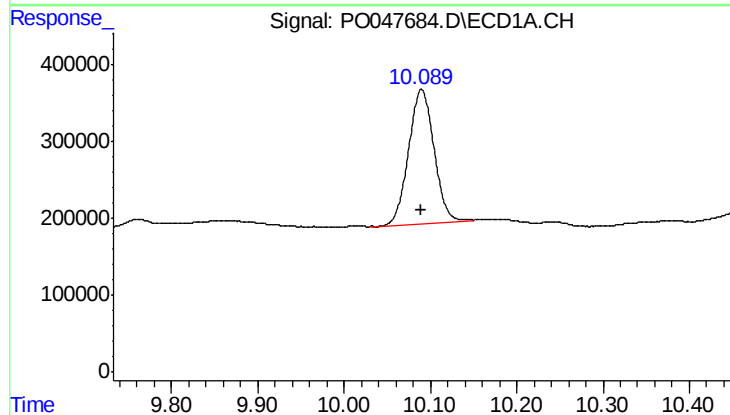

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 3554619
Conc: 21.79 ng/ml

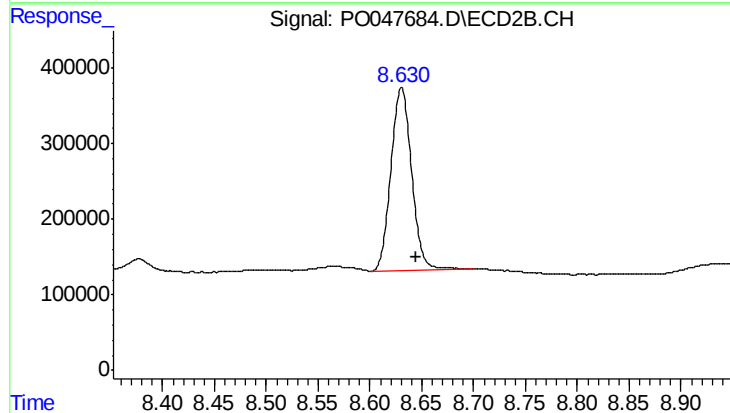

#2 Decachlorobiphenyl

R.T.: 8.630 min
Delta R.T.: -0.014 min
Response: 3351159
Conc: 21.32 ng/ml