

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080319\
 Data File : P0058814.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Aug 2019 16:48
 Operator : SM/AJ
 Sample : K4133-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DEWATERING-SCREEN-1-080119

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 17:25:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.162	3.516	721781	602838	17.103	15.090
2)	SA Decachlor...	9.636	8.400	778566	580691	14.376	14.711

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080319\
Data File : PO058814.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2019 16:48
Operator : SM/AJ
Sample : K4133-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DEWATERING-SCREEN-1-080119

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 17:25:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

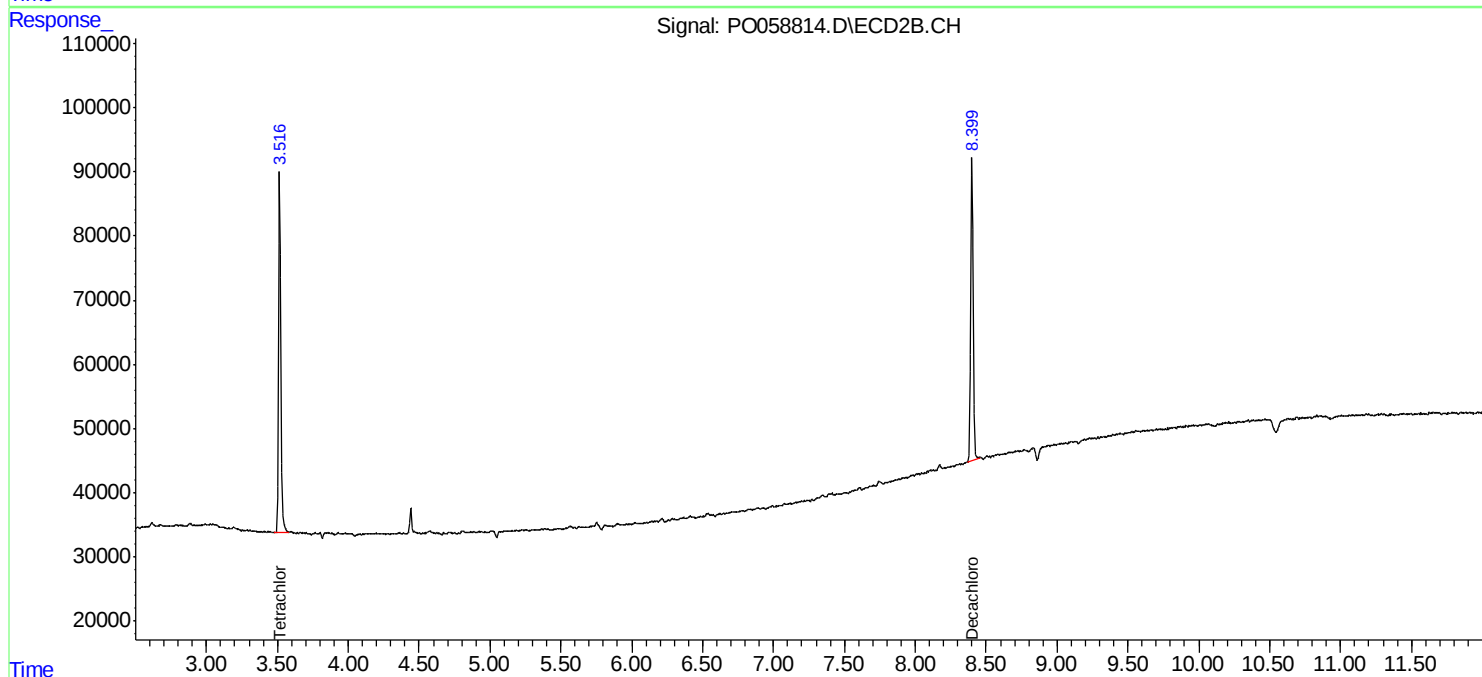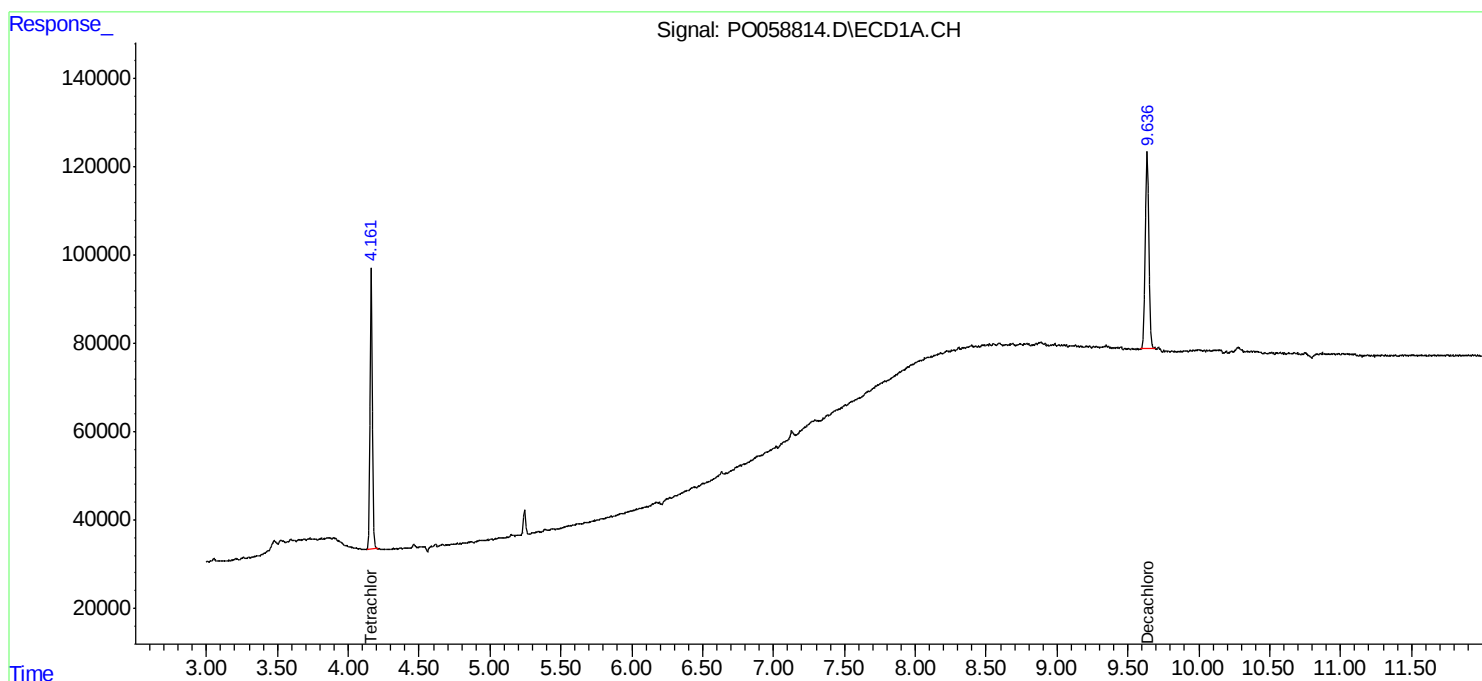


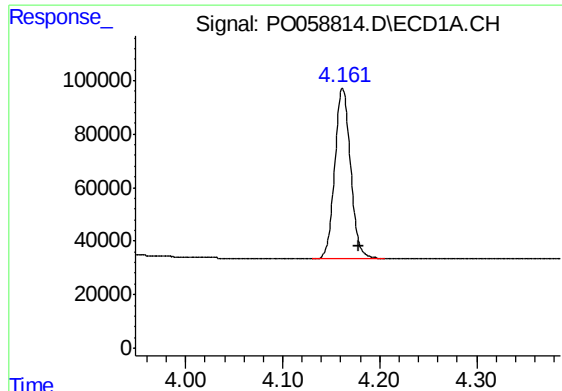

#1 Tetrachloro-m-xylene


R.T.: 4.162 min
Delta R.T.: -0.017 min
Response: 721781
Conc: 17.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
DEWATERING-SCREEN-1-080119

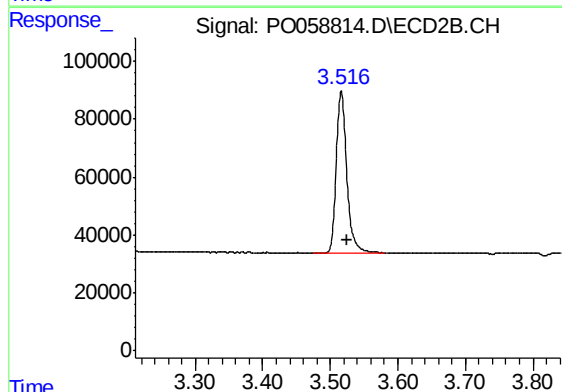


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.008 min
Response: 602838
Conc: 15.09 ng/ml

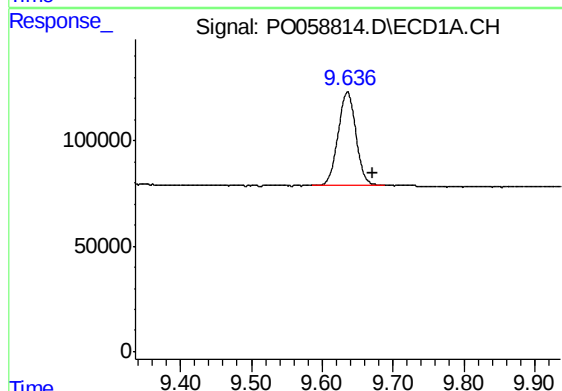

#2 Decachlorobiphenyl

R.T.: 9.636 min
Delta R.T.: -0.037 min
Response: 778566
Conc: 14.38 ng/ml

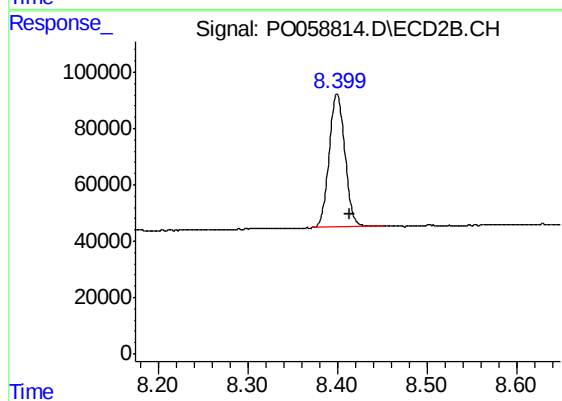

#2 Decachlorobiphenyl

R.T.: 8.400 min
Delta R.T.: -0.014 min
Response: 580691
Conc: 14.71 ng/ml