

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080319\
 Data File : P0058831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Aug 2019 21:57
 Operator : SM/AJ
 Sample : K4130-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1S-F1-F4-COMP-(30)

Manual Integrations
 APPROVED

Ankita
 8/5/2019 11:14:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 01:23:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.161	3.517	926120	810526	21.945	20.288
2) SA Decachlor...	9.634	8.399	857139	637164	15.827m	16.142m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080319\
Data File : PO058831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2019 21:57
Operator : SM/AJ
Sample : K4130-06
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1S-F1-F4-COMP-(30)


Manual Integrations
APPROVED

Ankita
8/5/2019 11:14:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 01:23:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

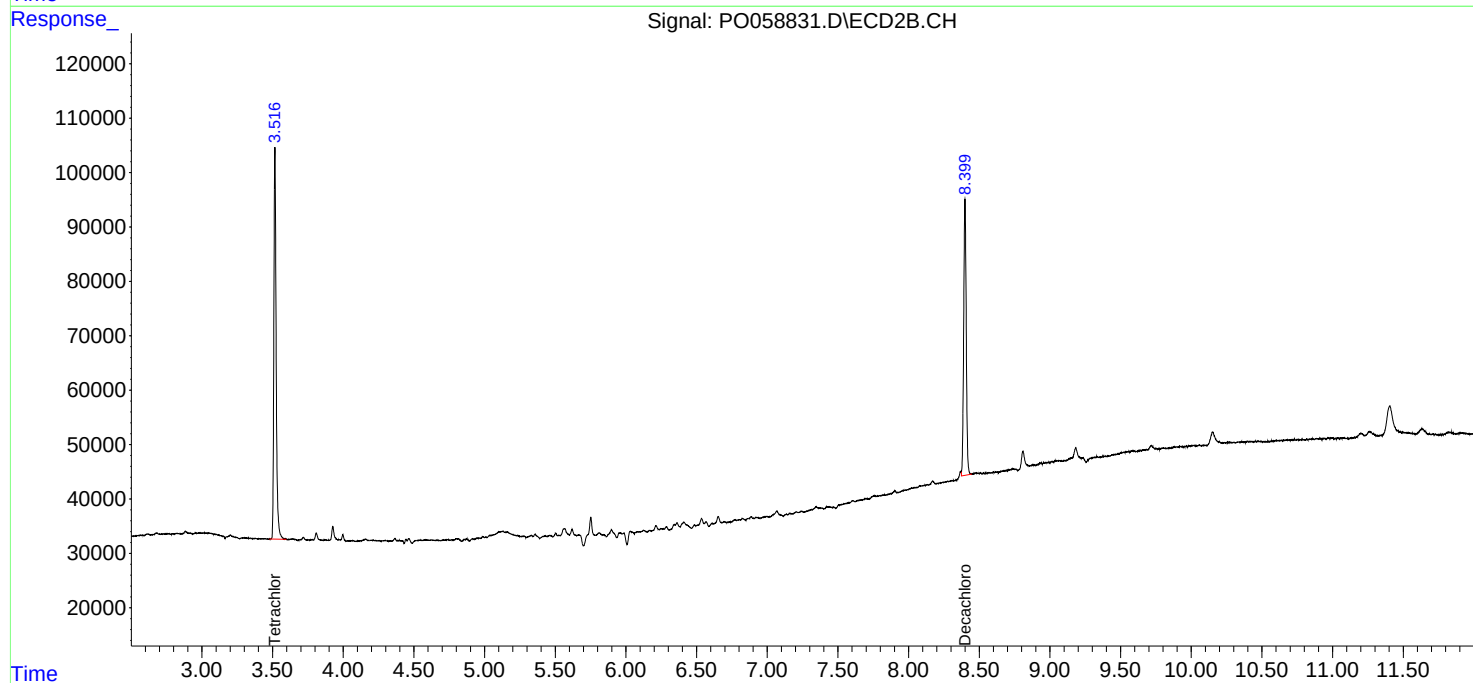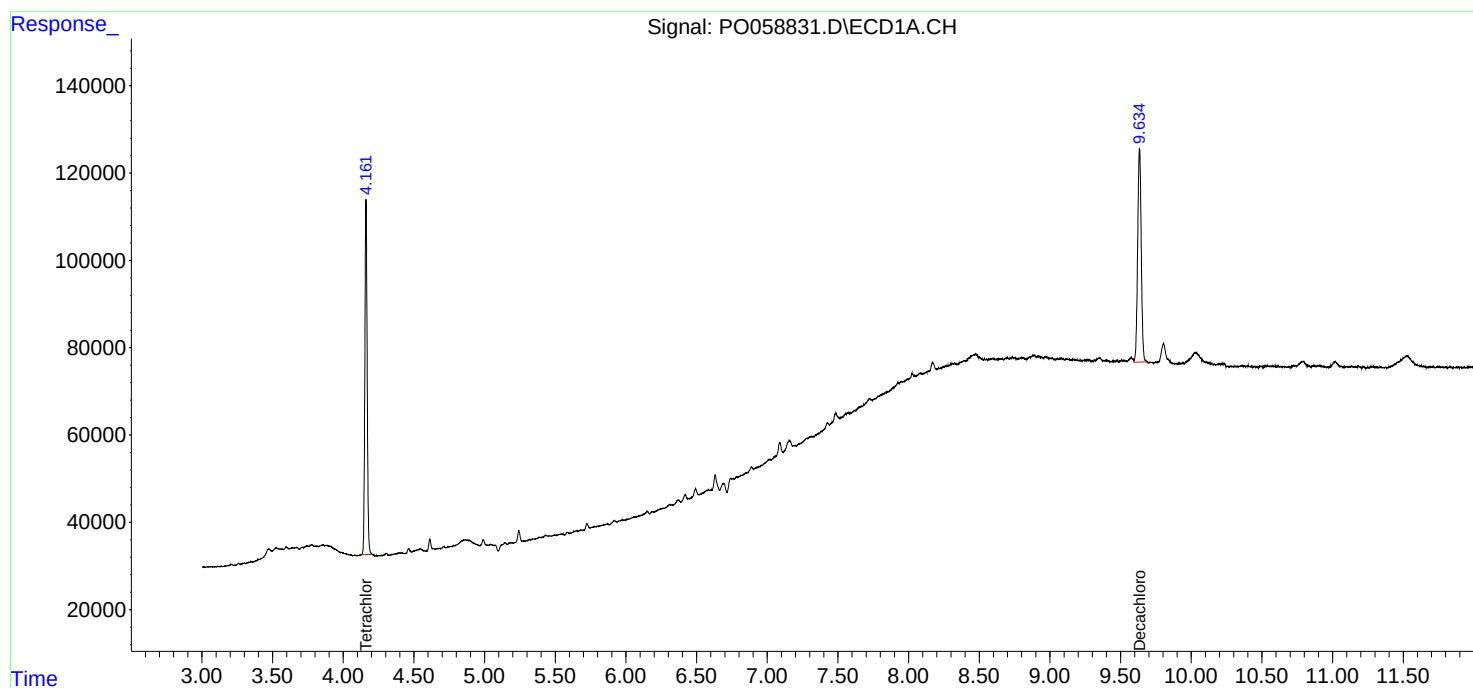

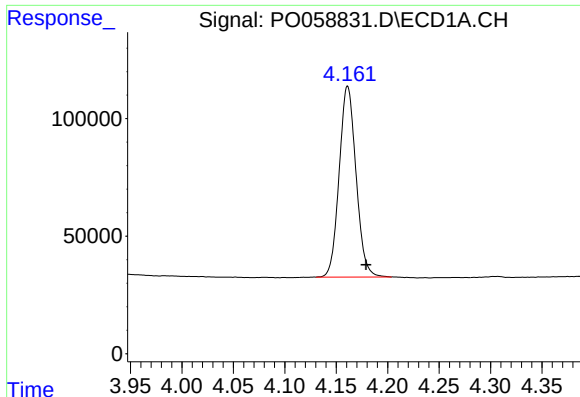


#1 Tetrachloro-m-xylene

R.T.: 4.161 min
Delta R.T.: -0.018 min
Response: 926120
Conc: 21.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
1S-F1-F4-COMP-(30)


Manual Integrations
APPROVED

Ankita
8/5/2019 11:14:33 AM

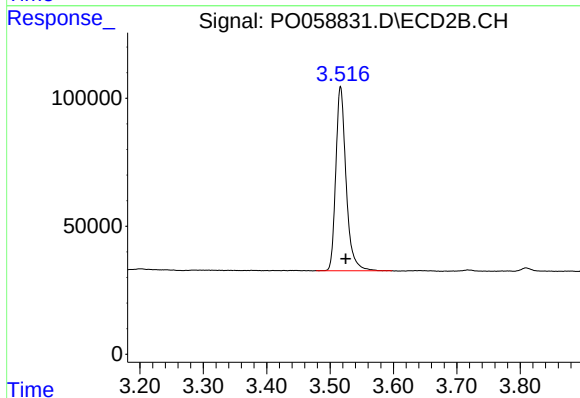


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.008 min
Response: 810526
Conc: 20.29 ng/ml

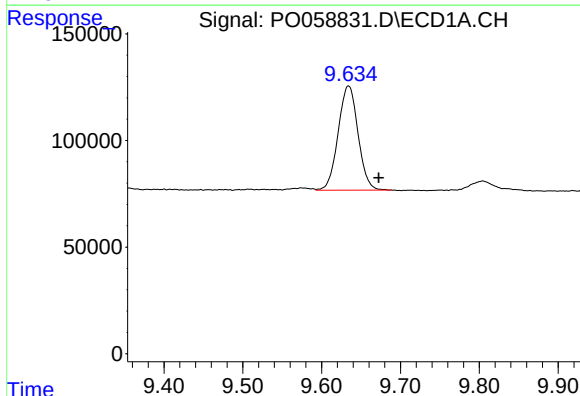

#2 Decachlorobiphenyl

R.T.: 9.634 min
Delta R.T.: -0.039 min
Response: 857139
Conc: 15.83 ng/ml m

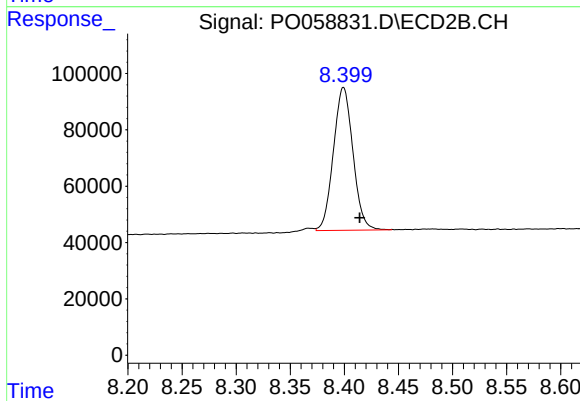

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.015 min
Response: 637164
Conc: 16.14 ng/ml m