

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080319\
 Data File : P0058837.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Aug 2019 23:40
 Operator : SM/AJ
 Sample : K4131-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1S-D1-D4-COMP-(30)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:02:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.162	3.517	817658	720246	19.374	18.029
2) SA Decachlor...	9.679	8.400	716471	557419	13.230	14.122

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080319\
Data File : PO058837.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2019 23:40
Operator : SM/AJ
Sample : K4131-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1S-D1-D4-COMP-(30)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:02:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

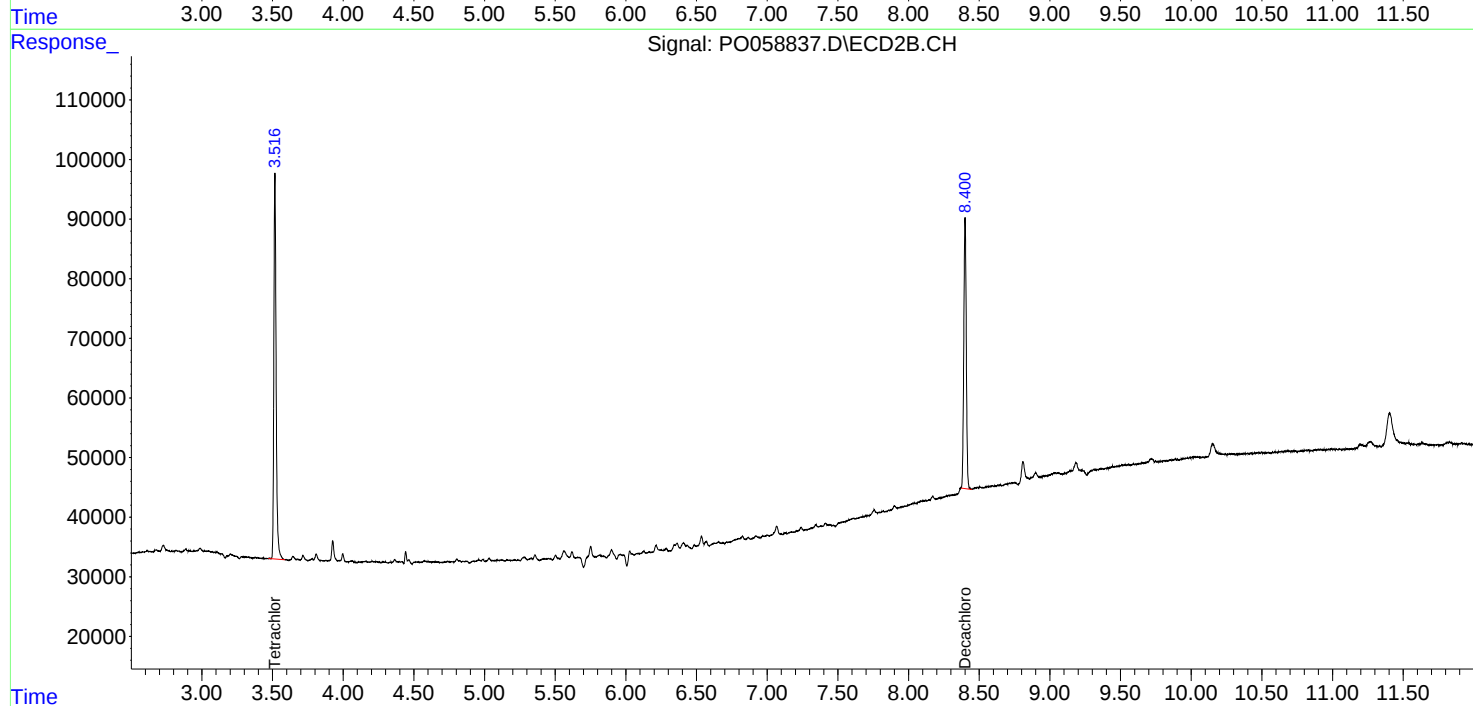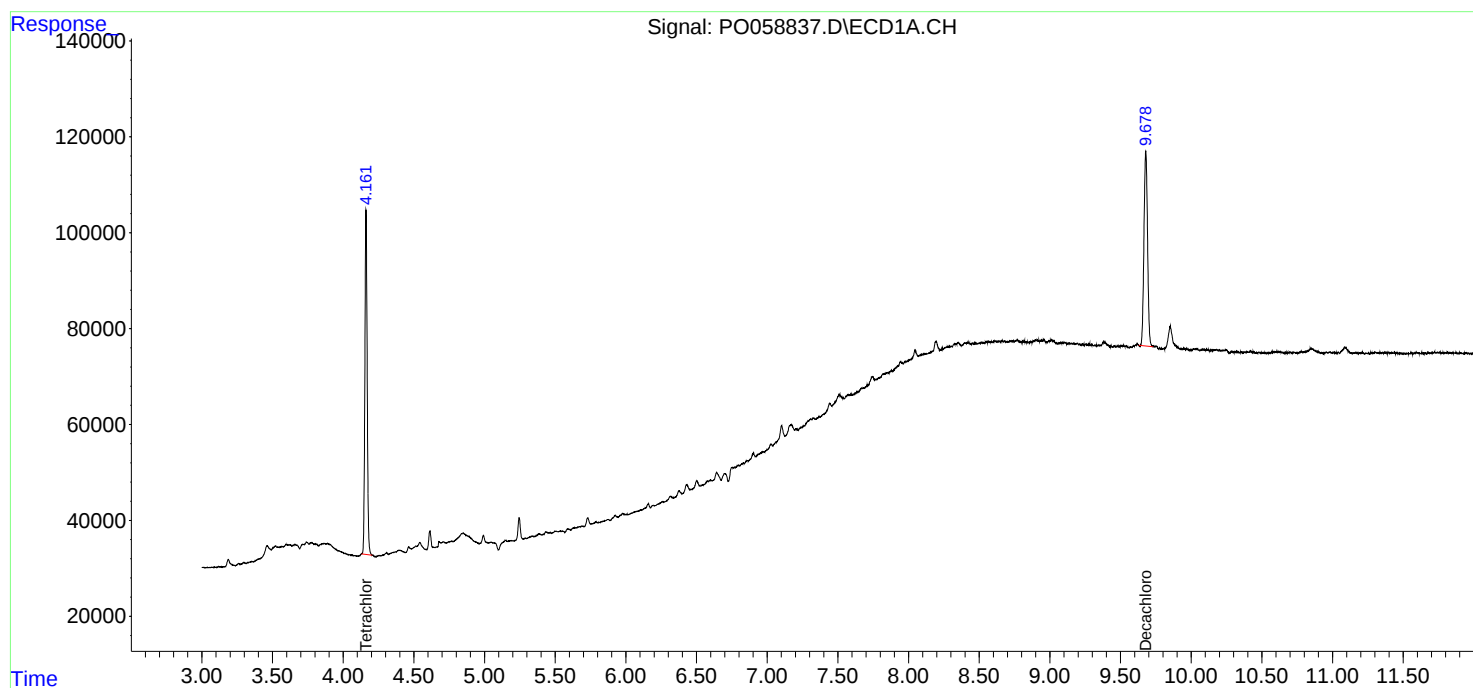


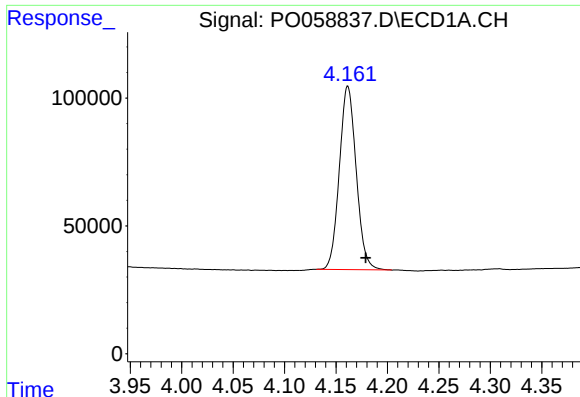

#1 Tetrachloro-m-xylene


R.T.: 4.162 min
Delta R.T.: -0.017 min
Response: 817658
Conc: 19.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
1S-D1-D4-COMP-(30)

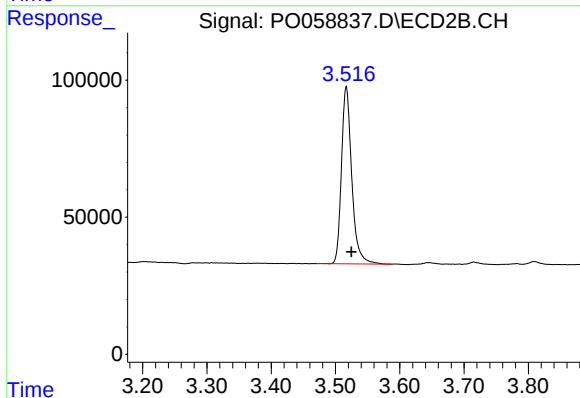


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.008 min
Response: 720246
Conc: 18.03 ng/ml

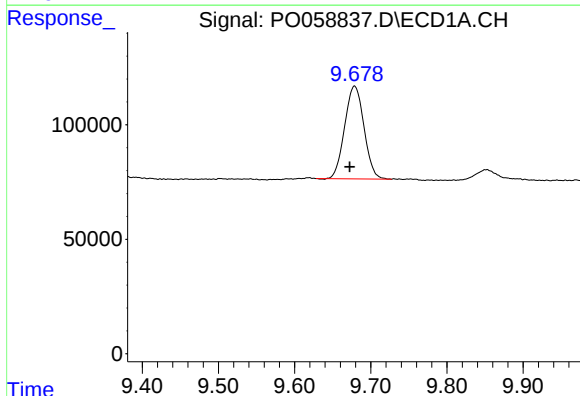

#2 Decachlorobiphenyl

R.T.: 9.679 min
Delta R.T.: 0.006 min
Response: 716471
Conc: 13.23 ng/ml

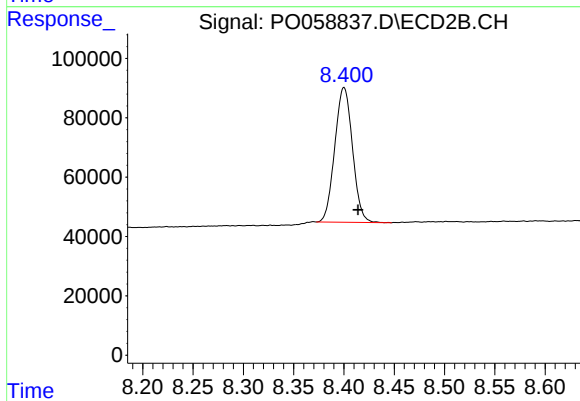

#2 Decachlorobiphenyl

R.T.: 8.400 min
Delta R.T.: -0.014 min
Response: 557419
Conc: 14.12 ng/ml