

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
 Data File : P0070279.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2020 17:36
 Operator : DD\AJ
 Sample : L3521-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-CD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 05:13:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.560	1163009	1103023	25.197	26.398
2) SA Decachlor...	10.007	8.754	1327622	1179541	20.533	19.048
Target Compounds						
9) L2 AR-1221-2	4.719	0.000	17110	0	43.380	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
Data File : P0070279.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2020 17:36
Operator : DD\AJ
Sample : L3521-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-CD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 05:13:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

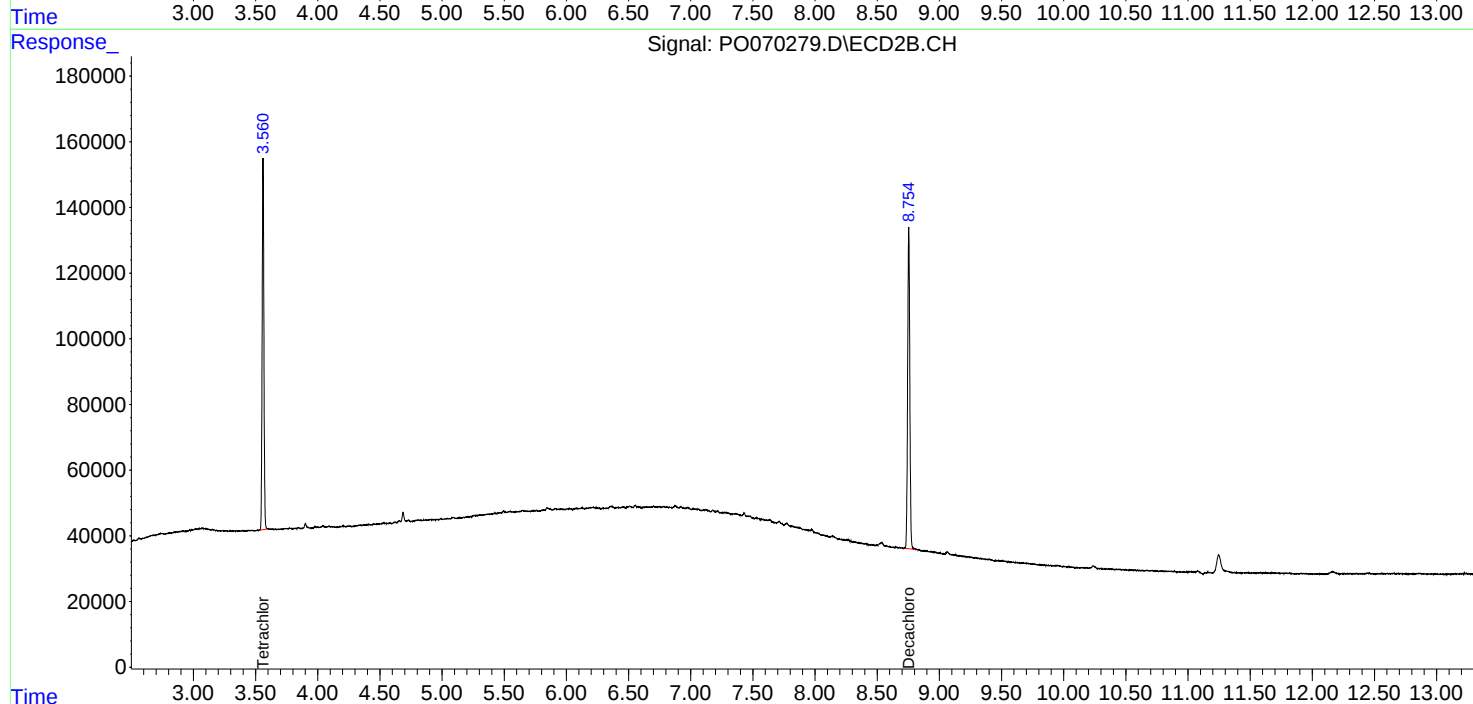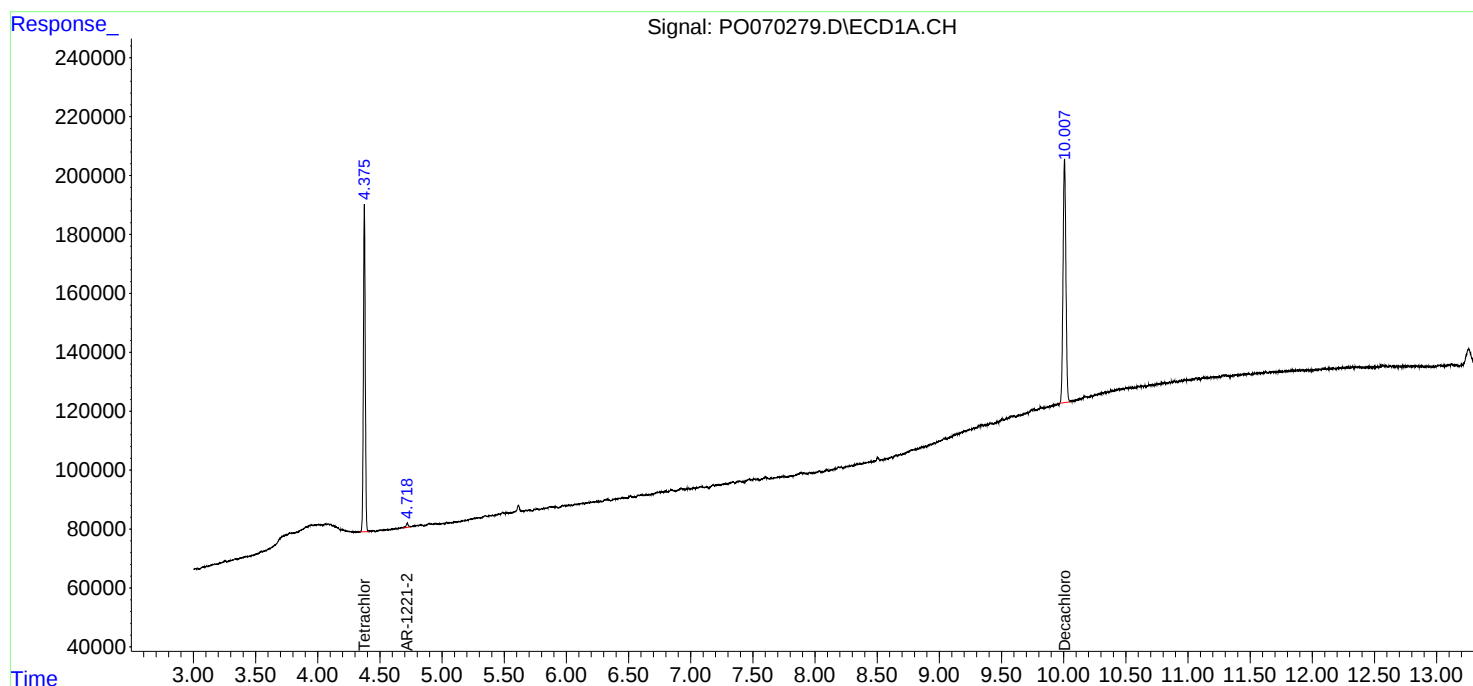


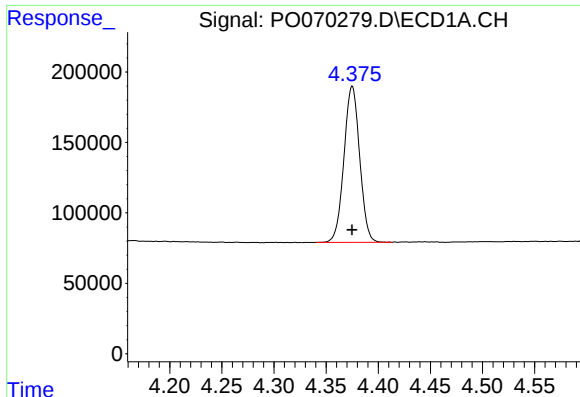

#1 Tetrachloro-m-xylene


R.T.: 4.375 min
Delta R.T.: 0.000 min
Response: 1163009
Conc: 25.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-CD

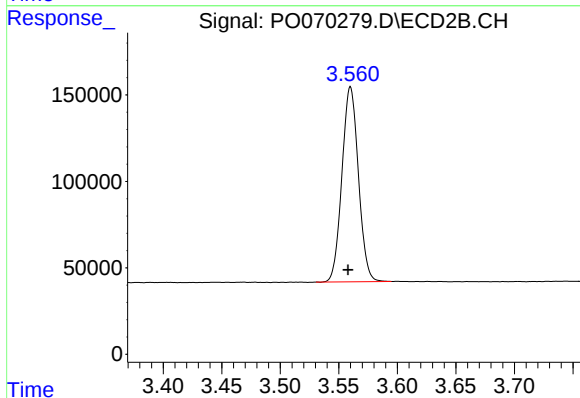


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.002 min
Response: 1103023
Conc: 26.40 ng/ml

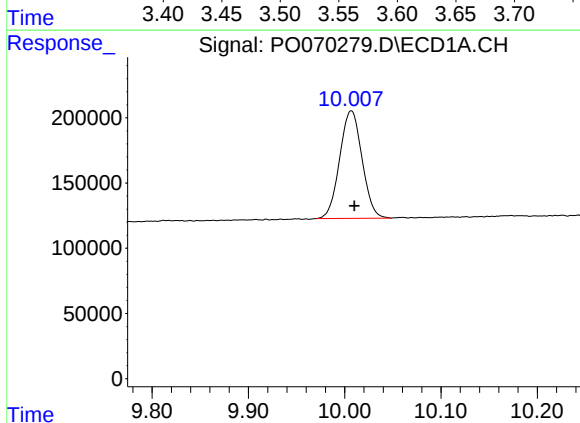


#2 Decachlorobiphenyl

R.T.: 10.007 min
Delta R.T.: -0.003 min
Response: 1327622
Conc: 20.53 ng/ml

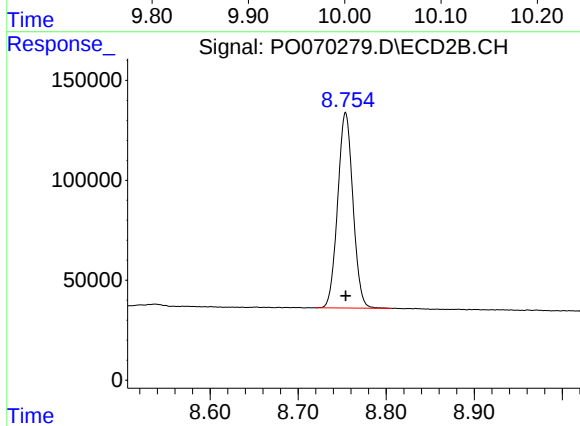

#2 Decachlorobiphenyl


R.T.: 8.754 min
Delta R.T.: 0.000 min
Response: 1179541
Conc: 19.05 ng/ml

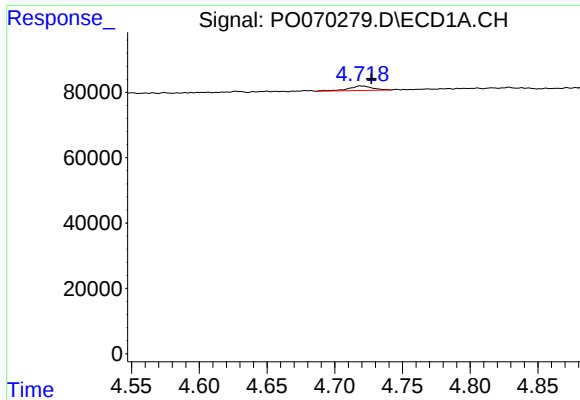

#9 AR-1221-2

R.T.: 4.719 min
Delta R.T.: -0.008 min
Response: 17110
Conc: 43.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-CD

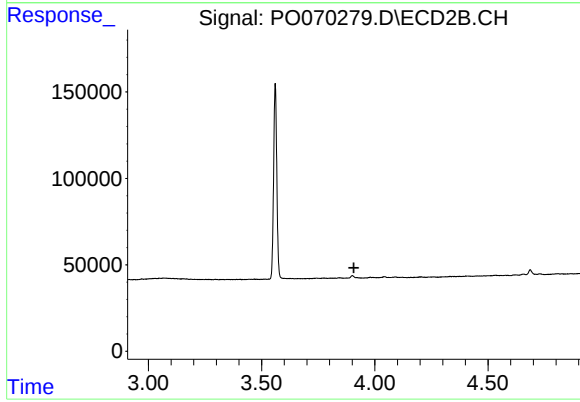

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.