

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
 Data File : P0070268.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2020 14:28
 Operator : DD\AJ
 Sample : L3512-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 USED-ANTIFREEZE-1456

Manual Integrations
 APPROVED

Ankita
 8/5/2020 8:49:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 17:17:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.376	3.561	816212	1103519	17.684m	26.409 #
2) SA Decachlor...	10.005	8.754	695140	798231	10.751m	12.890

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
Data File : P0070268.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2020 14:28
Operator : DD\AJ
Sample : L3512-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
USED-ANTIFREEZE-1456


Manual Integrations
APPROVED

Ankita
8/5/2020 8:49:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 17:17:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

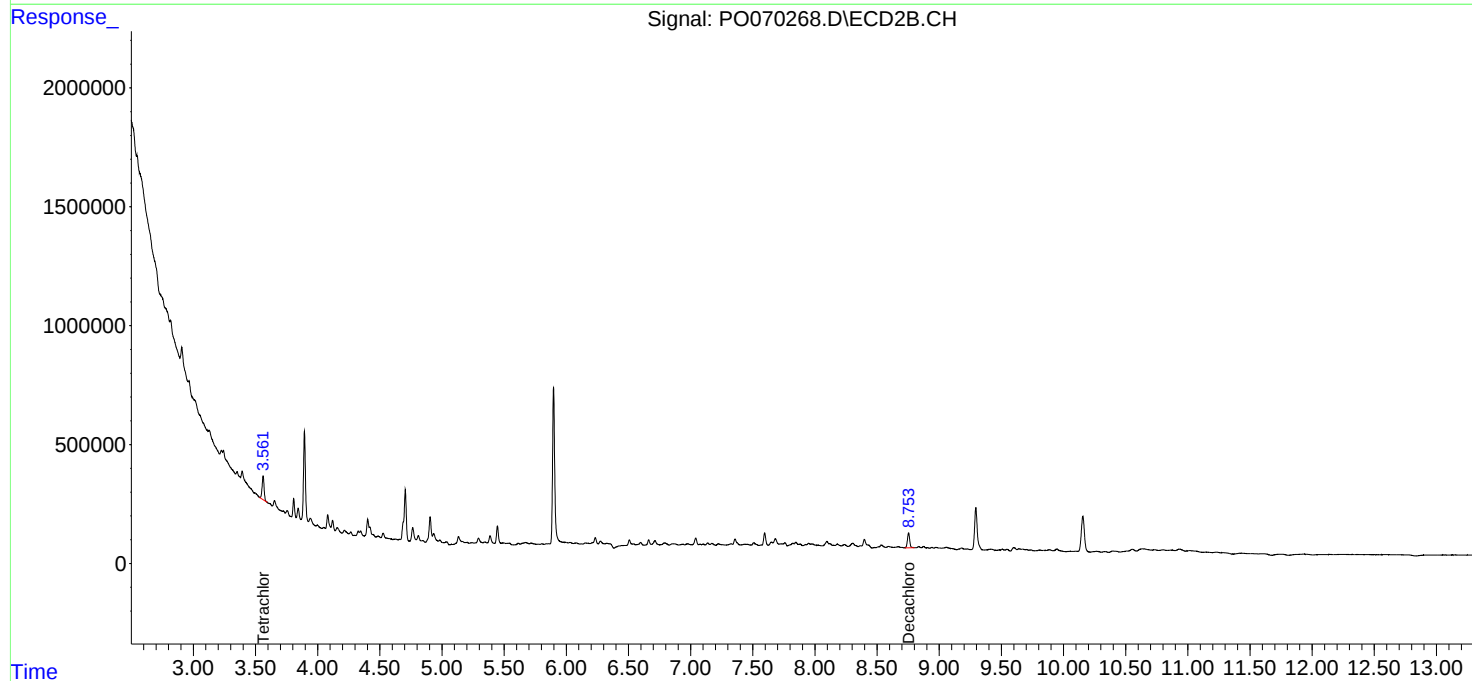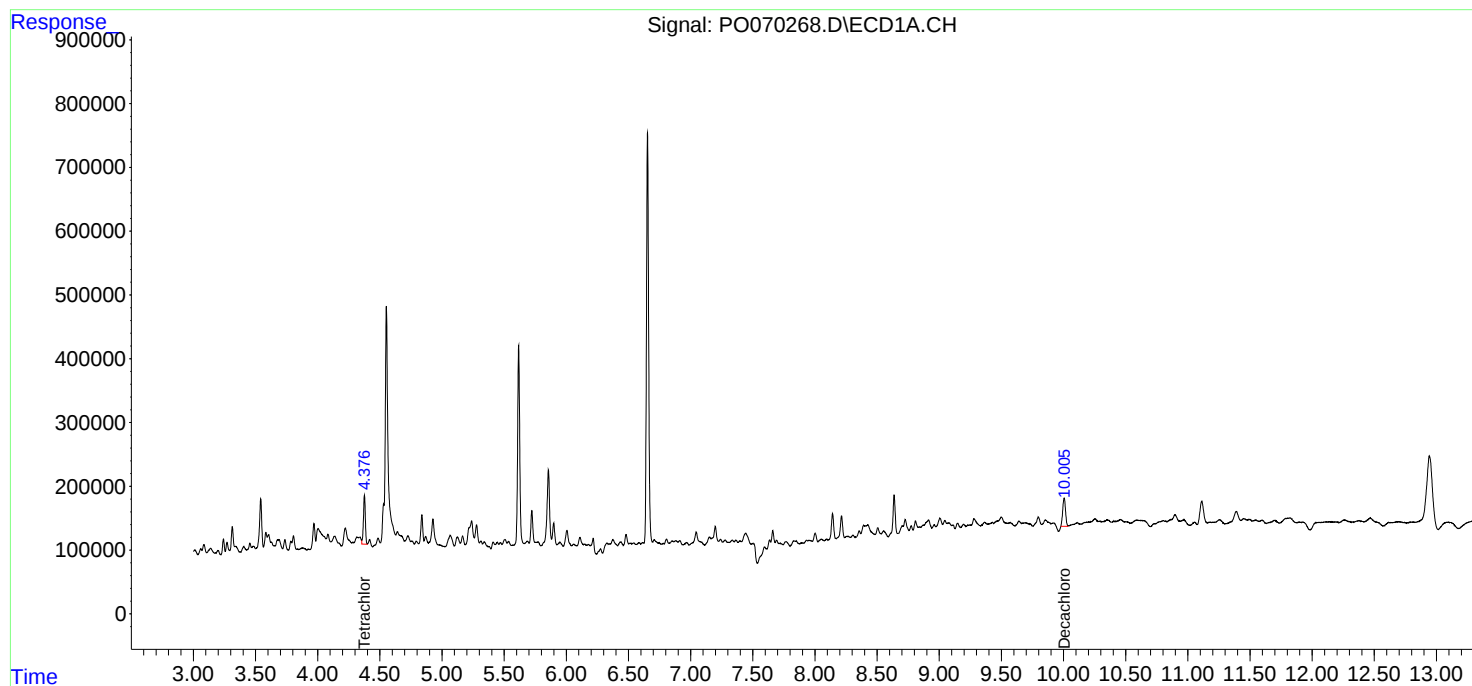

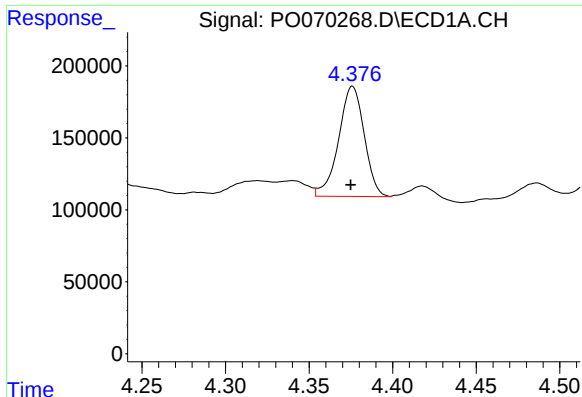


#1 Tetrachloro-m-xylene

R.T.: 4.376 min
Delta R.T.: 0.000 min
Response: 816212
Conc: 17.68 ng/ml m

Instrument :
ECD_O
ClientSampleId :
USED-ANTIFREEZE-1456


Manual Integrations
APPROVED

Ankita
8/5/2020 8:49:14 AM

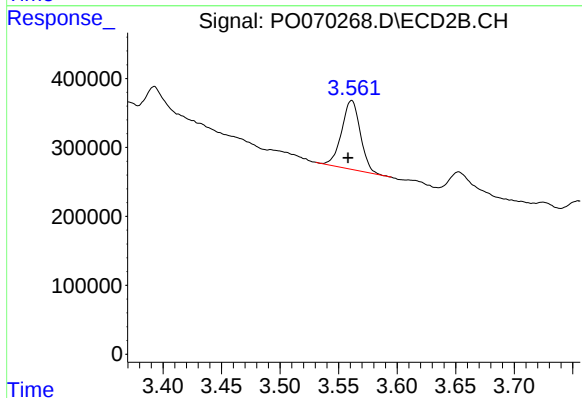


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.003 min
Response: 1103519
Conc: 26.41 ng/ml

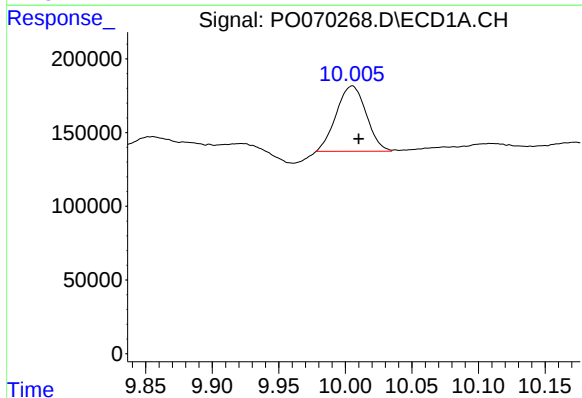

#2 Decachlorobiphenyl

R.T.: 10.005 min
Delta R.T.: -0.005 min
Response: 695140
Conc: 10.75 ng/ml m

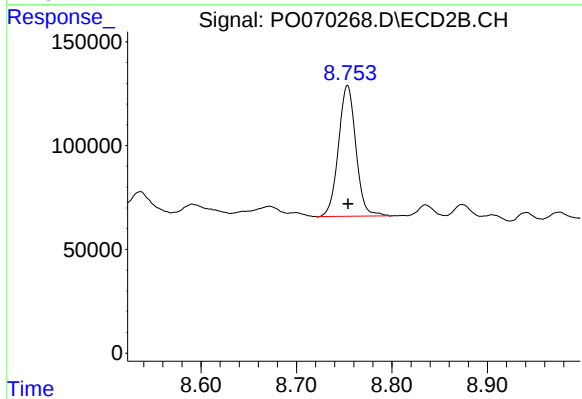

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: 0.000 min
Response: 798231
Conc: 12.89 ng/ml