

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
 Data File : P0070270.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2020 15:02
 Operator : DD\AJ
 Sample : L3512-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER-1493

Manual Integrations
 APPROVED

Ankita
 8/5/2020 8:49:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 17:17:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.560	381265	442995	8.260m	10.602 #
2) SA Decachlor...	10.005	8.751	179269	176593	2.773	2.852m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
Data File : P0070270.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2020 15:02
Operator : DD\AJ
Sample : L3512-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER-1493


Manual Integrations
APPROVED

Ankita
8/5/2020 8:49:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 17:17:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

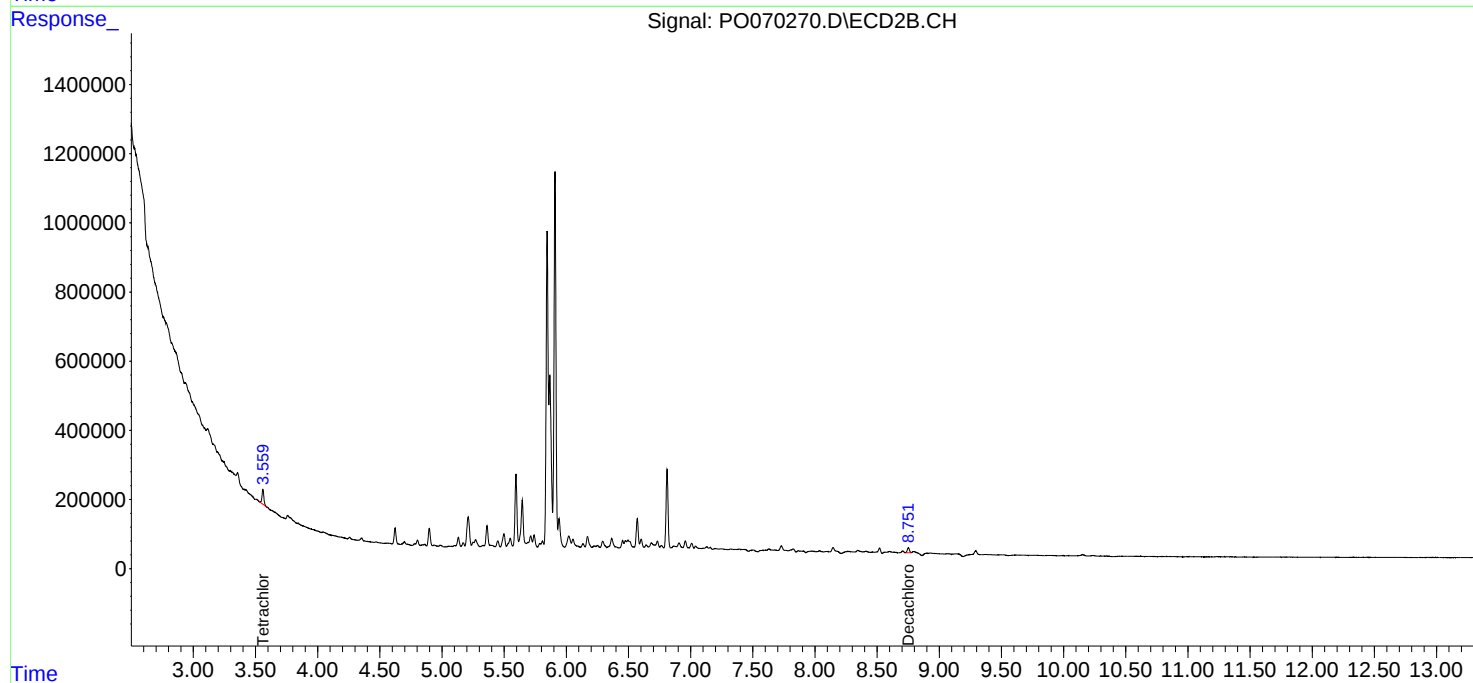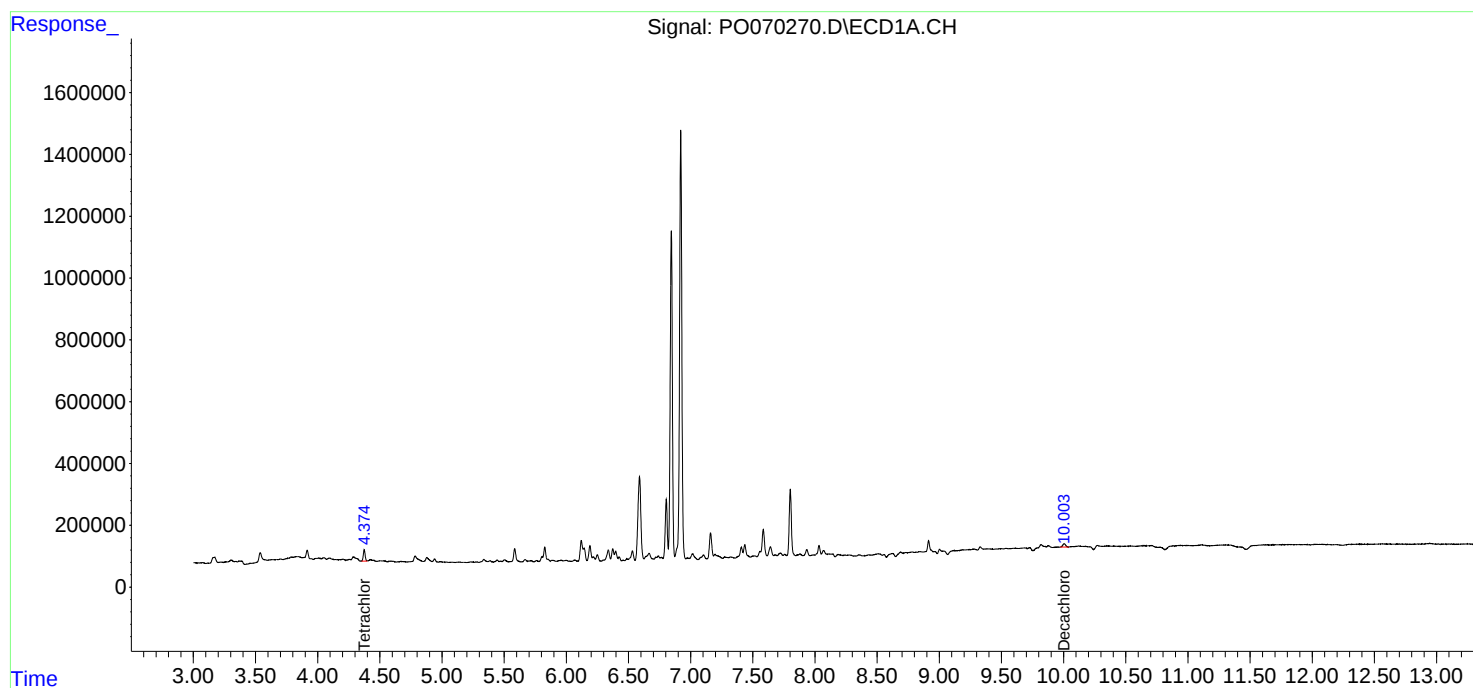

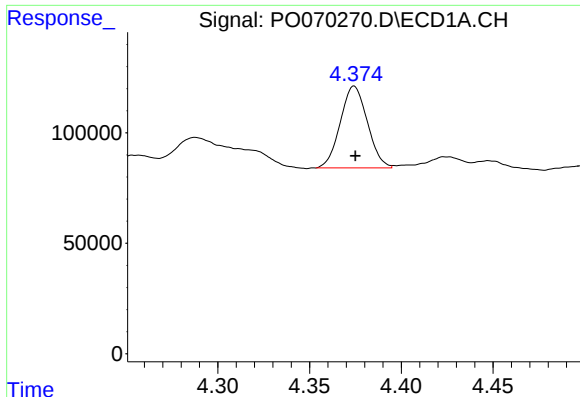


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: -0.001 min
Response: 381265
Conc: 8.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OILY-WATER-1493


Manual Integrations
APPROVED

Ankita
8/5/2020 8:49:17 AM

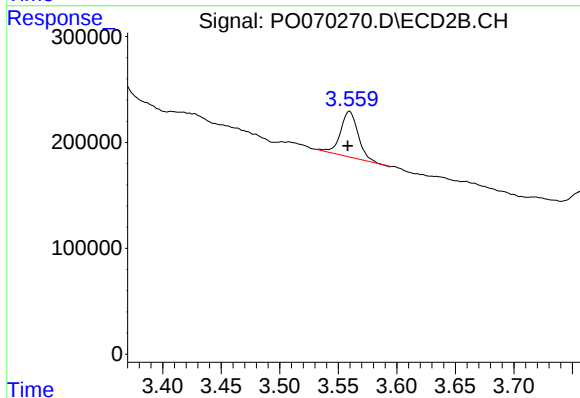


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.002 min
Response: 442995
Conc: 10.60 ng/ml

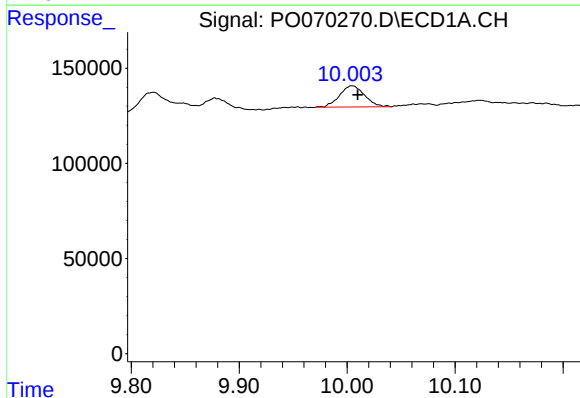

#2 Decachlorobiphenyl

R.T.: 10.005 min
Delta R.T.: -0.005 min
Response: 179269
Conc: 2.77 ng/ml

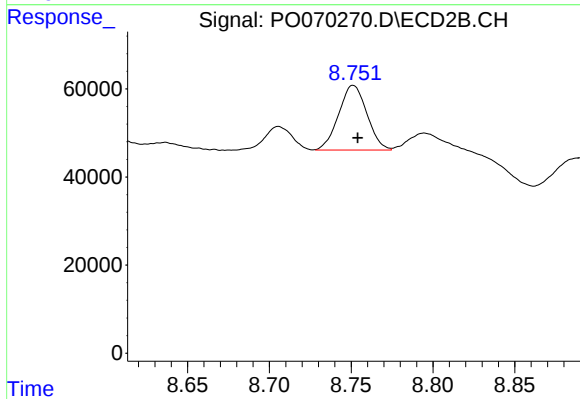

#2 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.003 min
Response: 176593
Conc: 2.85 ng/ml m