

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
Data File : P0070283.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2020 18:44
Operator : DD\AJ
Sample : L3525-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TILCON-FL-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 05:14:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.558	915556	875314	19.836	20.948
2) SA Decachlor...	10.007	8.754	1292269	1152532	19.987	18.612

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080320\
Data File : P0070283.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2020 18:44
Operator : DD\AJ
Sample : L3525-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TILCON-FL-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 05:14:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

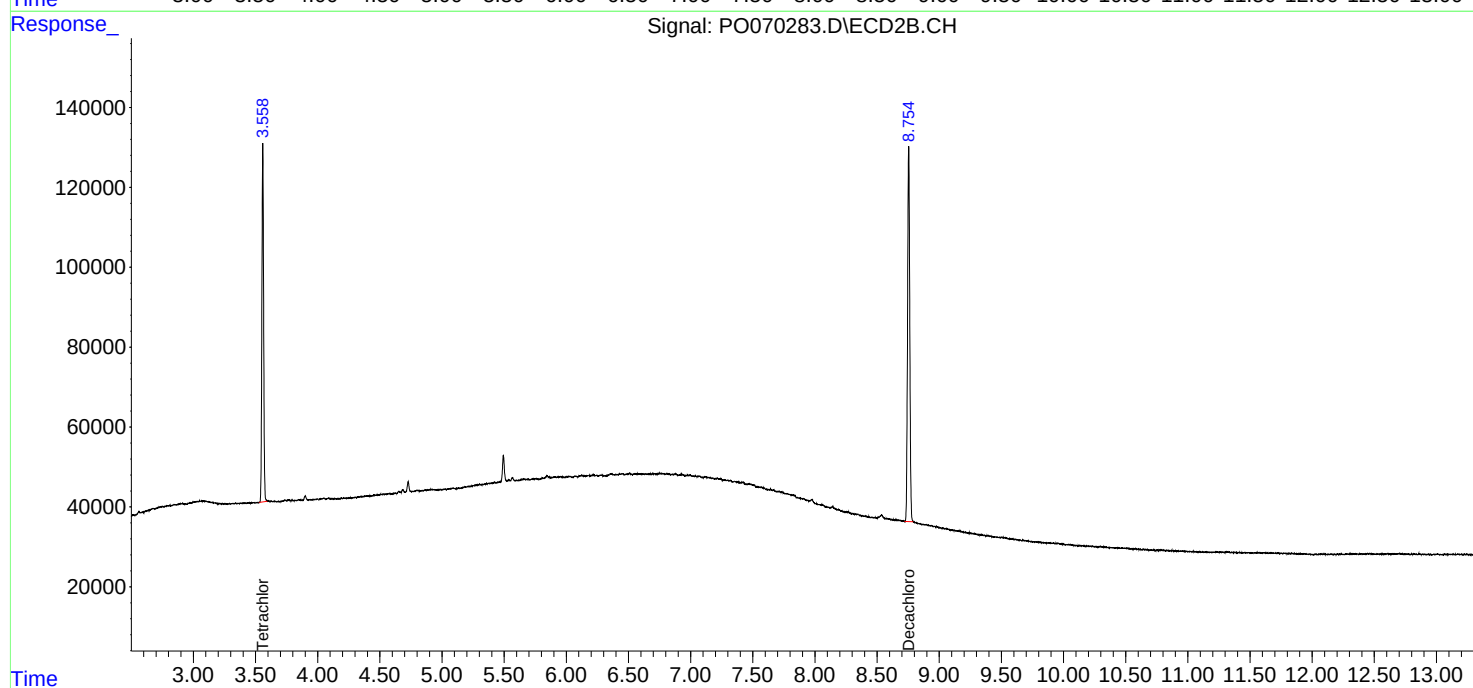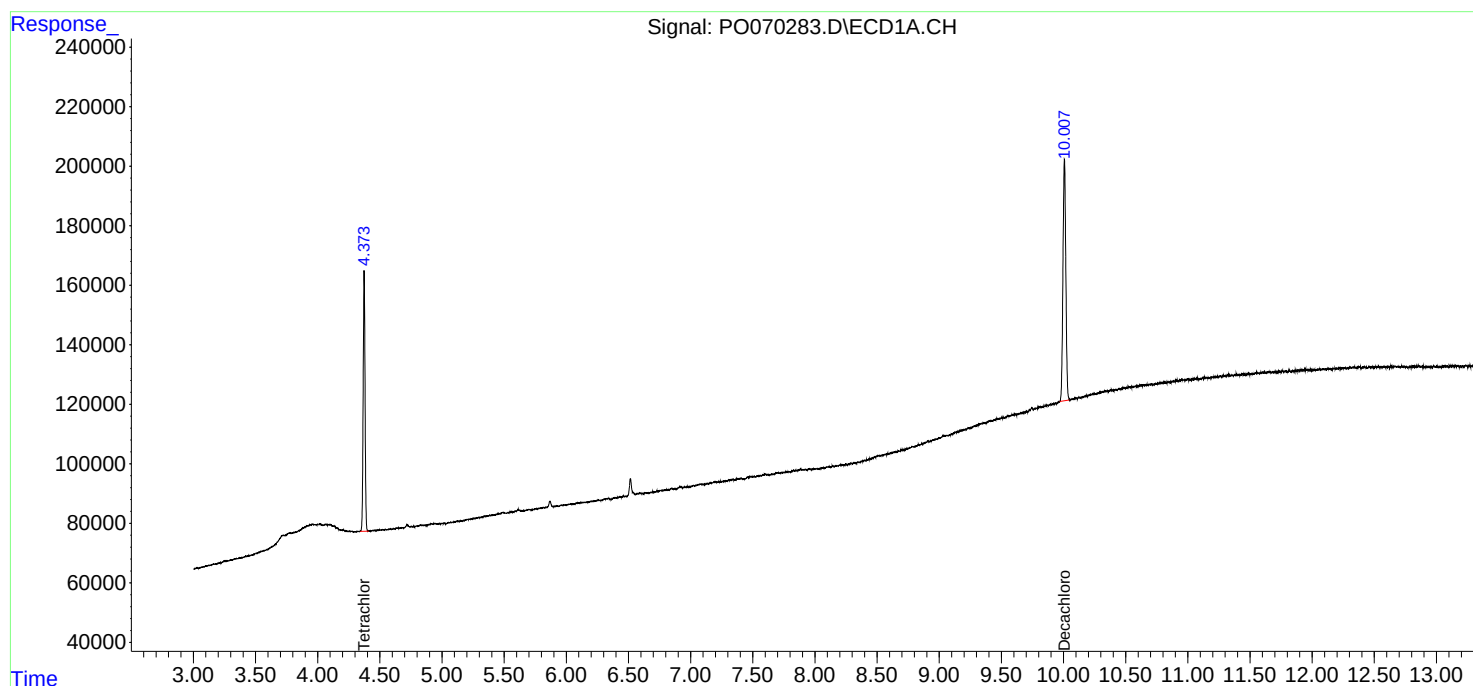


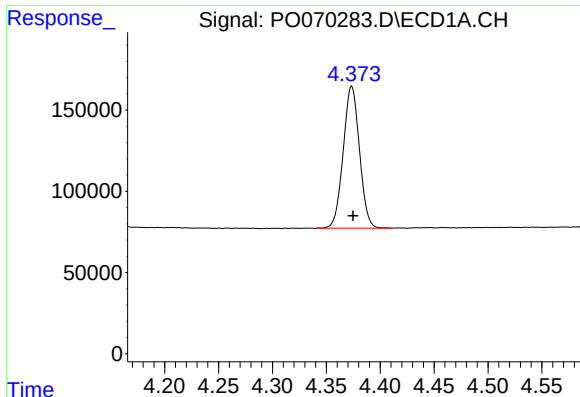

#1 Tetrachloro-m-xylene


R.T.: 4.374 min
Delta R.T.: -0.001 min
Response: 915556
Conc: 19.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
TILCON-FL-002

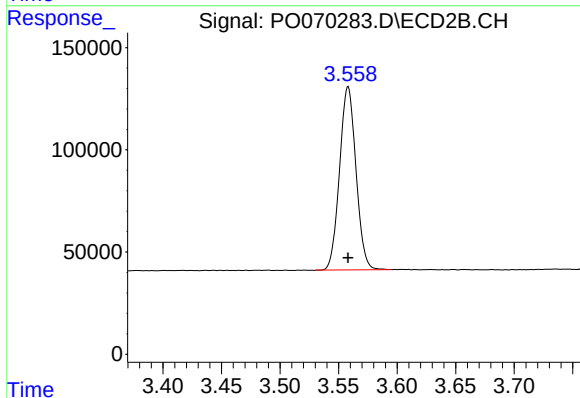


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: 0.000 min
Response: 875314
Conc: 20.95 ng/ml

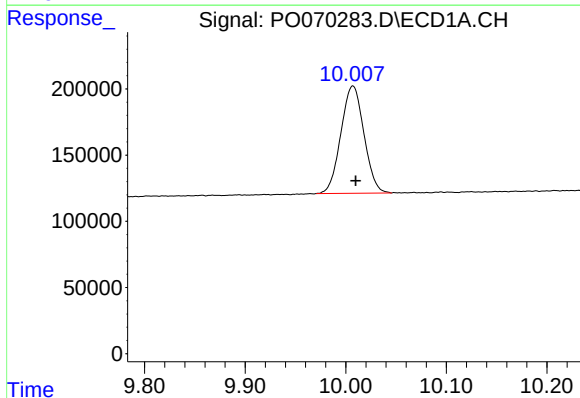

#2 Decachlorobiphenyl

R.T.: 10.007 min
Delta R.T.: -0.003 min
Response: 1292269
Conc: 19.99 ng/ml

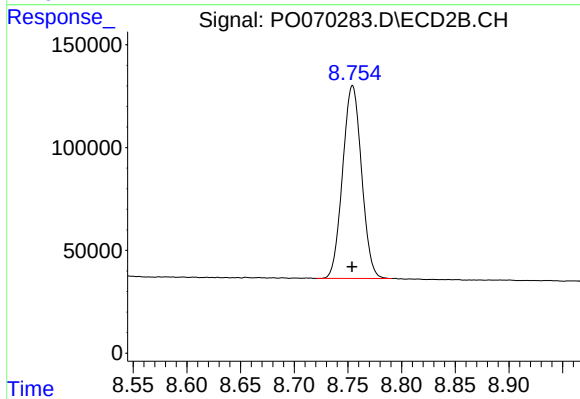

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: 0.000 min
Response: 1152532
Conc: 18.61 ng/ml