

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080321\
 Data File : P0080122.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2021 18:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 03:22:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.001	4.118	1491257	547836	24.748	23.922
2)	SA Decachlor...	11.110	9.527	1050588	487414	22.396	23.454
Target Compounds							
28)	L6 AR-1254-3	7.877f	0.000	24167	0	7.019	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080122\
Data File : P0080122.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2021 18:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 03:22:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

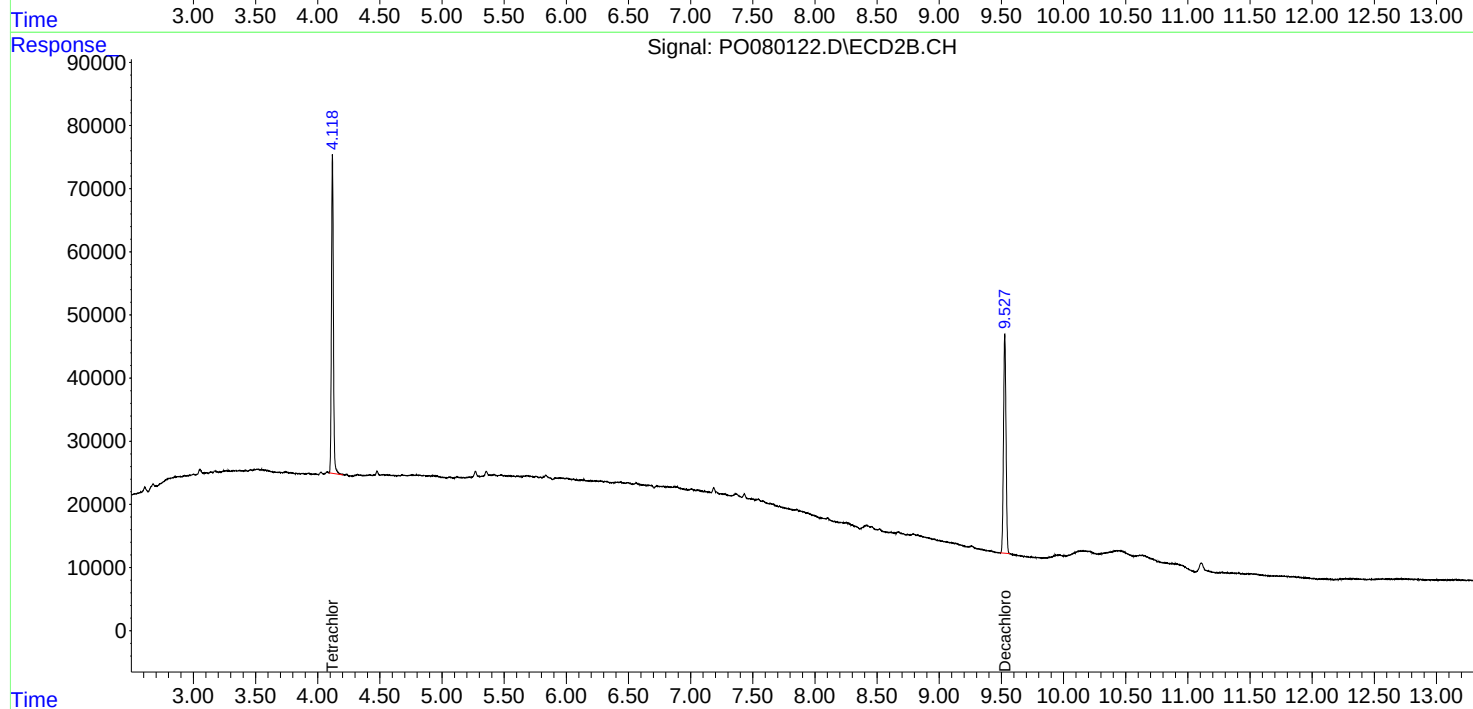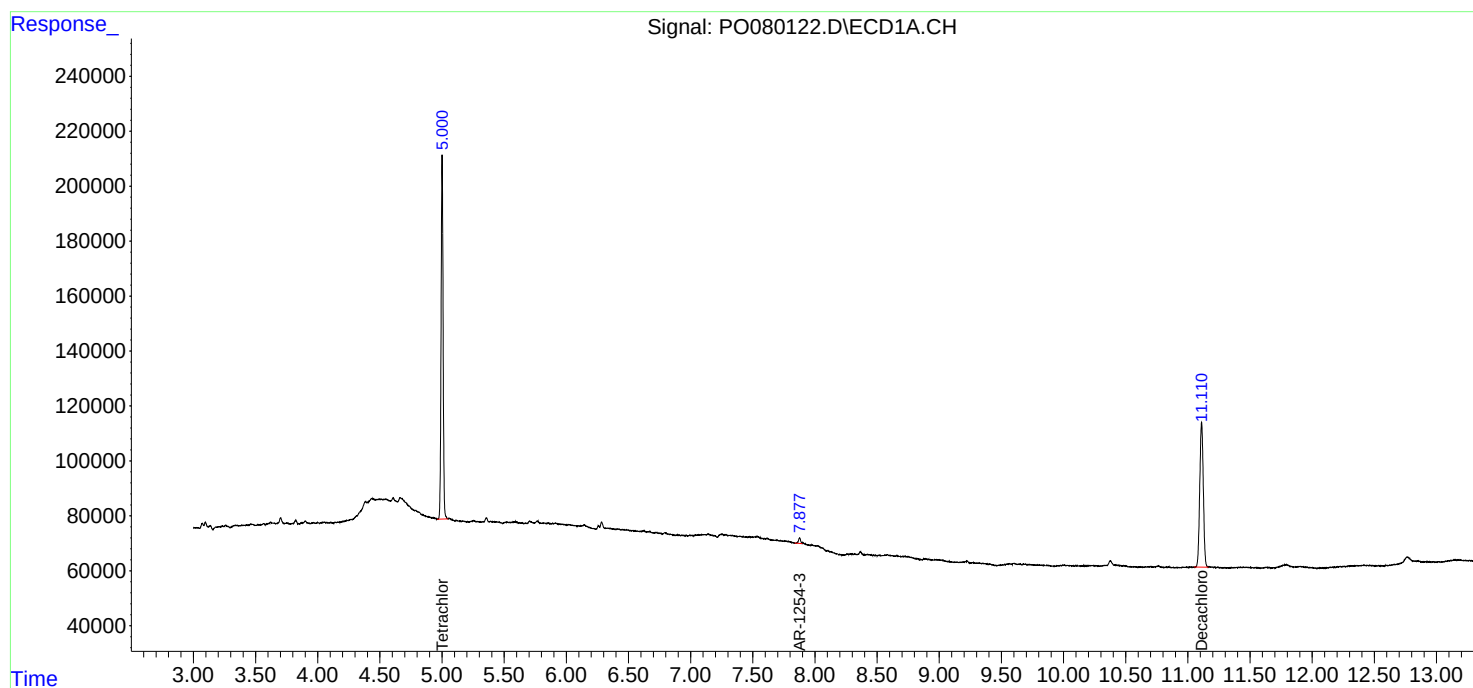


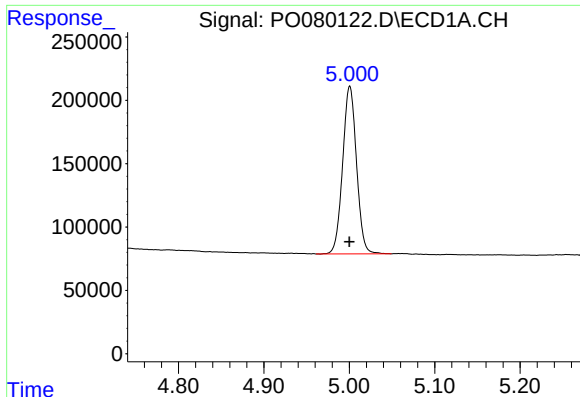

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: 0.000 min
Response: 1491257
Conc: 24.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

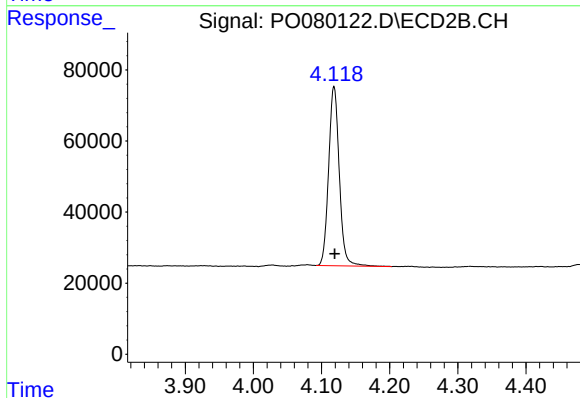


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: 0.000 min
Response: 547836
Conc: 23.92 ng/ml

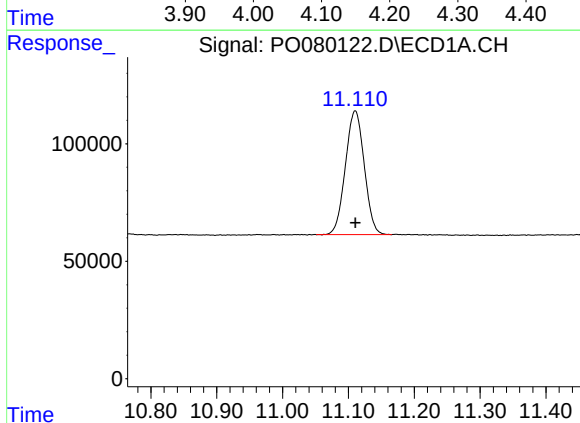


#2 Decachlorobiphenyl

R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 1050588
Conc: 22.40 ng/ml

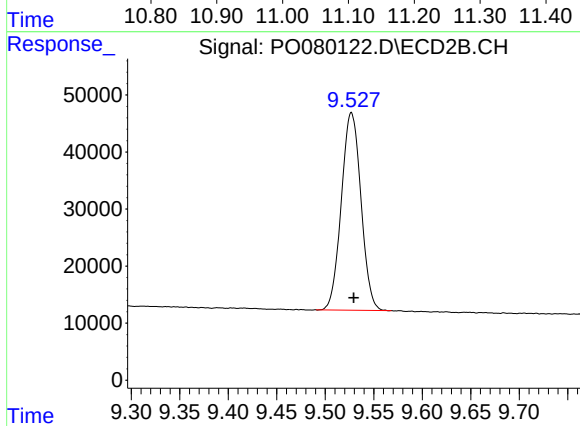

#2 Decachlorobiphenyl


R.T.: 9.527 min
Delta R.T.: -0.002 min
Response: 487414
Conc: 23.45 ng/ml

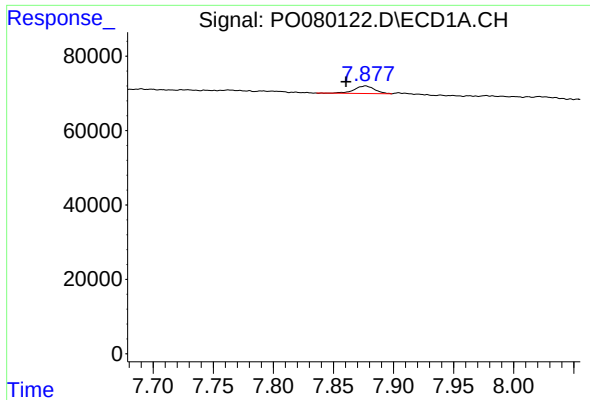

#28 AR-1254-3

R.T.: 7.877 min
Delta R.T.: 0.016 min
Response: 24167
Conc: 7.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

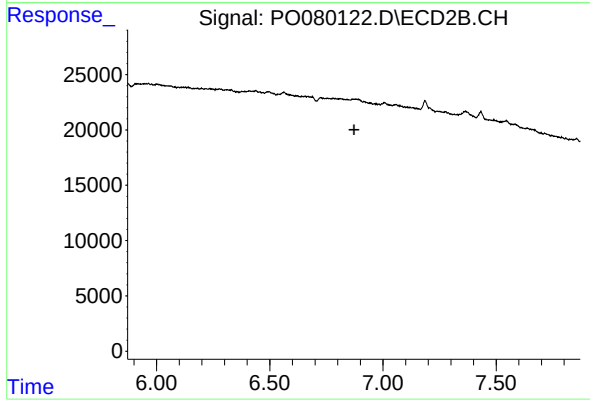

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.872 min
Response: 0
Conc: N.D.