

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080321\
 Data File : P0080123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Aug 2021 18:39
 Operator : DD\AJ
 Sample : M3247-21 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF3176(2-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 03:22:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.001	4.118	71963	34974	1.194m	1.527 #
2) SA Decachlor...	11.110	9.527	87171	40498	1.858m	1.949

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P00801231\
Data File : P0080123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Aug 2021 18:39
Operator : DD\AJ
Sample : M3247-21 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEF3176(2-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 03:22:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

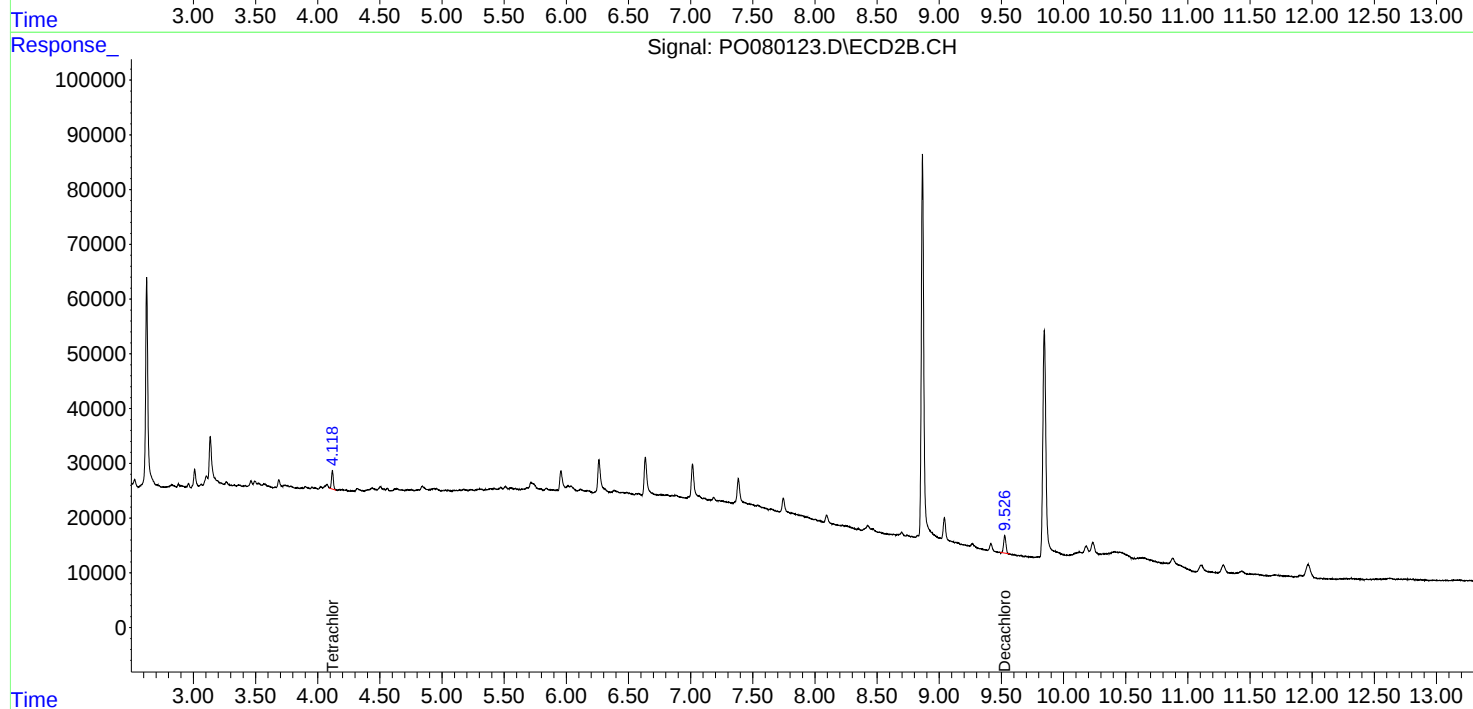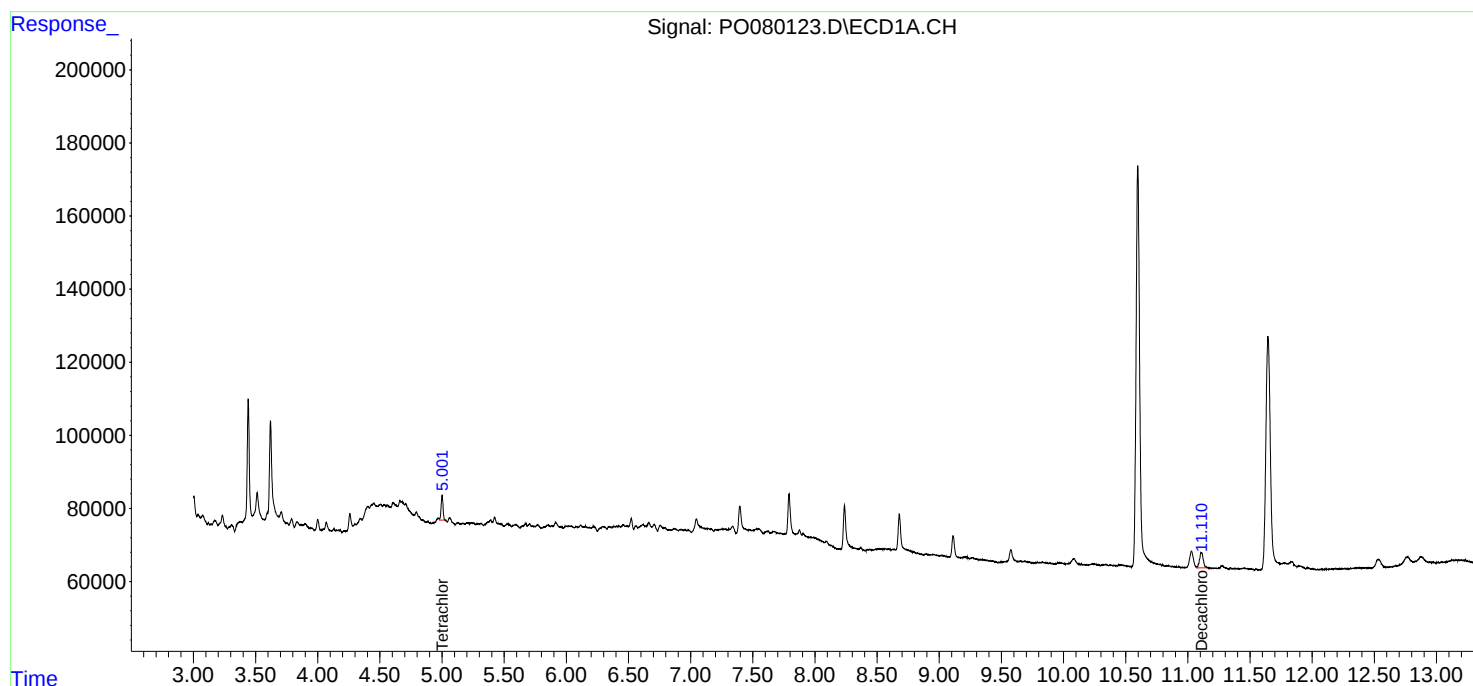


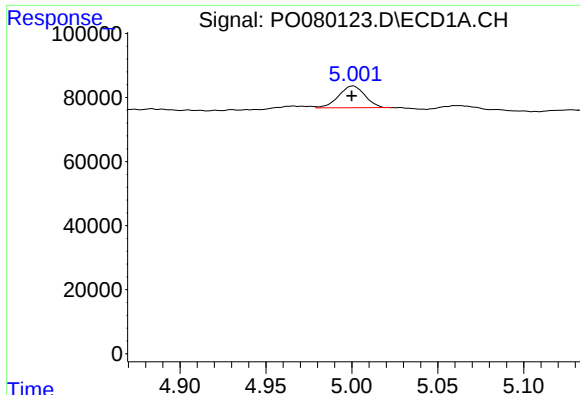

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: 0.000 min
Response: 71963
Conc: 1.19 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HEF3176(2-2)

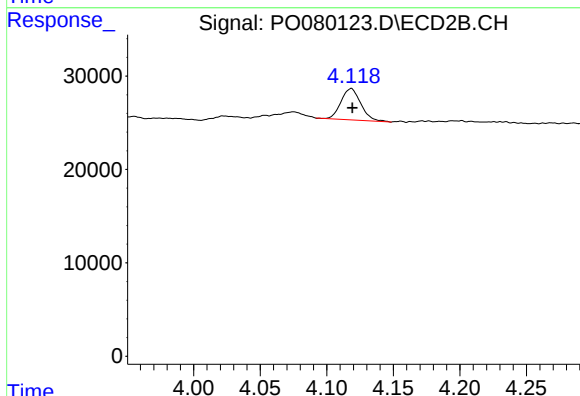


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: 0.000 min
Response: 34974
Conc: 1.53 ng/ml

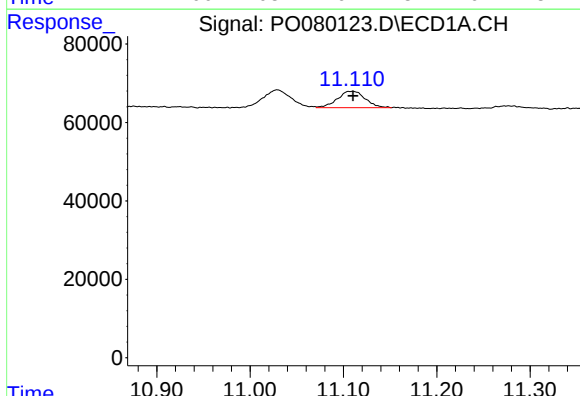

#2 Decachlorobiphenyl

R.T.: 11.110 min
Delta R.T.: -0.001 min
Response: 87171
Conc: 1.86 ng/ml m

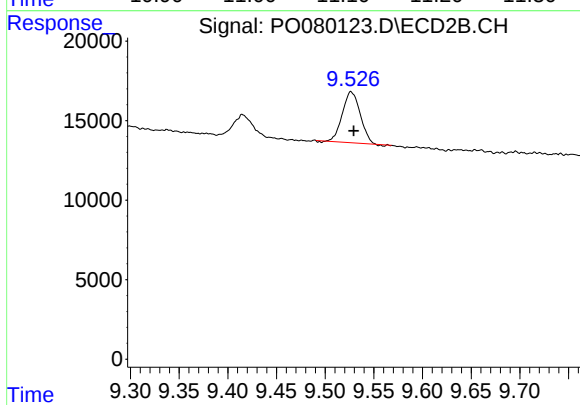

#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.003 min
Response: 40498
Conc: 1.95 ng/ml