

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080323\
 Data File : P0096648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 14:24
 Operator : YP/AJ
 Sample : 03877-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/04/2023
 Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 01:27:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.622	65691233	27648980	19.661	19.519
2) SA Decachlor...	10.234	8.643	43777271	23294483	19.786m	19.803m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080323\
Data File : PO096648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 14:24
Operator : YP/AJ
Sample : 03877-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 01:27:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

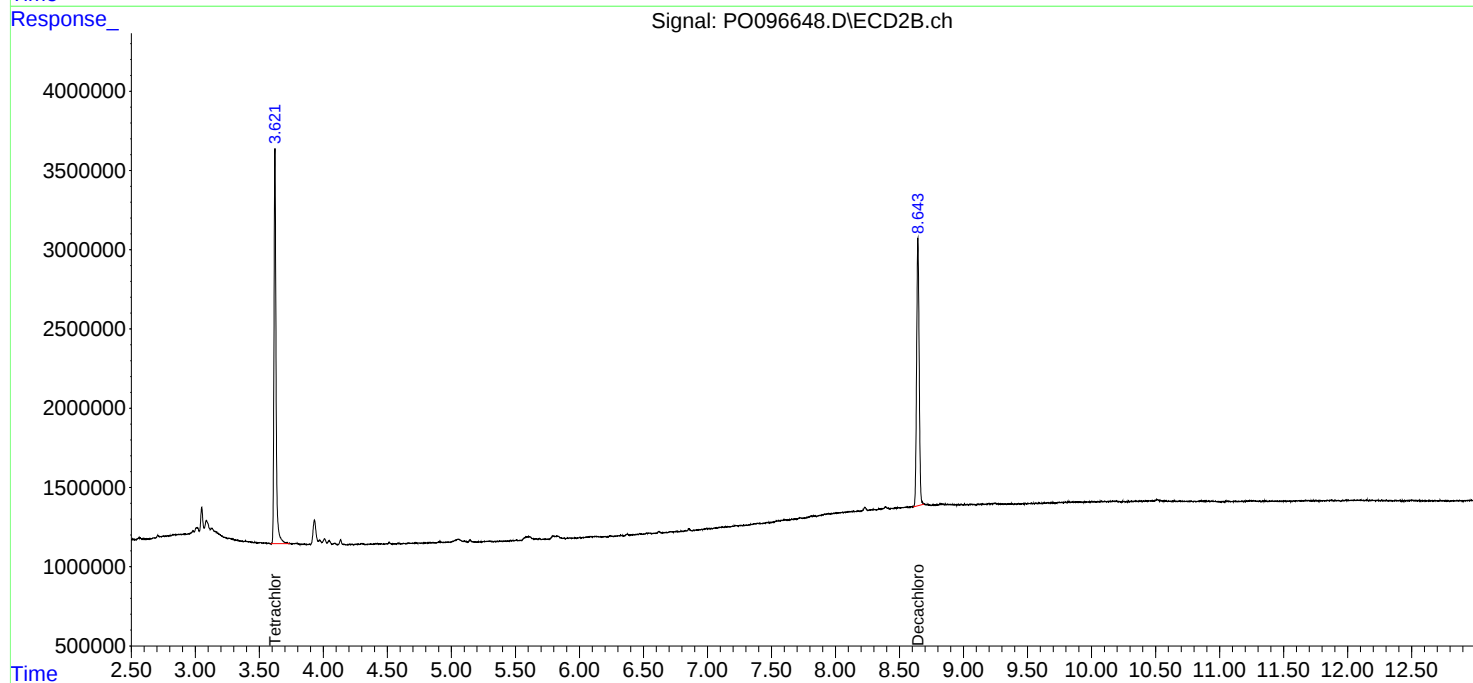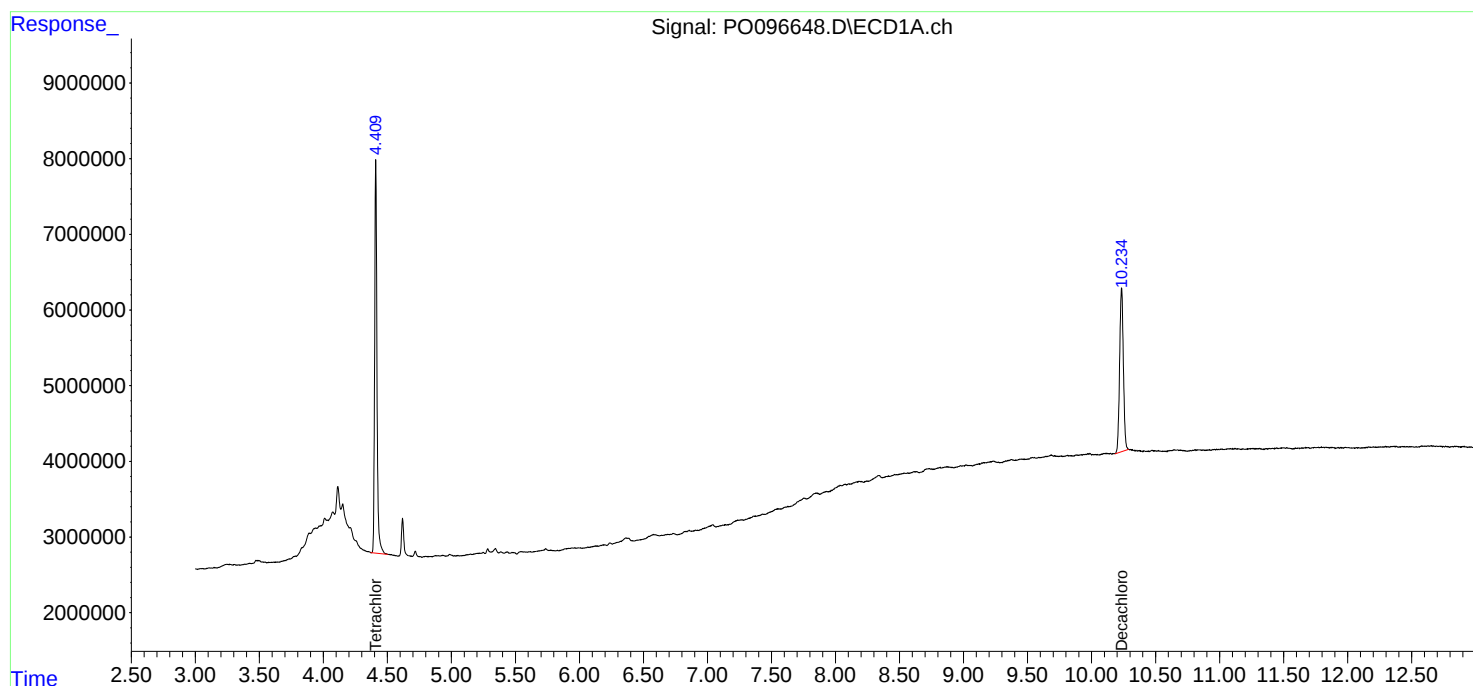

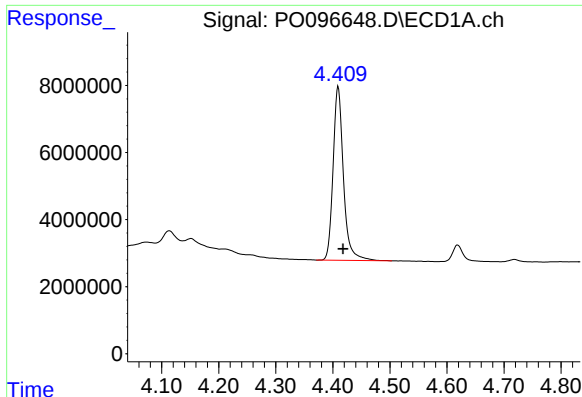

#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: -0.009 min
Response: 65691233
Conc: 19.66 ng/ml

Instrument :


ECD_O

ClientSampleId :

COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

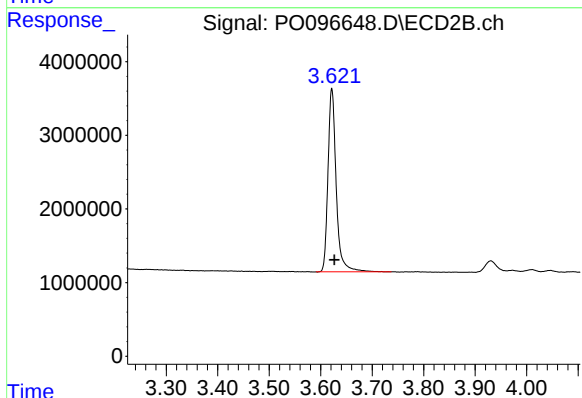


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 27648980
Conc: 19.52 ng/ml

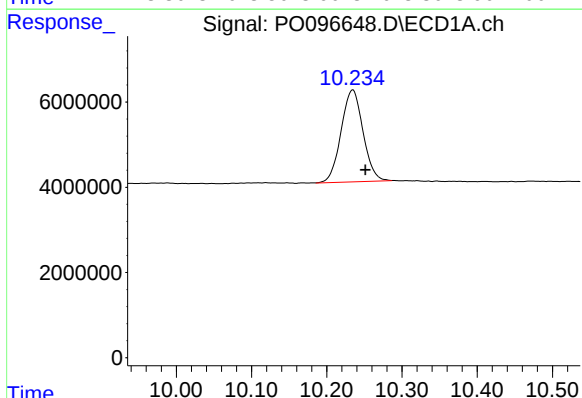

#2 Decachlorobiphenyl

R.T.: 10.234 min
Delta R.T.: -0.017 min
Response: 43777271
Conc: 19.79 ng/ml m

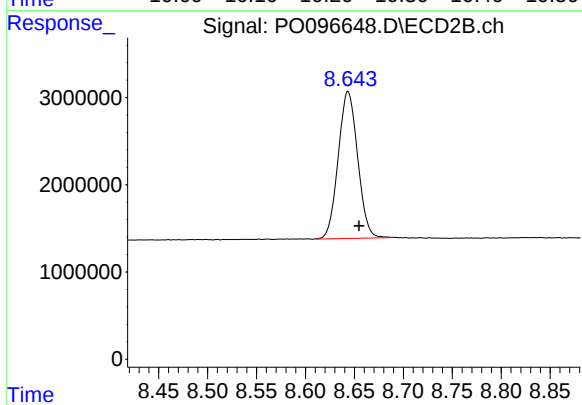

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.012 min
Response: 23294483
Conc: 19.80 ng/ml m