

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080323\
 Data File : P0096656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 16:40
 Operator : YP/AJ
 Sample : 03887-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MCLEAN-TP6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/04/2023
 Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 01:29:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.622	67815184	28200616	20.297	19.908
2) SA Decachlor...	10.228	8.645	47331560	25299184	21.393m	21.507
Target Compounds						
31) L7 AR-1260-1	7.205	6.195	2224111	1555877	17.093	21.351
32) L7 AR-1260-2	7.464	6.384	1954039	1522323	14.263	17.603
33) L7 AR-1260-3	7.750	6.537	4550436	1316915	29.762	16.455 #
34) L7 AR-1260-4	8.041	7.011	3144759	528834	25.826	8.098 #
35) L7 AR-1260-5	8.377	7.255	1421855	884320	6.465m	6.241

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080323\
Data File : PO096656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 16:40
Operator : YP/AJ
Sample : 03887-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MCLEAN-TP6


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 08/04/2023
Supervised By : Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 01:29:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

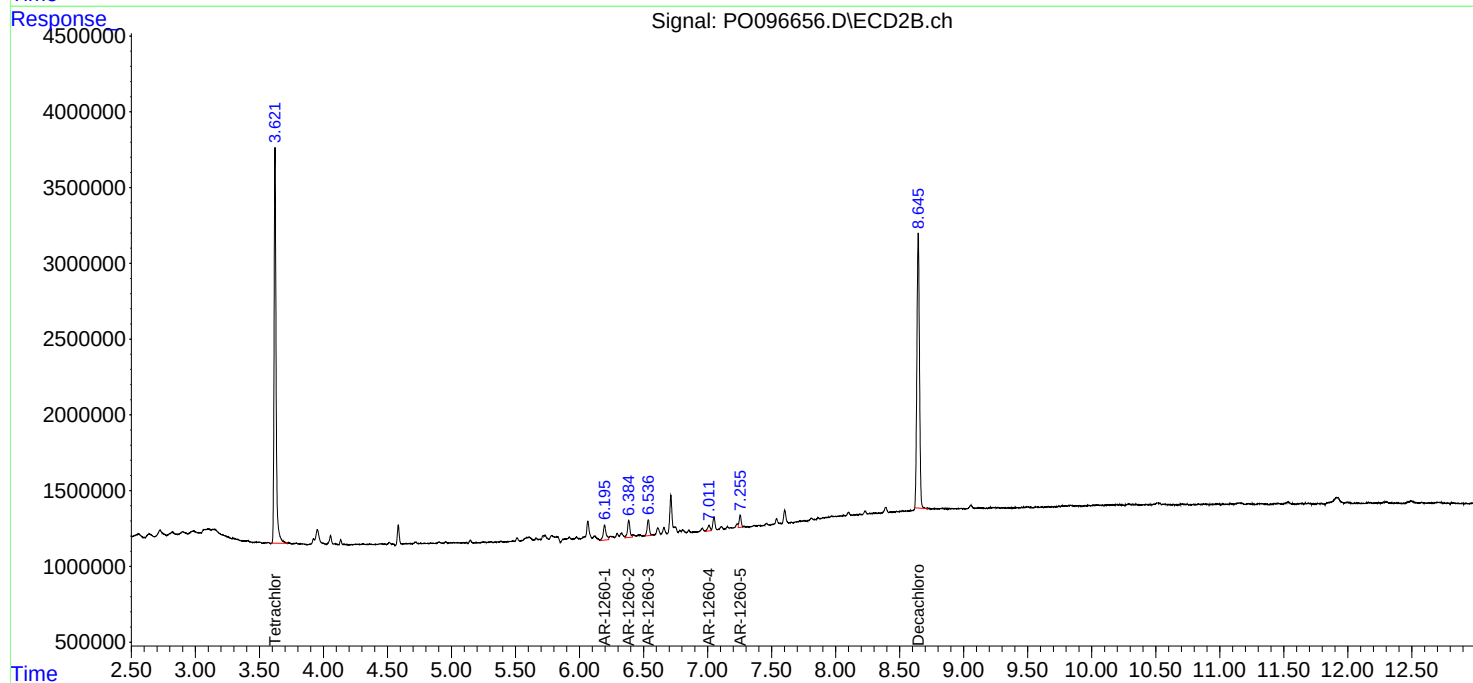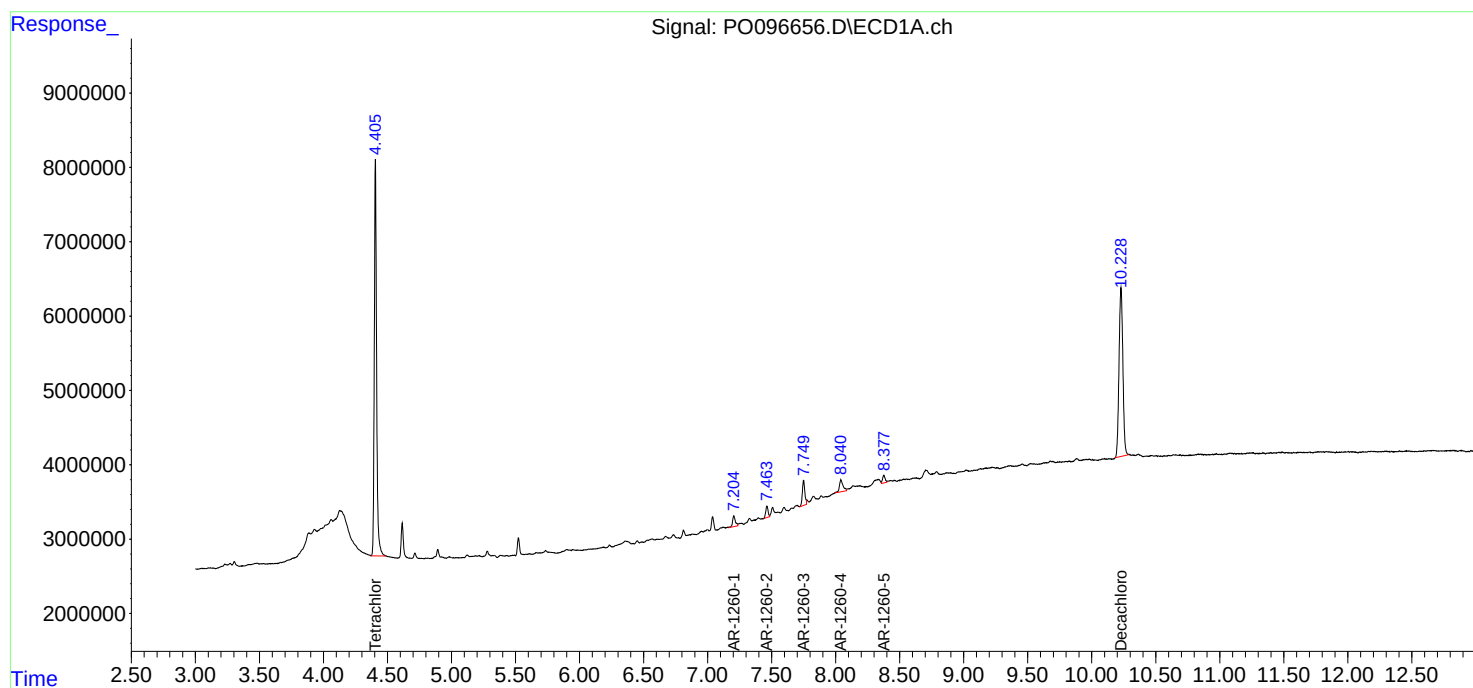

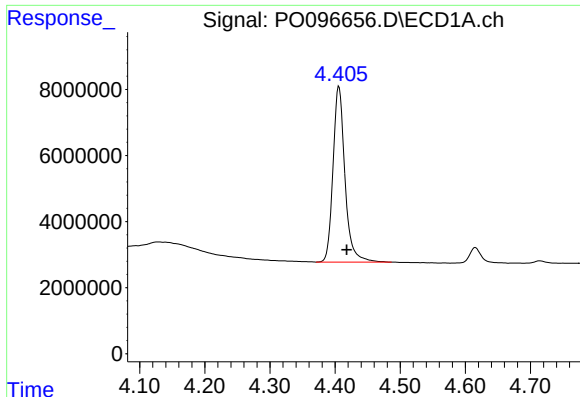

#1 Tetrachloro-m-xylene

R.T.: 4.406 min
Delta R.T.: -0.012 min
Response: 67815184
Conc: 20.30 ng/ml


Instrument :

ECD_O

ClientSampleId :
MCLEAN-TP6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

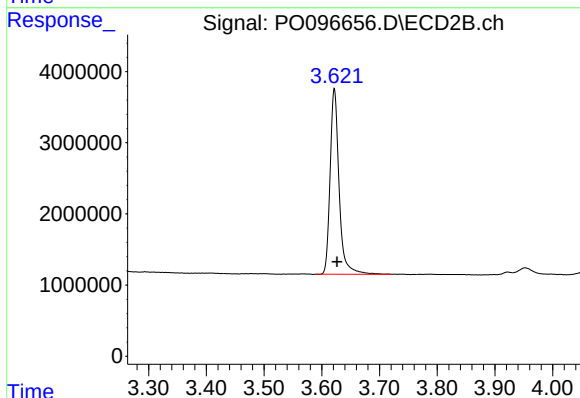


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 28200616
Conc: 19.91 ng/ml

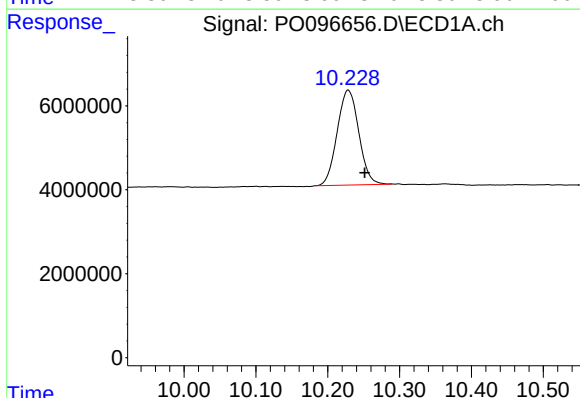


#2 Decachlorobiphenyl

R.T.: 10.228 min
Delta R.T.: -0.024 min
Response: 47331560
Conc: 21.39 ng/ml m

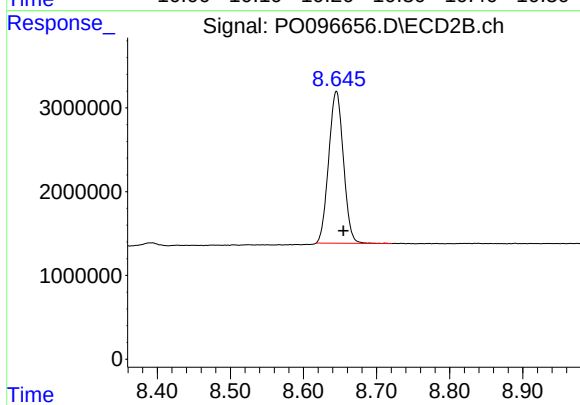

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.010 min
Response: 25299184
Conc: 21.51 ng/ml

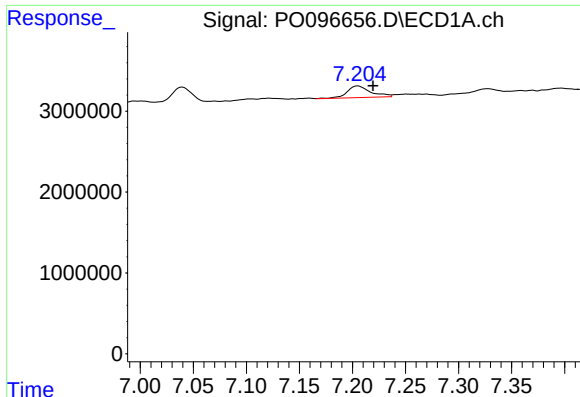


#31 AR-1260-1

R.T.: 7.205 min
Delta R.T.: -0.014 min
Response: 2224111
Conc: 17.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MCLEAN-TP6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

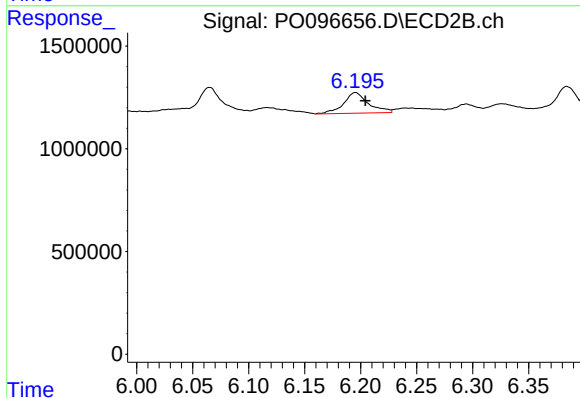


#31 AR-1260-1

R.T.: 6.195 min
Delta R.T.: -0.009 min
Response: 1555877
Conc: 21.35 ng/ml

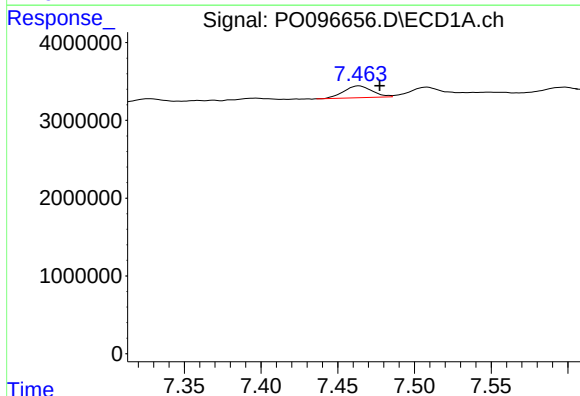


#32 AR-1260-2

R.T.: 7.464 min
Delta R.T.: -0.013 min
Response: 1954039
Conc: 14.26 ng/ml

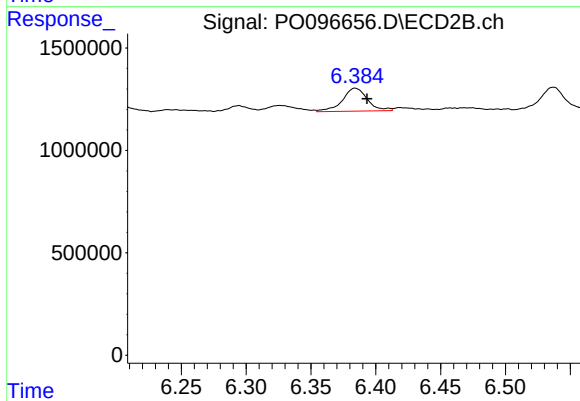

#32 AR-1260-2

R.T.: 6.384 min
Delta R.T.: -0.009 min
Response: 1522323
Conc: 17.60 ng/ml

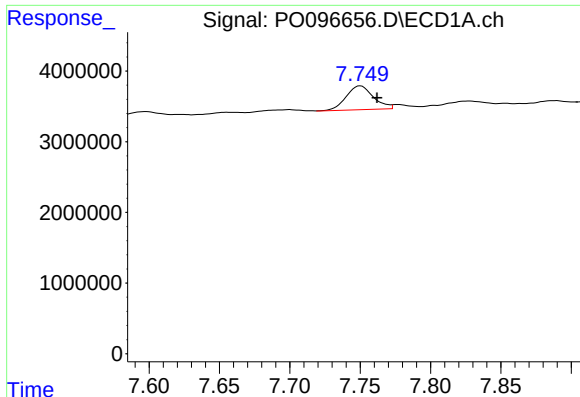


#33 AR-1260-3

R.T.: 7.750 min
Delta R.T.: -0.012 min
Response: 4550436
Conc: 29.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MCLEAN-TP6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

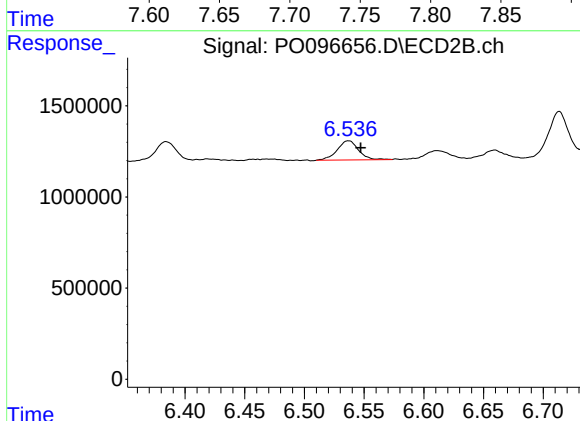


#33 AR-1260-3

R.T.: 6.537 min
Delta R.T.: -0.010 min
Response: 1316915
Conc: 16.45 ng/ml

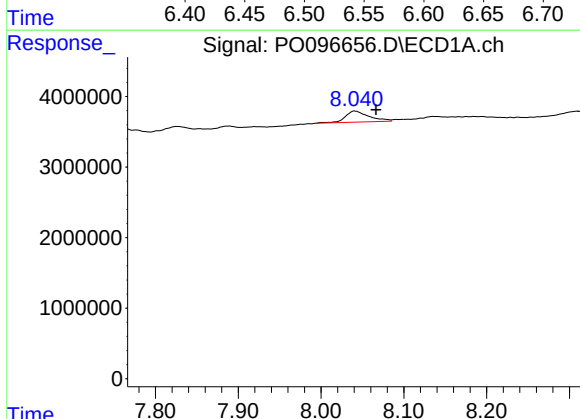


#34 AR-1260-4

R.T.: 8.041 min
Delta R.T.: -0.026 min
Response: 3144759
Conc: 25.83 ng/ml

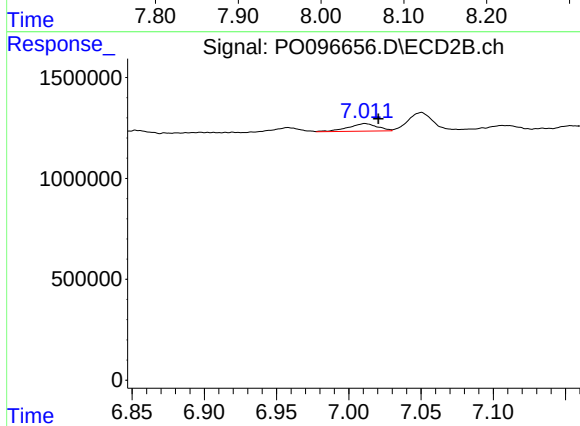

#34 AR-1260-4

R.T.: 7.011 min
Delta R.T.: -0.009 min
Response: 528834
Conc: 8.10 ng/ml

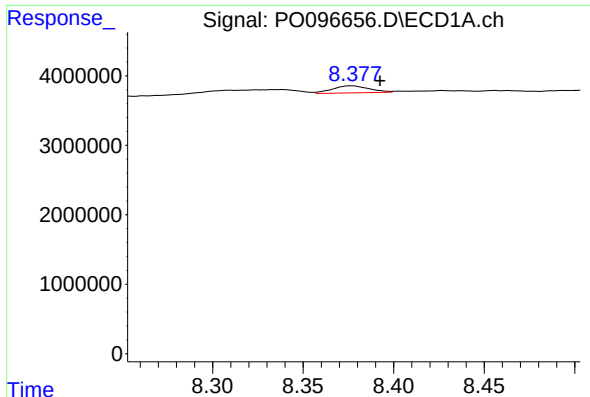


#35 AR-1260-5

R.T.: 8.377 min
Delta R.T.: -0.015 min
Response: 1421855
Conc: 6.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MCLEAN-TP6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

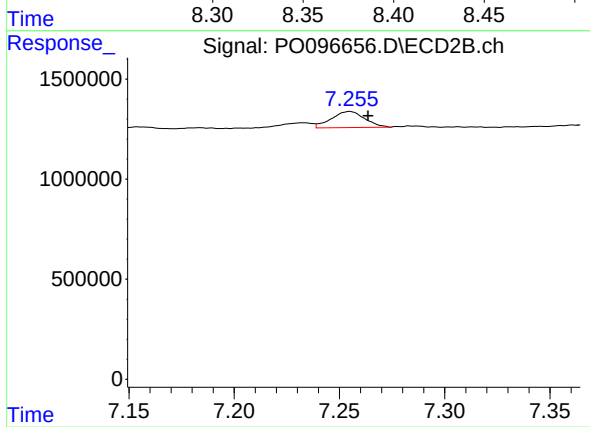

#35 AR-1260-5

R.T.: 7.255 min
Delta R.T.: -0.009 min
Response: 884320
Conc: 6.24 ng/ml