

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0080323\  
 Data File : P0096658.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Aug 2023 17:13  
 Operator : YP/AJ  
 Sample : 03887-07  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 MCLEAN-TP4

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 04 06:29:56 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0072723.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Jul 28 01:38:03 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|--------|-------|----------|----------|---------|---------|
| -----                       |        |       |          |          |         |         |
| System Monitoring Compounds |        |       |          |          |         |         |
| 1) SA Tetrachlo...          | 4.406  | 3.622 | 66382670 | 27339752 | 19.868  | 19.300  |
| 2) SA Decachlor...          | 10.229 | 8.645 | 43805935 | 23768833 | 19.799m | 20.206m |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO080323\  
Data File : PO096658.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Aug 2023 17:13  
Operator : YP/AJ  
Sample : 03887-07  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
MCLEAN-TP4

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 04 06:29:56 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO072723.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Jul 28 01:38:03 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

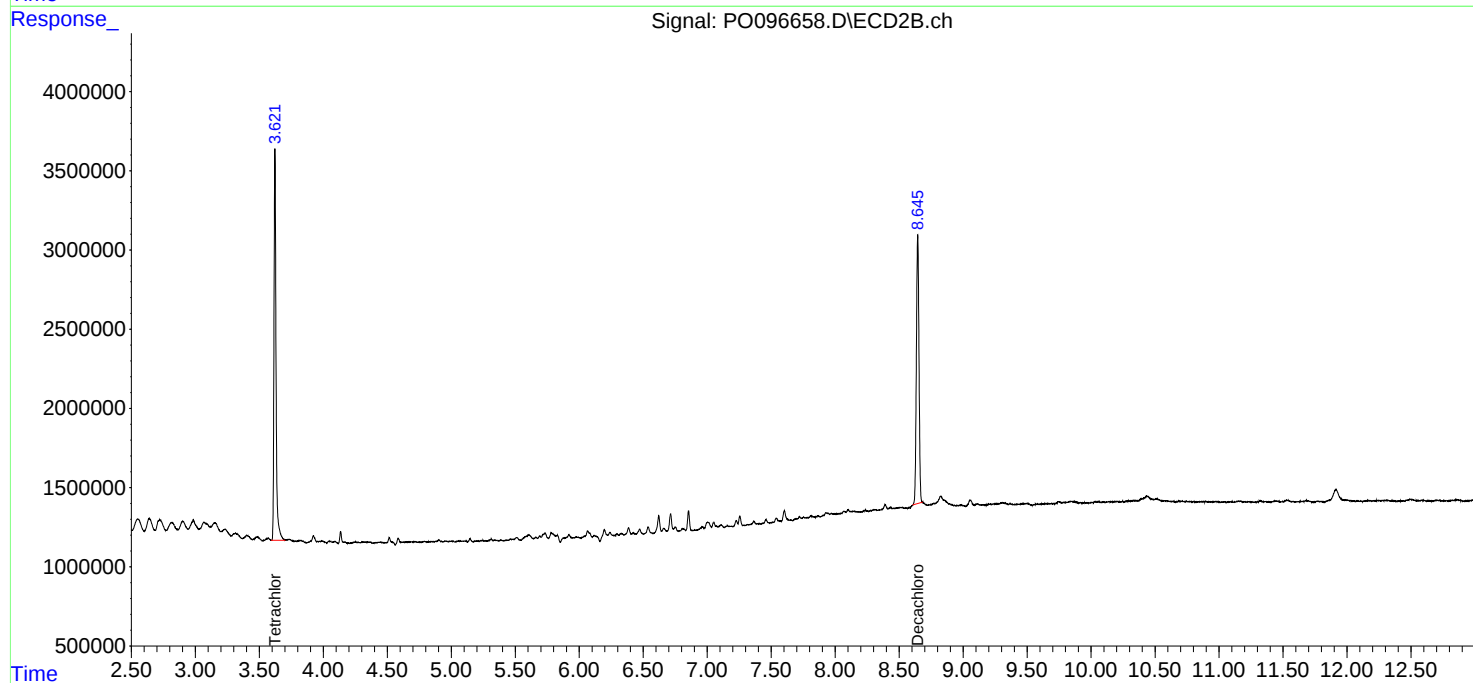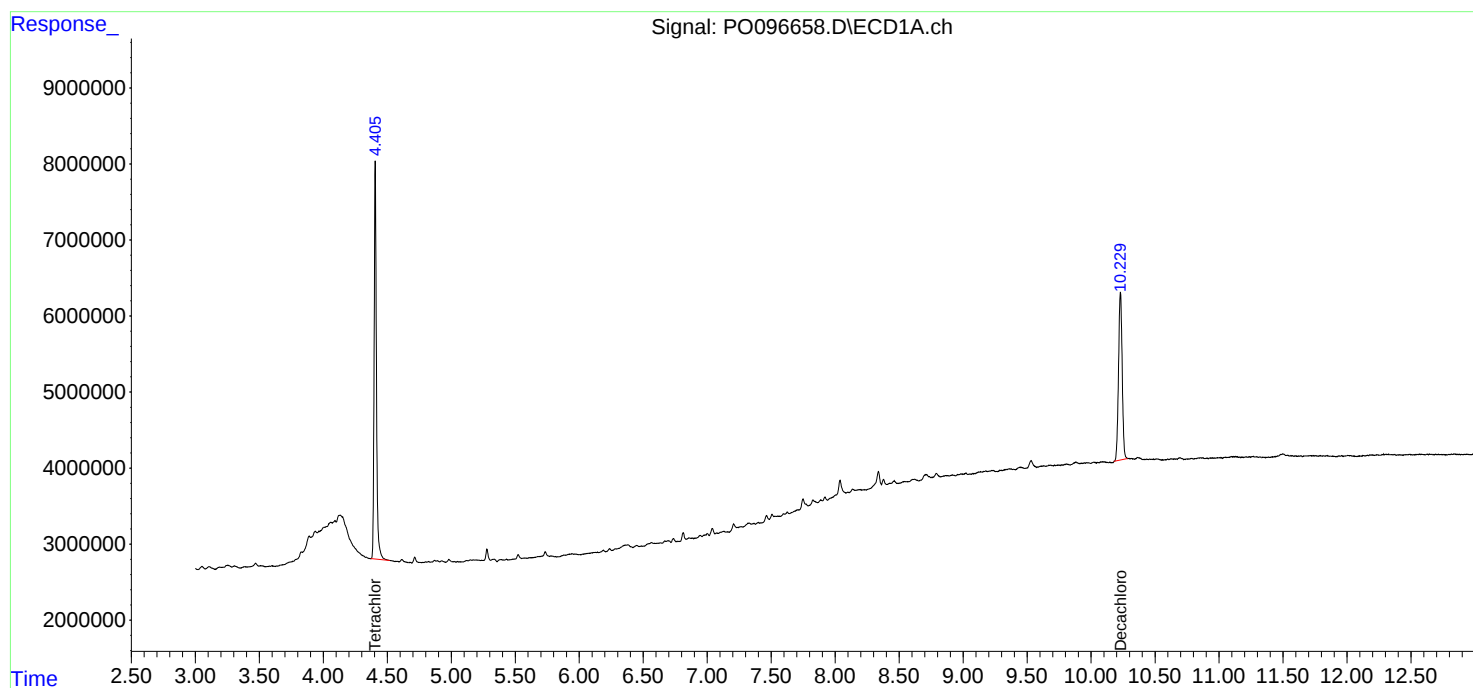


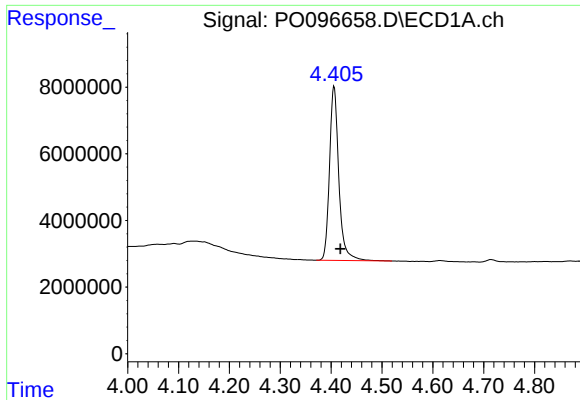

#1 Tetrachloro-m-xylene


R.T.: 4.406 min  
Delta R.T.: -0.012 min  
Response: 66382670  
Conc: 19.87 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
MCLEAN-TP4

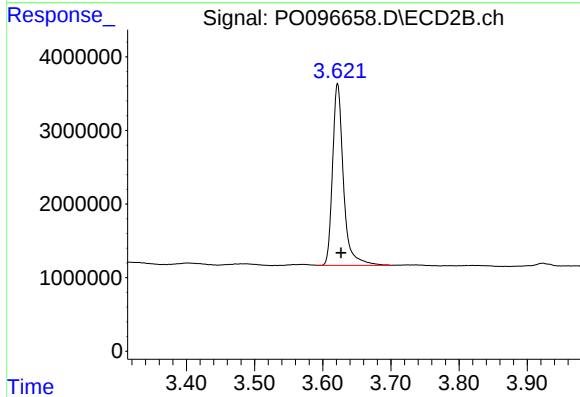


#1 Tetrachloro-m-xylene

R.T.: 3.622 min  
Delta R.T.: -0.005 min  
Response: 27339752  
Conc: 19.30 ng/ml

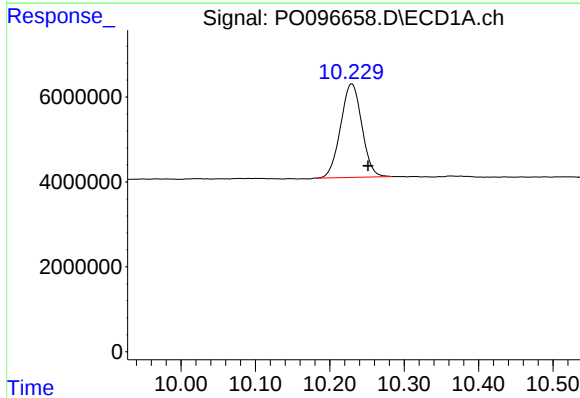

#2 Decachlorobiphenyl

R.T.: 10.229 min  
Delta R.T.: -0.023 min  
Response: 43805935  
Conc: 19.80 ng/ml m

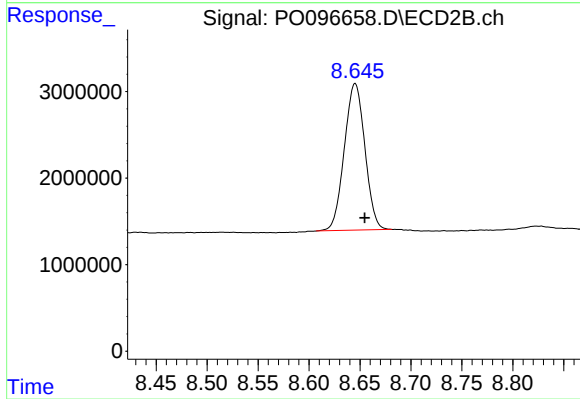

#2 Decachlorobiphenyl

R.T.: 8.645 min  
Delta R.T.: -0.010 min  
Response: 23768833  
Conc: 20.21 ng/ml m