

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080323\
 Data File : P0096672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 21:24
 Operator : YP/AJ
 Sample : 03876-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1030

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/04/2023
 Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 01:34:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.622	33507505	15632707	10.029	11.036
2) SA Decachlor...	10.229	8.645	31438836	12936928	14.209m	10.998
Target Compounds						
26) L6 AR-1254-1	6.450	5.513	10149521	7307384	95.974m	99.444
27) L6 AR-1254-2	6.671	5.661	15376633	7330079	99.110	112.305
28) L6 AR-1254-3	7.041	6.066	13304107	6626261	87.171	65.669
29) L6 AR-1254-4	7.328	6.303	8036939	8022173	82.228	134.477 #
30) L6 AR-1254-5	7.750	6.715	8186656	4238643	74.296	48.827 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080323\
Data File : PO096672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 21:24
Operator : YP/AJ
Sample : 03876-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1030


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 01:34:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

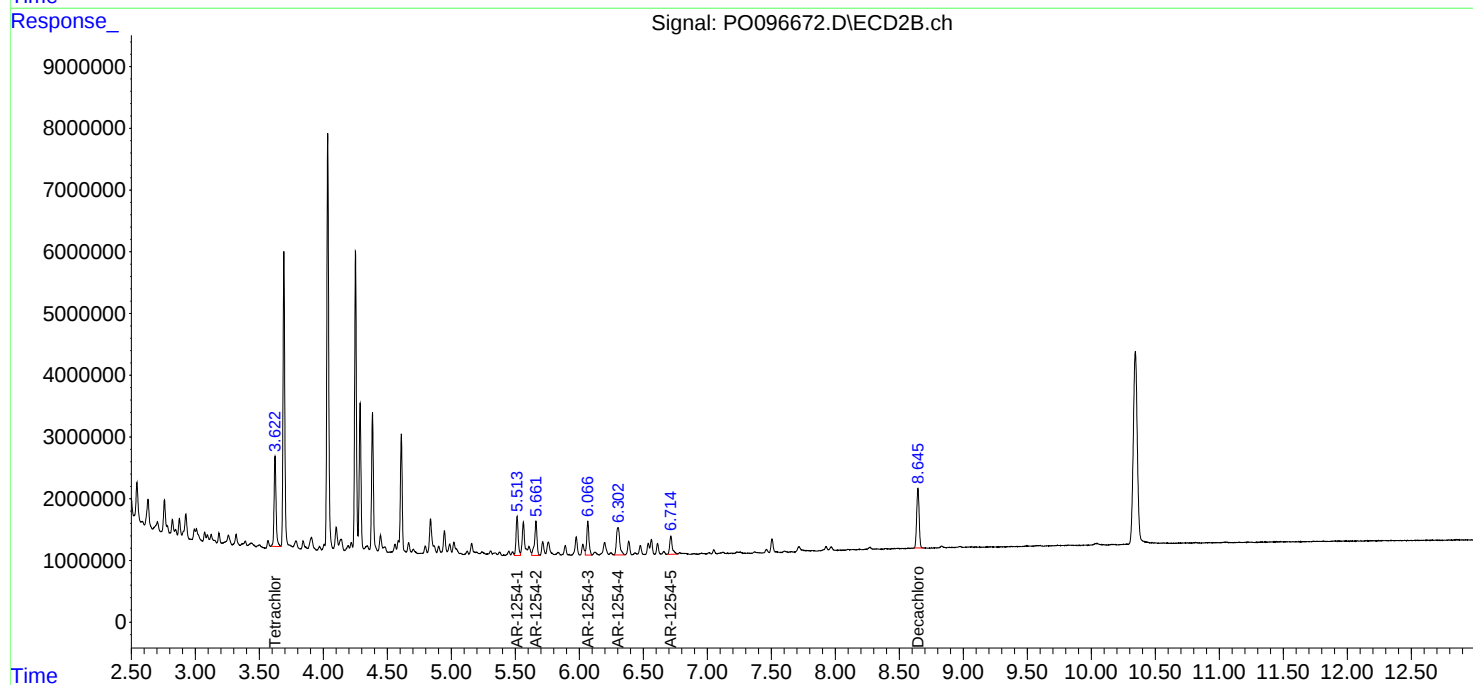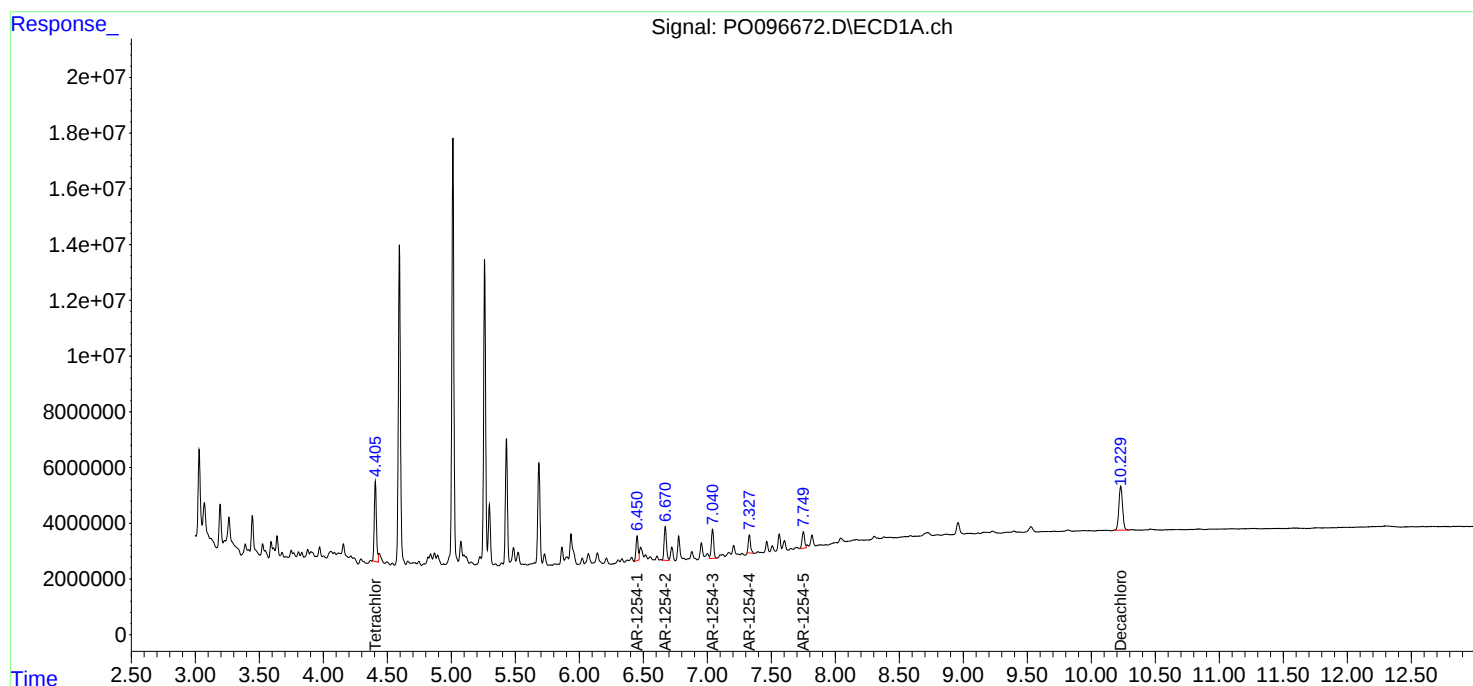

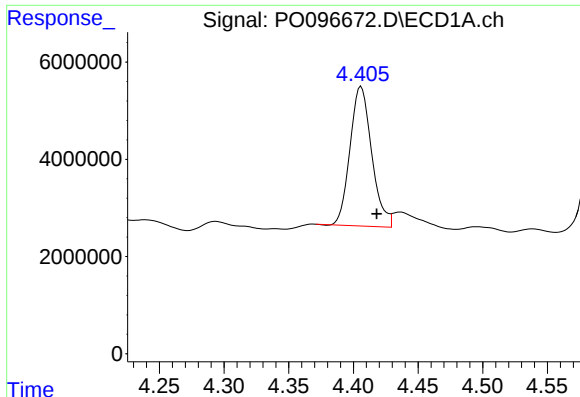


#1 Tetrachloro-m-xylene

R.T.: 4.406 min
Delta R.T.: -0.012 min
Response: 33507505
Conc: 10.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1030


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

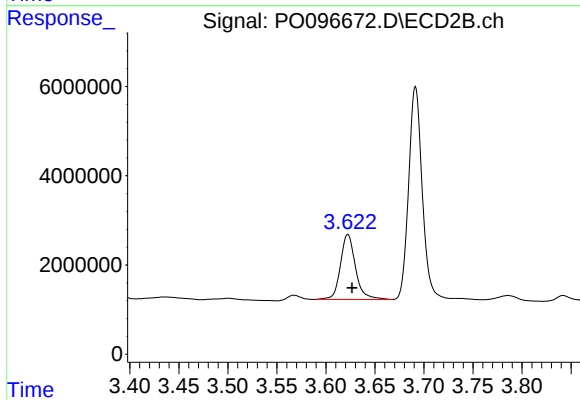


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.004 min
Response: 15632707
Conc: 11.04 ng/ml

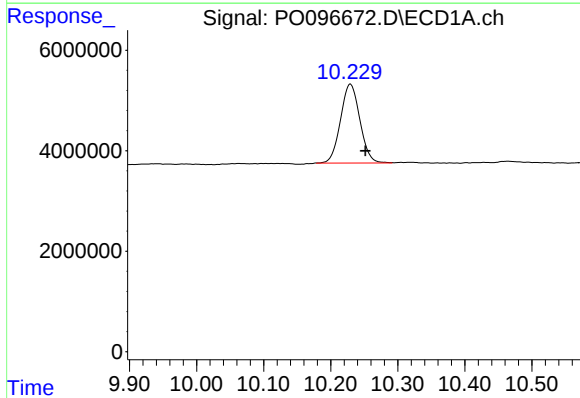


#2 Decachlorobiphenyl

R.T.: 10.229 min
Delta R.T.: -0.023 min
Response: 31438836
Conc: 14.21 ng/ml m

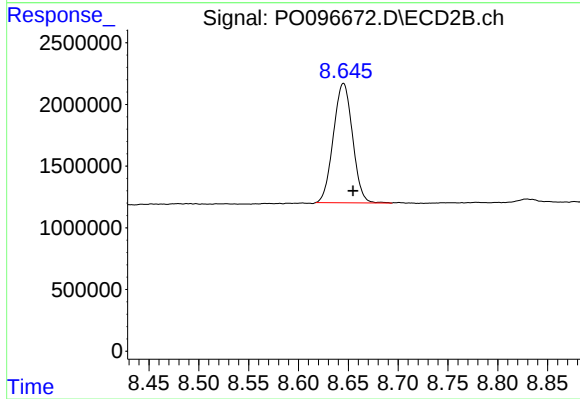

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.009 min
Response: 12936928
Conc: 11.00 ng/ml

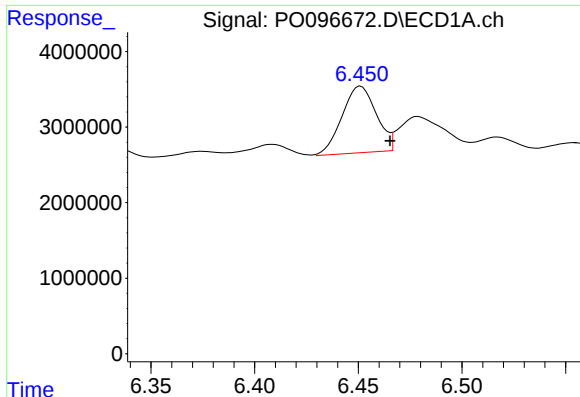


#26 AR-1254-1

R.T.: 6.450 min
Delta R.T.: -0.015 min
Response: 10149521
Conc: 95.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1030


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

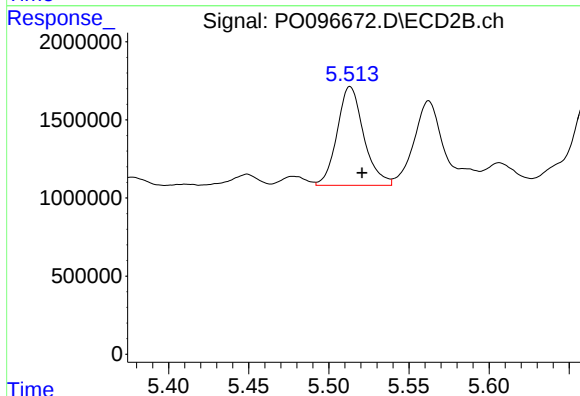


#26 AR-1254-1

R.T.: 5.513 min
Delta R.T.: -0.007 min
Response: 7307384
Conc: 99.44 ng/ml

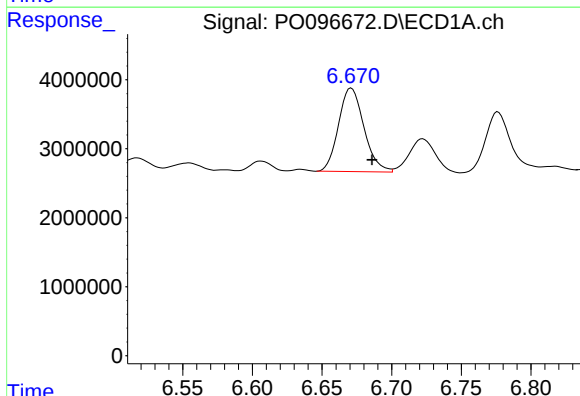


#27 AR-1254-2

R.T.: 6.671 min
Delta R.T.: -0.015 min
Response: 15376633
Conc: 99.11 ng/ml

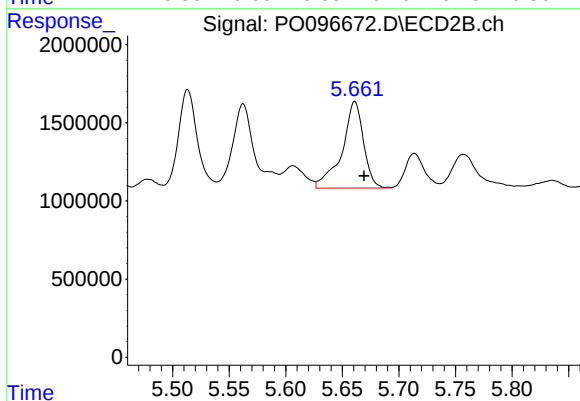

#27 AR-1254-2

R.T.: 5.661 min
Delta R.T.: -0.008 min
Response: 7330079
Conc: 112.31 ng/ml

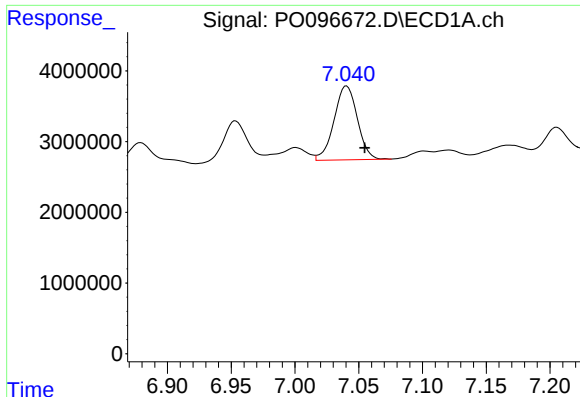


#28 AR-1254-3

R.T.: 7.041 min
Delta R.T.: -0.014 min
Response: 13304107
Conc: 87.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1030


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

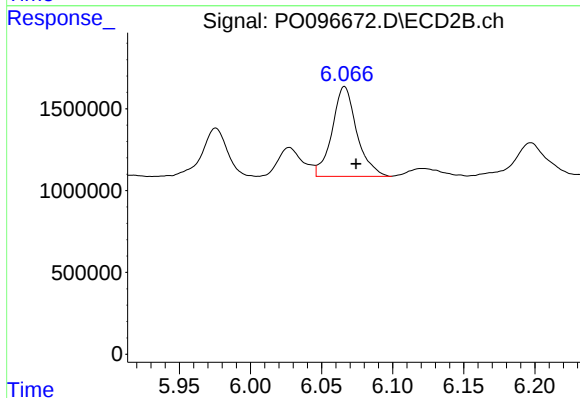


#28 AR-1254-3

R.T.: 6.066 min
Delta R.T.: -0.008 min
Response: 6626261
Conc: 65.67 ng/ml

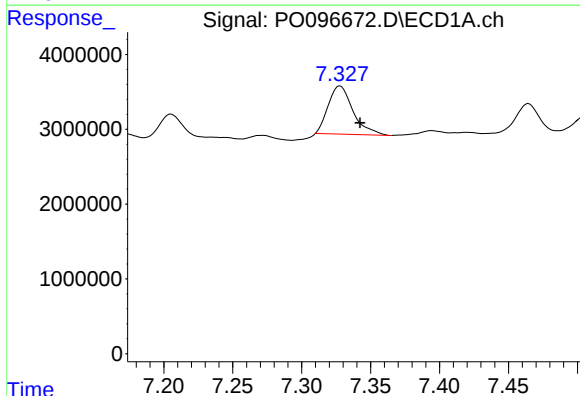


#29 AR-1254-4

R.T.: 7.328 min
Delta R.T.: -0.014 min
Response: 8036939
Conc: 82.23 ng/ml

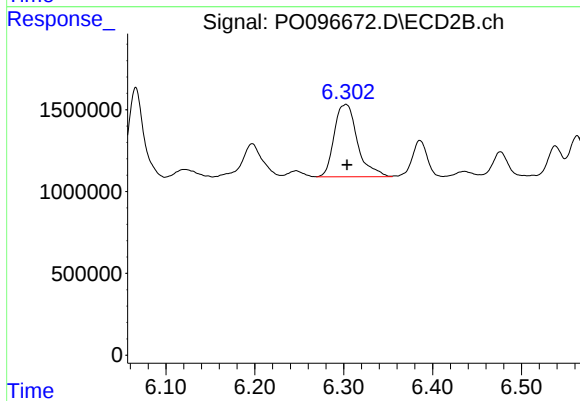

#29 AR-1254-4

R.T.: 6.303 min
Delta R.T.: -0.001 min
Response: 8022173
Conc: 134.48 ng/ml

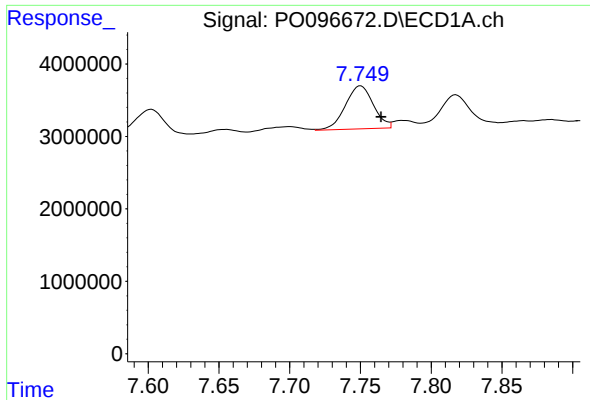


#30 AR-1254-5

R.T.: 7.750 min
Delta R.T.: -0.014 min
Response: 8186656
Conc: 74.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1030

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

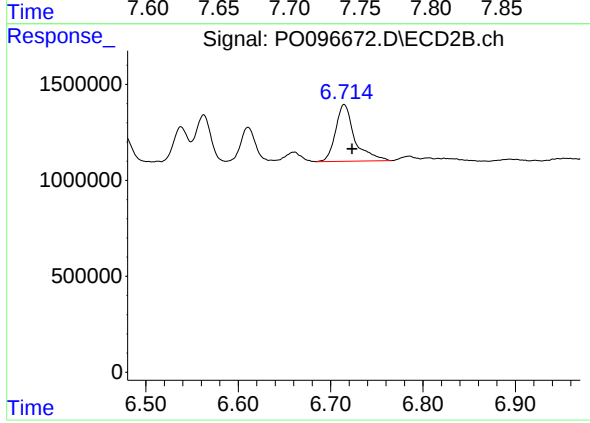

#30 AR-1254-5

R.T.: 6.715 min
Delta R.T.: -0.009 min
Response: 4238643
Conc: 48.83 ng/ml