

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080323\
 Data File : P0096677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2023 22:49
 Operator : YP/AJ
 Sample : 03882-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-1763

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/04/2023
 Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 01:35:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.404	3.622	35777010	15075929	10.708m	10.643
2) SA Decachlor...	10.227	8.643	21777079	11762176	9.843m	9.999

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080323\
Data File : PO096677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2023 22:49
Operator : YP/AJ
Sample : 03882-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRE-1763


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 01:35:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

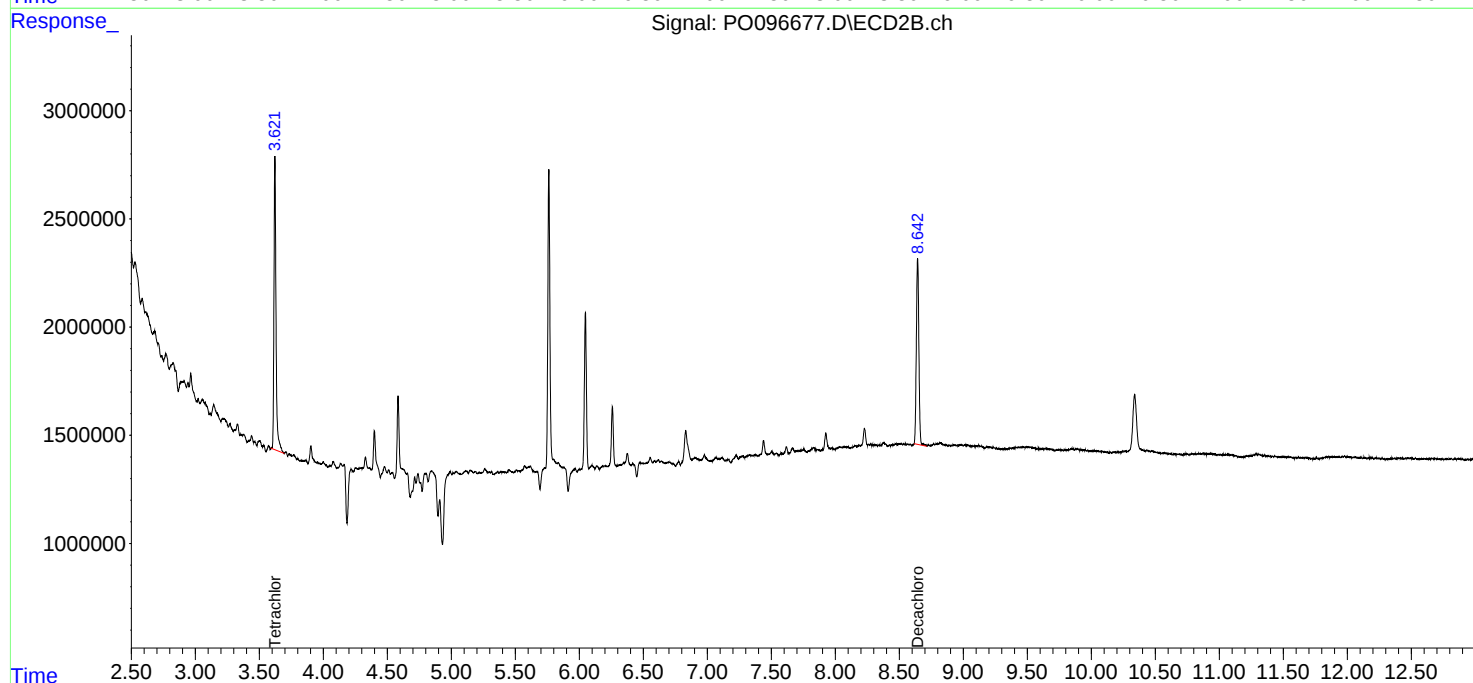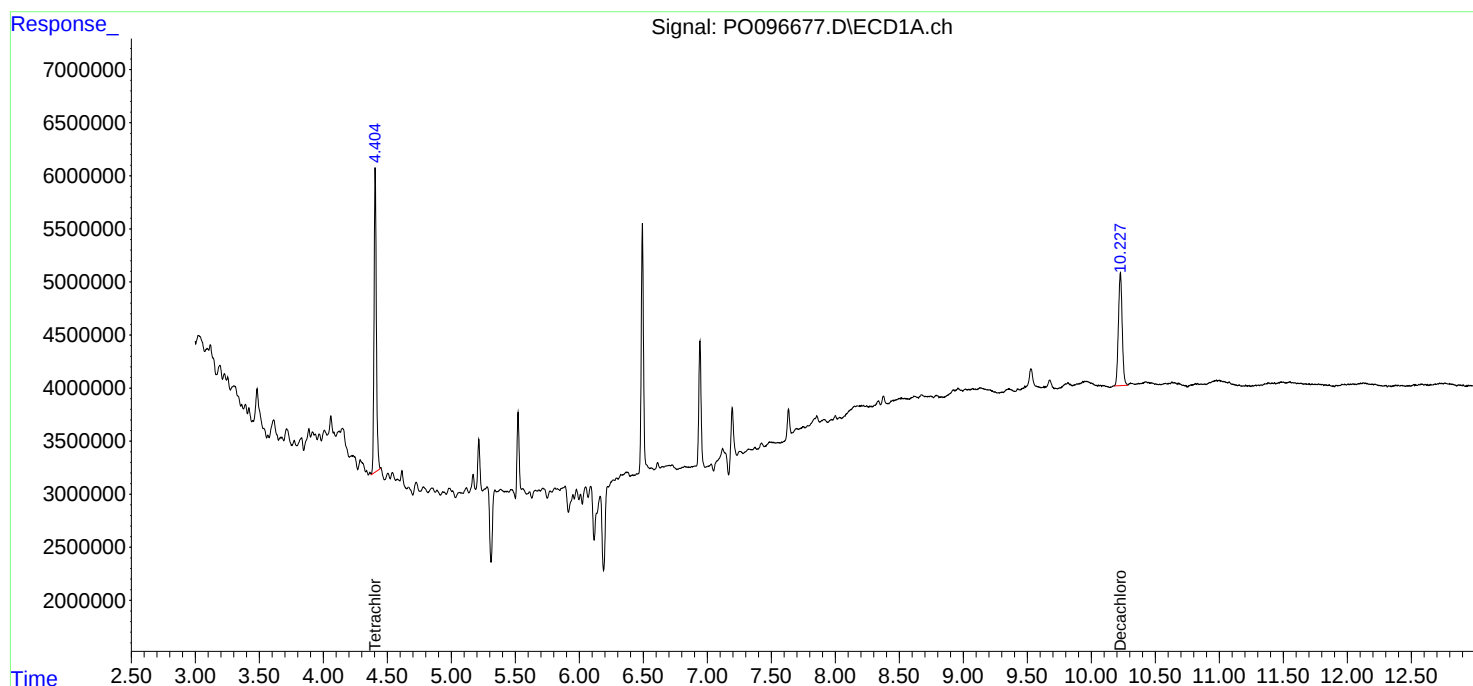

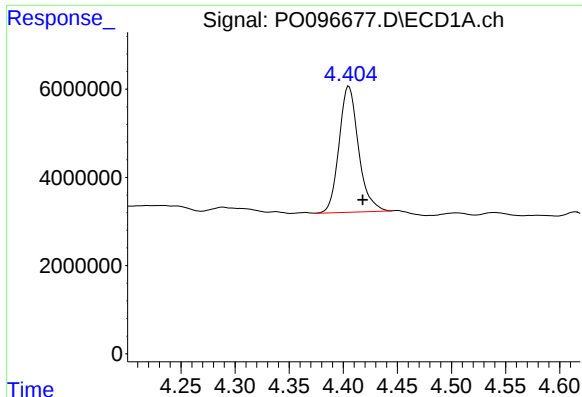


#1 Tetrachloro-m-xylene

R.T.: 4.404 min
Delta R.T.: -0.014 min
Response: 35777010
Conc: 10.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1763


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :Ankita Jodhani 08/04/2023

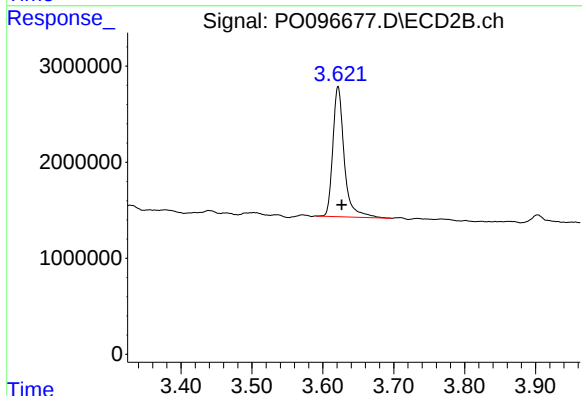


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 15075929
Conc: 10.64 ng/ml

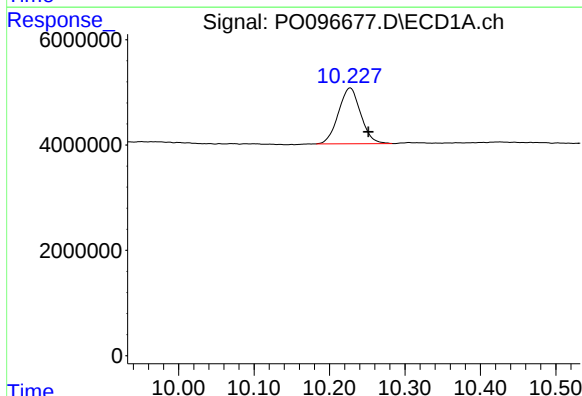

#2 Decachlorobiphenyl

R.T.: 10.227 min
Delta R.T.: -0.025 min
Response: 21777079
Conc: 9.84 ng/ml m

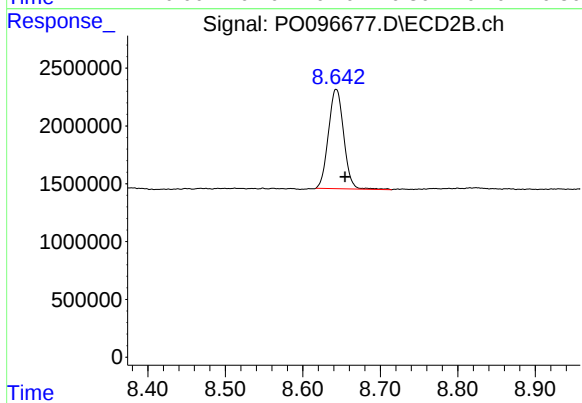

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.012 min
Response: 11762176
Conc: 10.00 ng/ml