

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080420\
 Data File : P0070290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Aug 2020 8:10
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 01:51:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0073020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 30 06:42:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
24)	L5	AR-1248-4	6.596	0.000	2118	0	0.744	N.D.	#
26)	L6	AR-1254-1	6.590f	0.000	6466	0	2.506	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070290\
Data File : PO070290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2020 8:10
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 01:51:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO073020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 30 06:42:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

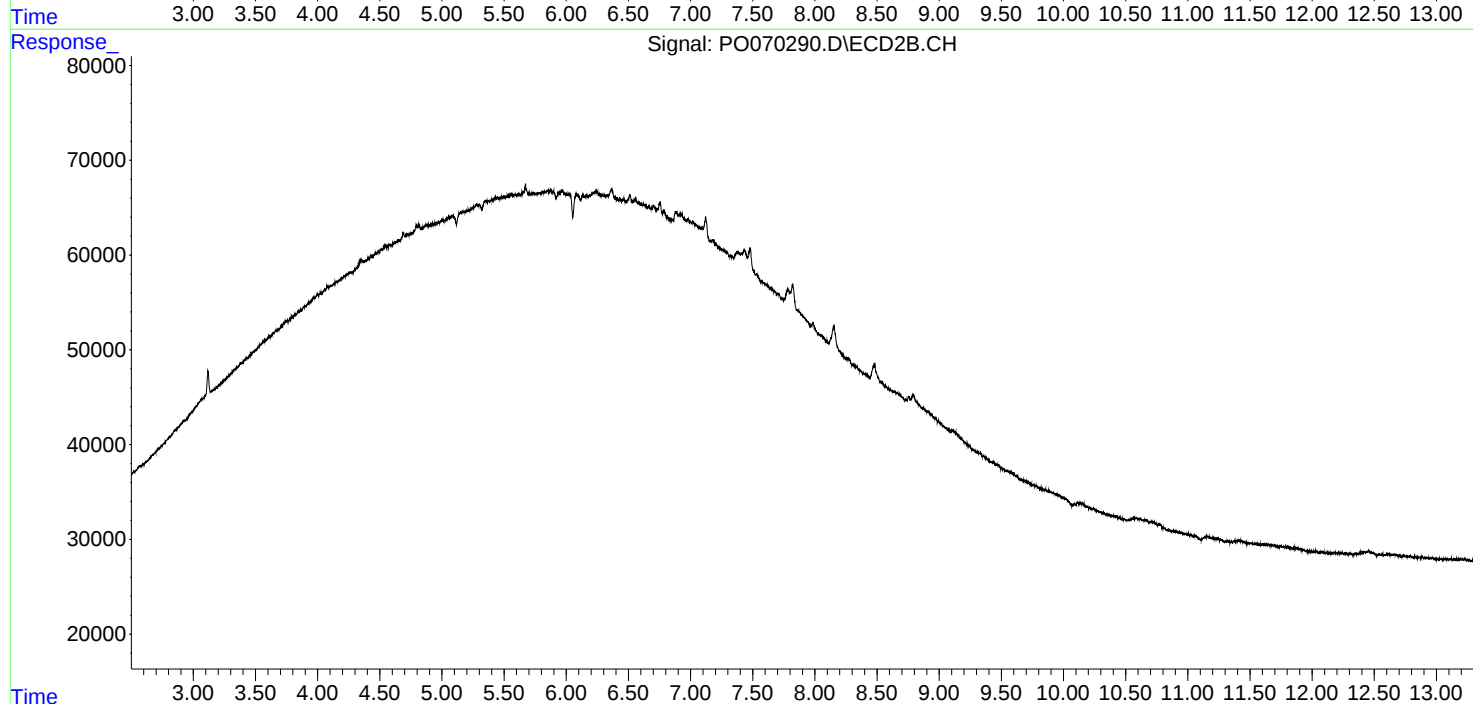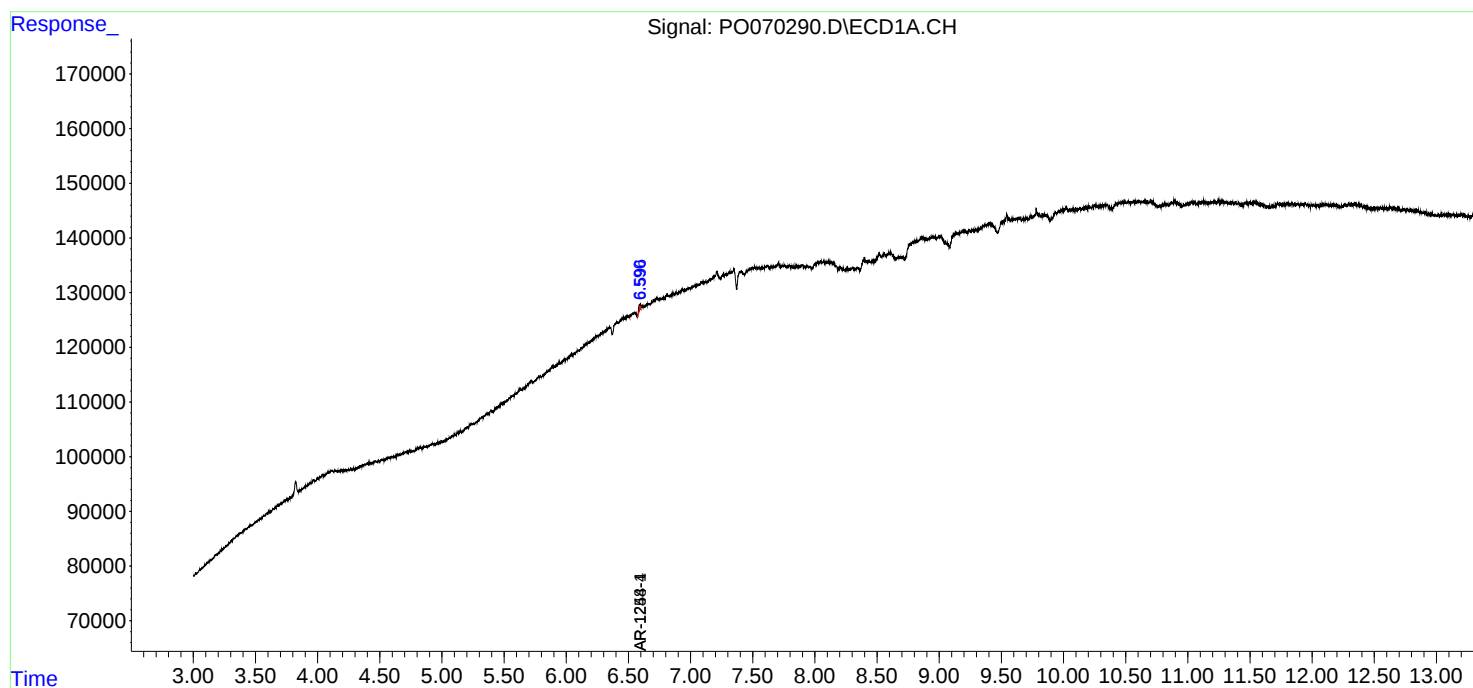


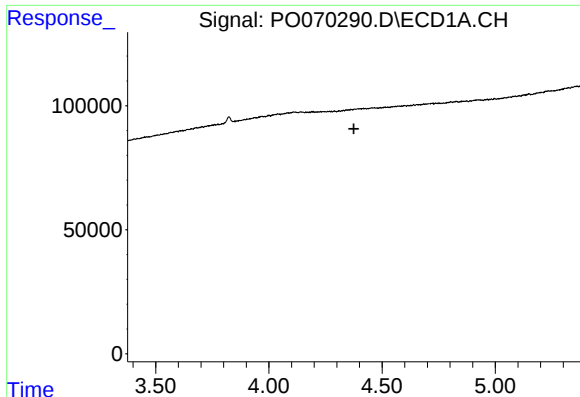

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

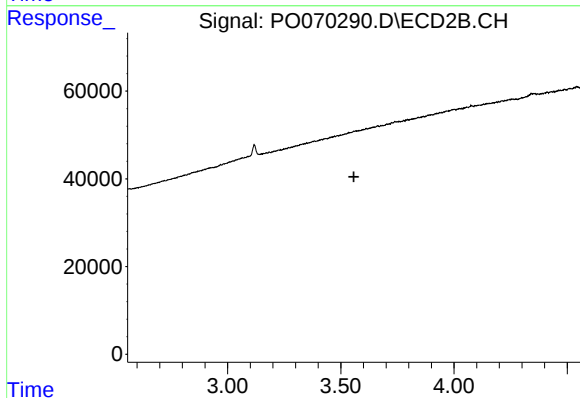


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.558 min
Response: 0
Conc: N.D.

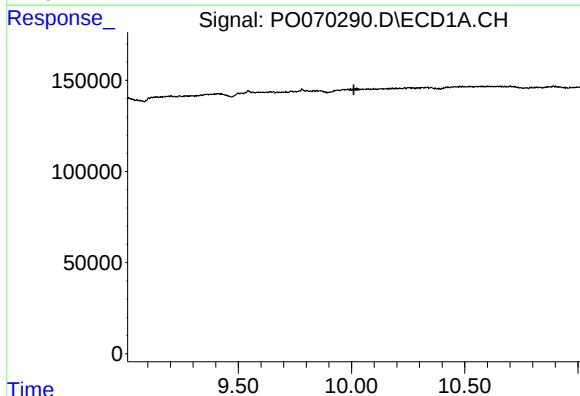


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.010 min
Response: 0
Conc: N.D.

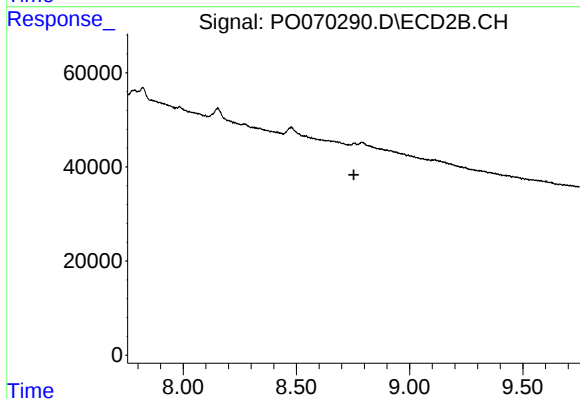

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.754 min
Response: 0
Conc: N.D.

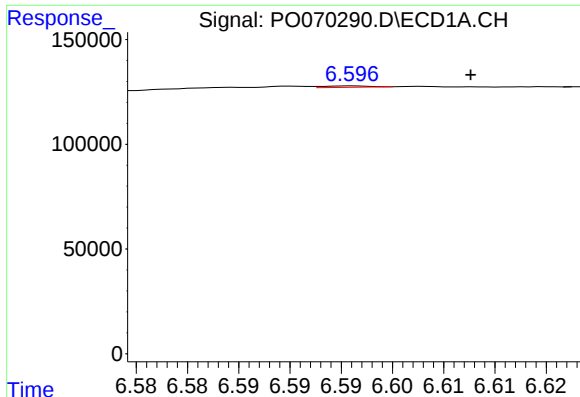

#24 AR-1248-4


R.T.: 6.596 min
Delta R.T.: -0.011 min
Response: 2118
Conc: 0.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

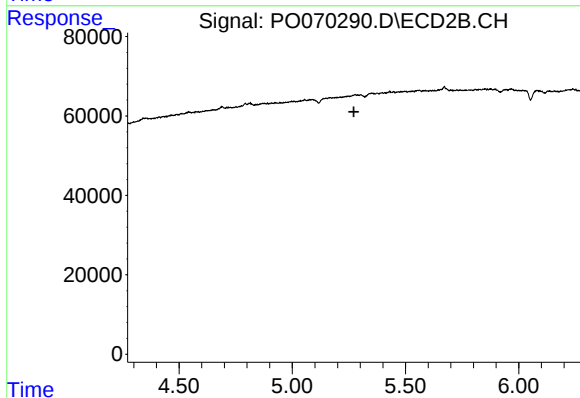


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.272 min
Response: 0
Conc: N.D.

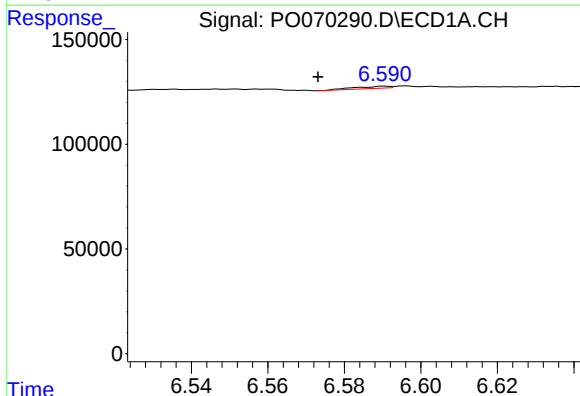

#26 AR-1254-1

R.T.: 6.590 min
Delta R.T.: 0.017 min
Response: 6466
Conc: 2.51 ng/ml

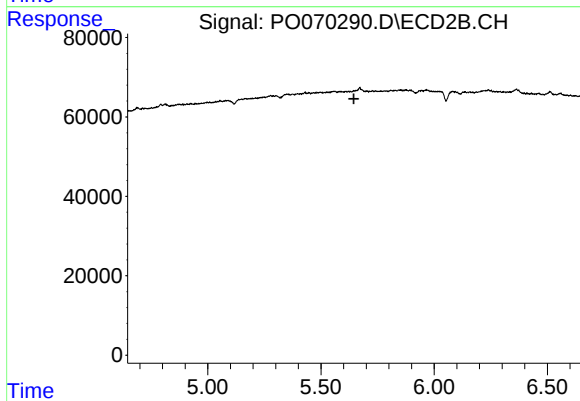

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.645 min
Response: 0
Conc: N.D.