

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080421\
 Data File : P0080151.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Aug 2021 18:33
 Operator : DD\AJ
 Sample : M3271-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:32:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.995	4.114	1431094	532965	23.750	23.272
2)	SA Decachlor...	11.099	9.519	887292	397356	18.915	19.120
Target Compounds							
8)	L2 AR-1221-1	5.248	0.000	612319	0	950.255	N.D. #
9)	L2 AR-1221-2	5.350	0.000	20612	0	44.890	N.D. #
20)	L4 AR-1242-5	7.318	0.000	17180	0	13.532	N.D. #
24)	L5 AR-1248-4	7.280	0.000	55437	0	23.682	N.D. #
25)	L5 AR-1248-5	7.318	0.000	17180	0	7.555	N.D. #
26)	L6 AR-1254-1	7.241	0.000	160326	0	73.396	N.D. #
28)	L6 AR-1254-3	7.869	0.000	37715	0	10.954	N.D. #
32)	L7 AR-1260-2	8.307	0.000	34450	0	11.210	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080421\
Data File : PO080151.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2021 18:33
Operator : DD\AJ
Sample : M3271-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:32:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

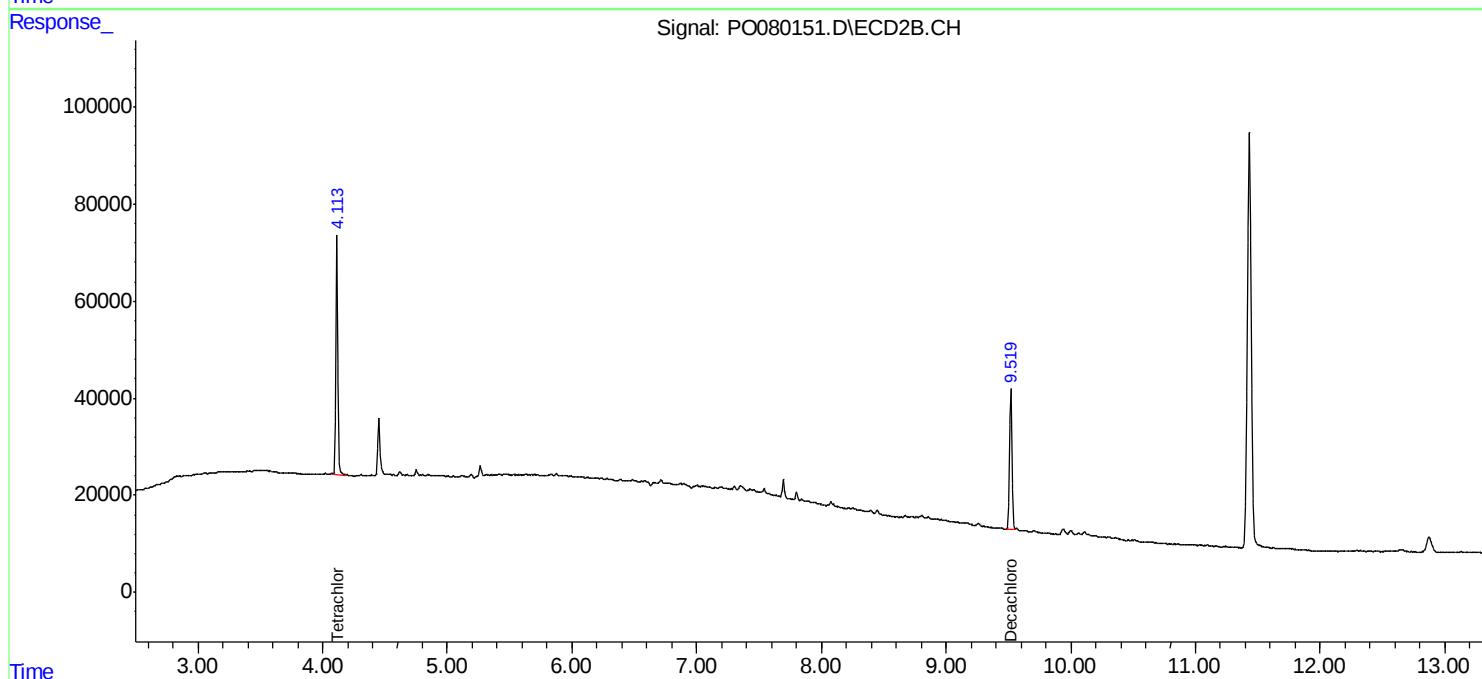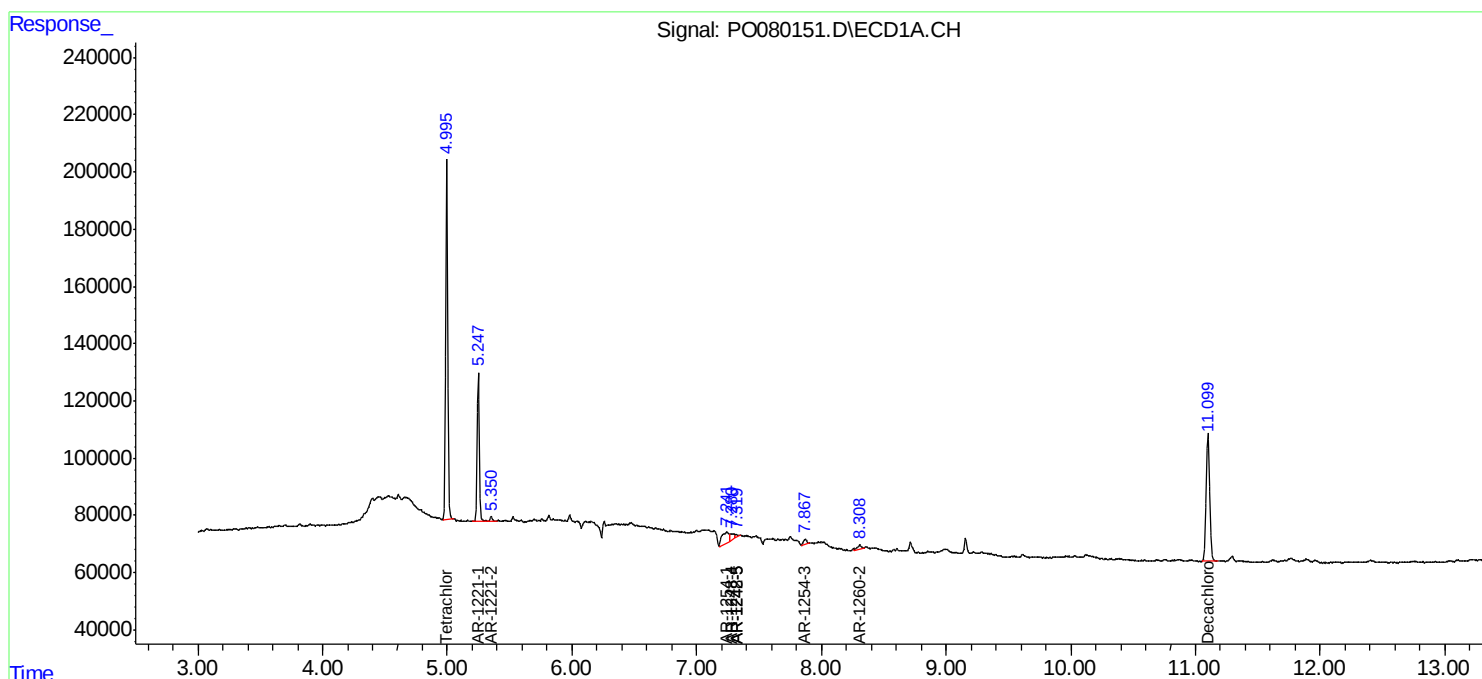


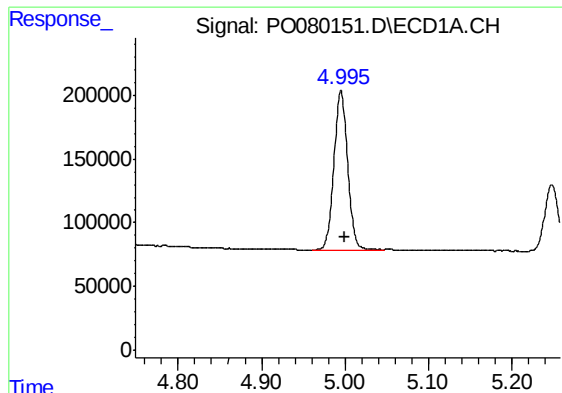

#1 Tetrachloro-m-xylene


R.T.: 4.995 min
Delta R.T.: -0.005 min
Response: 1431094
Conc: 23.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

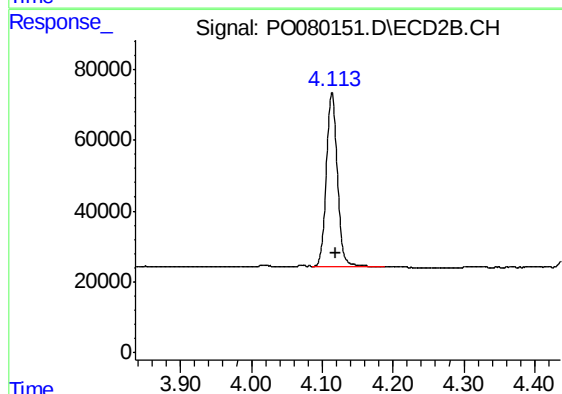


#1 Tetrachloro-m-xylene

R.T.: 4.114 min
Delta R.T.: -0.005 min
Response: 532965
Conc: 23.27 ng/ml

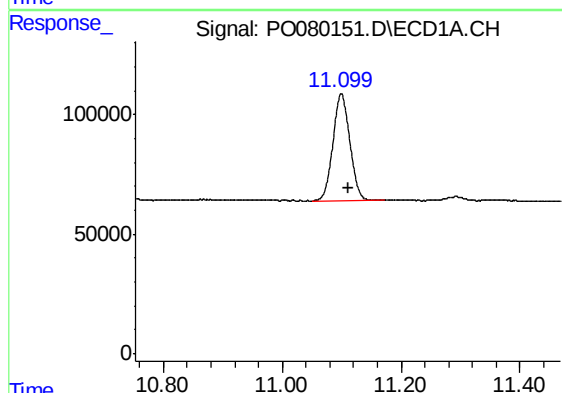


#2 Decachlorobiphenyl

R.T.: 11.099 min
Delta R.T.: -0.011 min
Response: 887292
Conc: 18.91 ng/ml

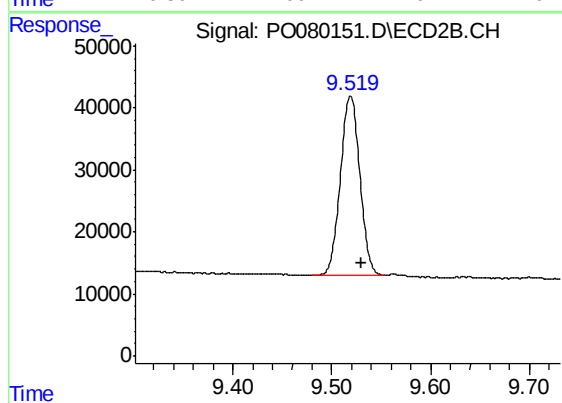

#2 Decachlorobiphenyl


R.T.: 9.519 min
Delta R.T.: -0.010 min
Response: 397356
Conc: 19.12 ng/ml

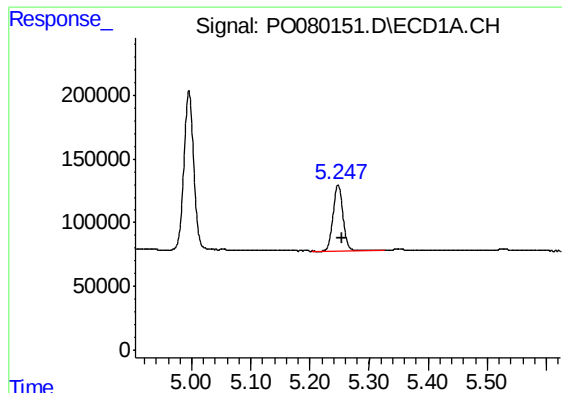

#8 AR-1221-1


R.T.: 5.248 min
Delta R.T.: -0.006 min
Response: 612319
Conc: 950.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

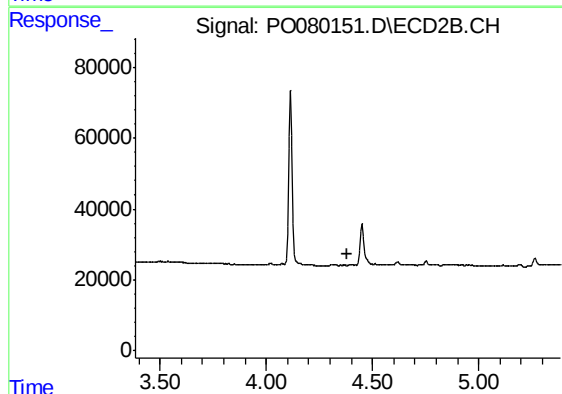


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.384 min
Response: 0
Conc: N.D.

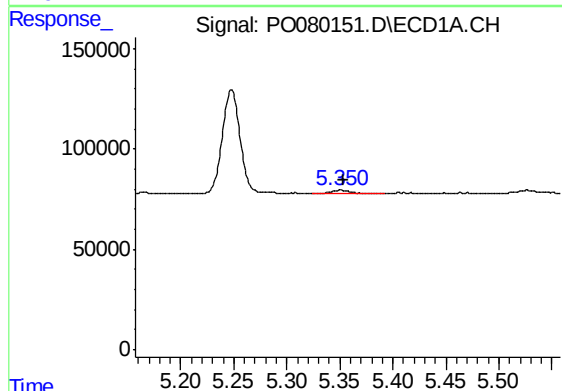


#9 AR-1221-2

R.T.: 5.350 min
Delta R.T.: -0.003 min
Response: 20612
Conc: 44.89 ng/ml

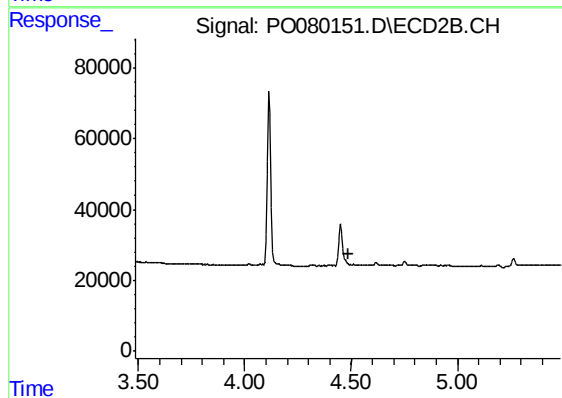

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.485 min
Response: 0
Conc: N.D.

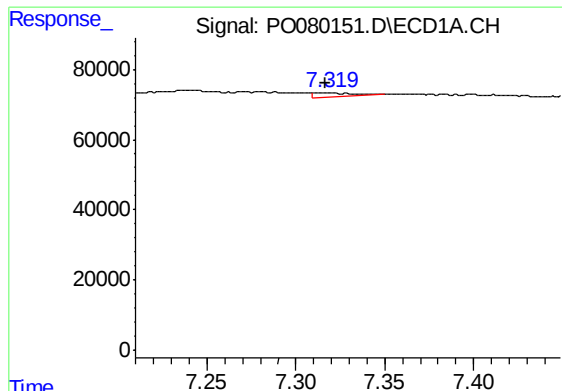

#20 AR-1242-5


R.T.: 7.318 min
Delta R.T.: 0.002 min
Response: 17180
Conc: 13.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

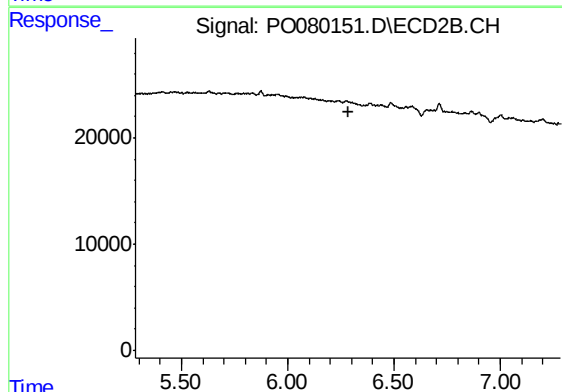


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.284 min
Response: 0
Conc: N.D.

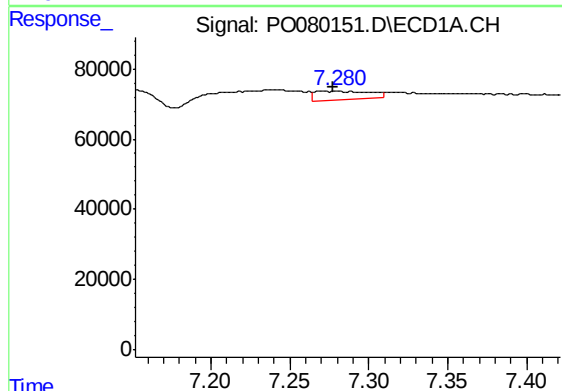


#24 AR-1248-4

R.T.: 7.280 min
Delta R.T.: 0.003 min
Response: 55437
Conc: 23.68 ng/ml

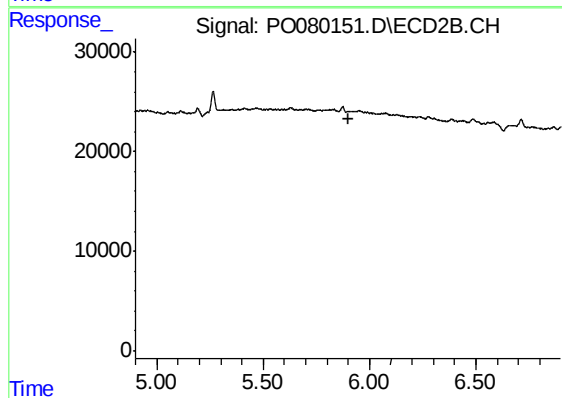

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.899 min
Response: 0
Conc: N.D.

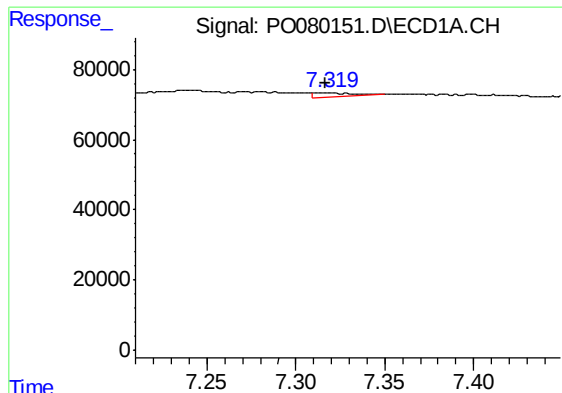

#25 AR-1248-5


R.T.: 7.318 min
Delta R.T.: 0.001 min
Response: 17180
Conc: 7.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

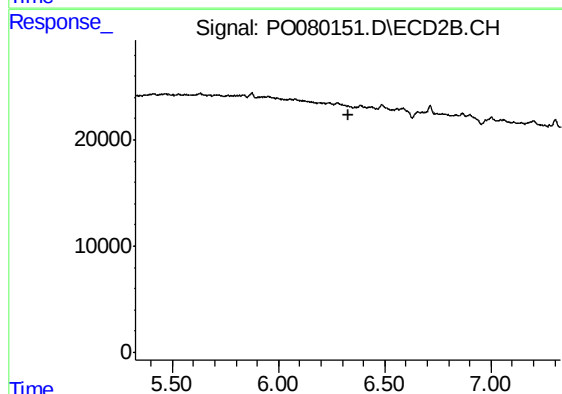


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

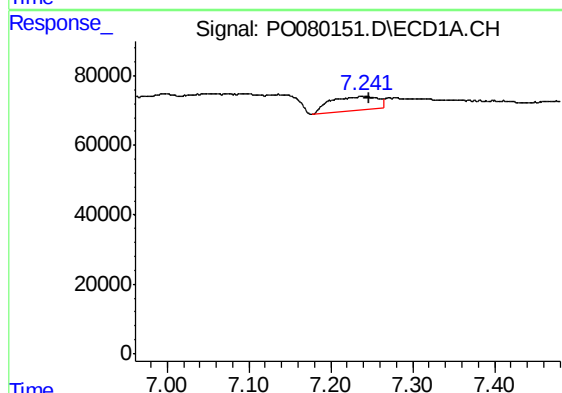


#26 AR-1254-1

R.T.: 7.241 min
Delta R.T.: -0.006 min
Response: 160326
Conc: 73.40 ng/ml

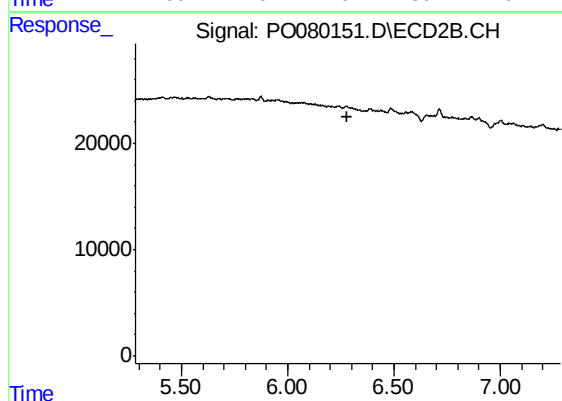

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

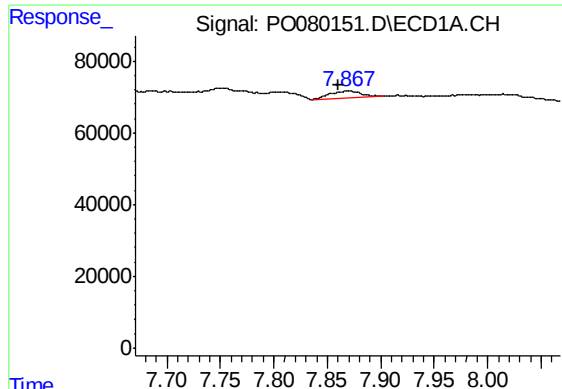

#28 AR-1254-3


R.T.: 7.869 min
Delta R.T.: 0.009 min
Response: 37715
Conc: 10.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

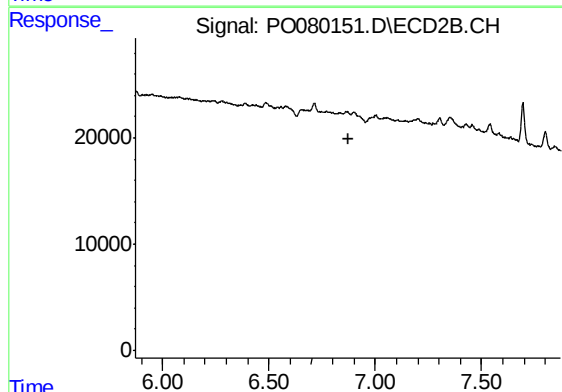


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.872 min
Response: 0
Conc: N.D.

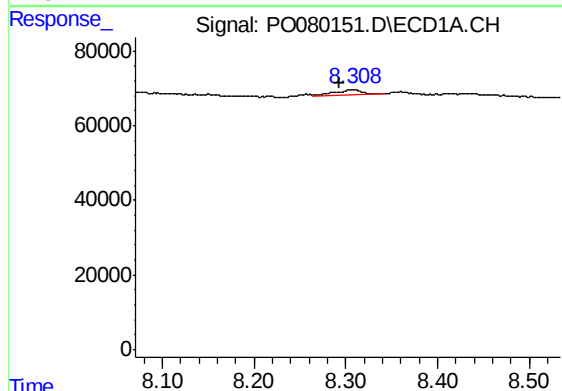

#32 AR-1260-2

R.T.: 8.307 min
Delta R.T.: 0.014 min
Response: 34450
Conc: 11.21 ng/ml

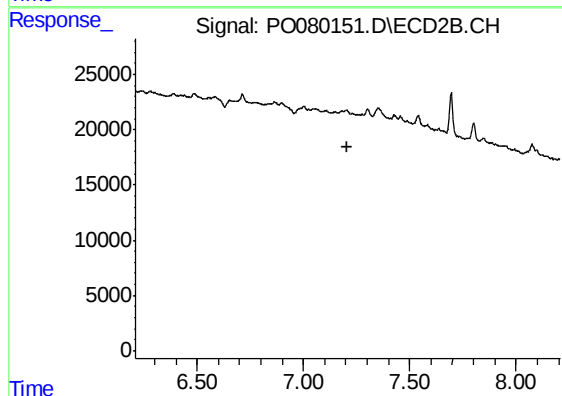

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.