

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080421\
Data File : P0080132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2021 11:55
Operator : DD\AJ
Sample : M3241-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-AMENDED-COM-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:20:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.996	4.115	1283750	451981	21.304	19.736
2)	SA Decachlor...	11.101	9.521	889864	406064	18.970	19.540

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080421\
Data File : P0080132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2021 11:55
Operator : DD\AJ
Sample : M3241-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-AMENDED-COM-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:20:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

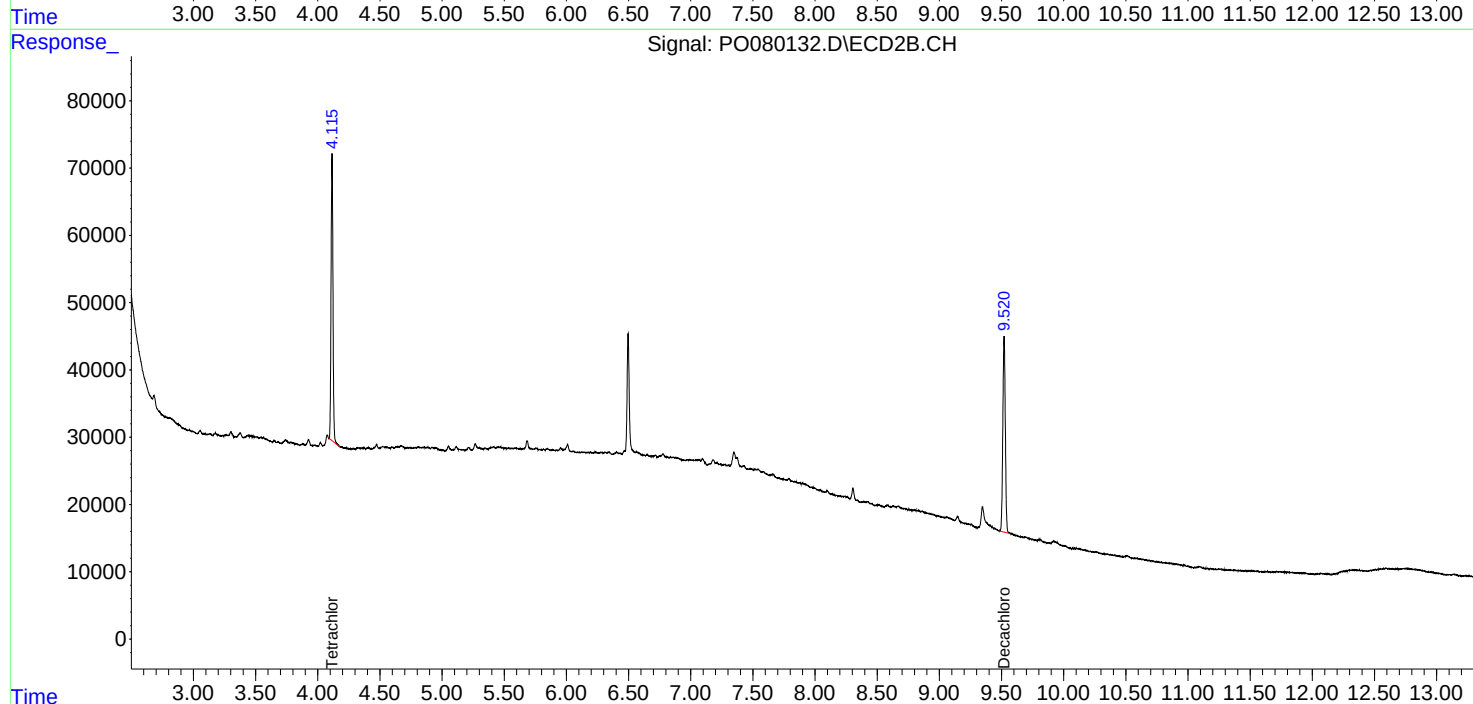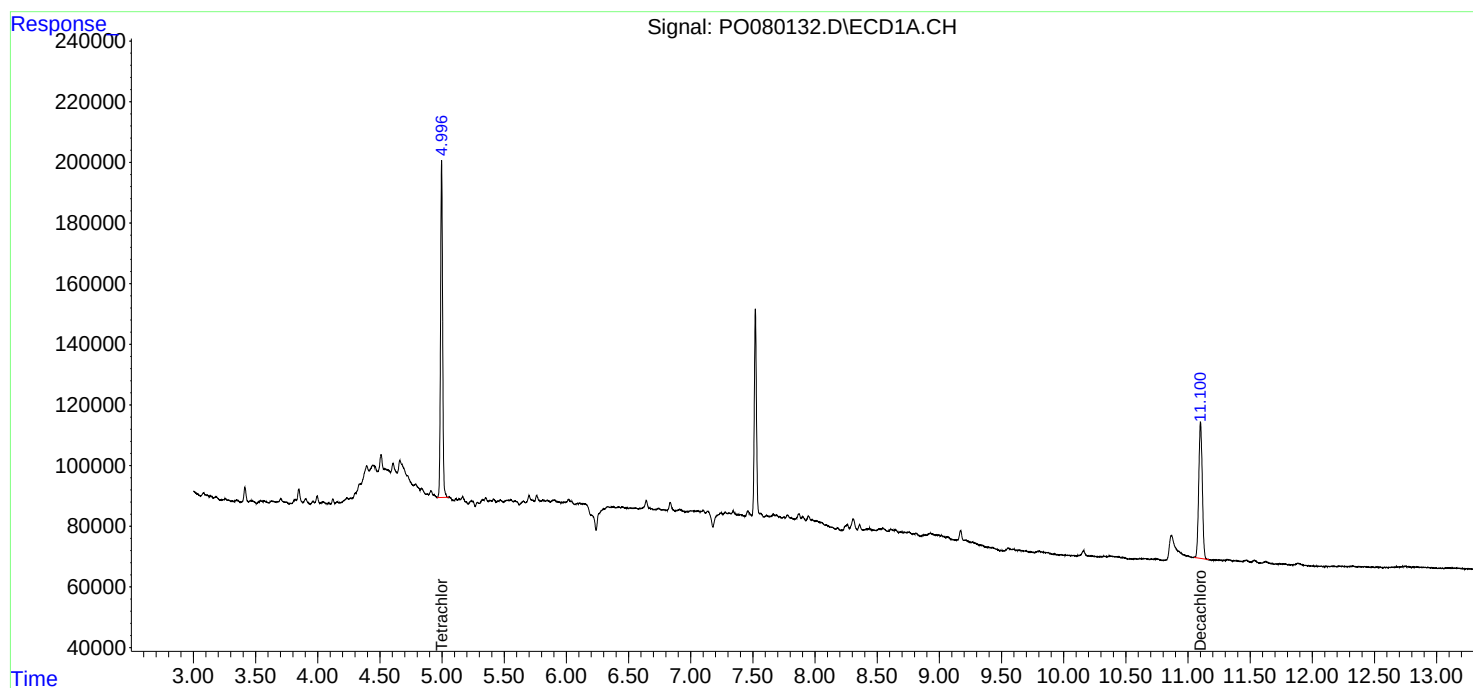


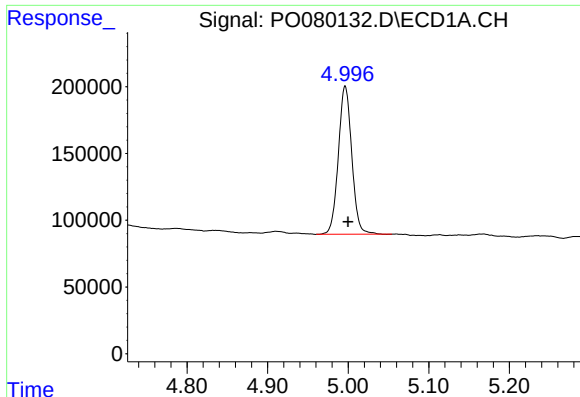

#1 Tetrachloro-m-xylene


R.T.: 4.996 min
Delta R.T.: -0.004 min
Response: 1283750
Conc: 21.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMENDED-COM-6

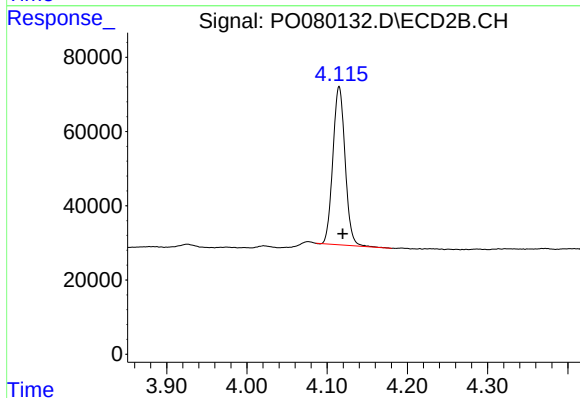


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.004 min
Response: 451981
Conc: 19.74 ng/ml

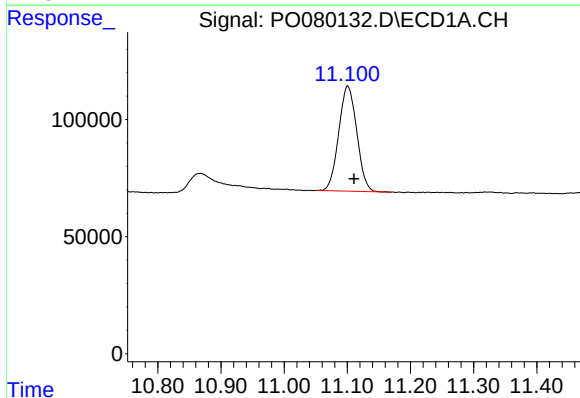

#2 Decachlorobiphenyl

R.T.: 11.101 min
Delta R.T.: -0.010 min
Response: 889864
Conc: 18.97 ng/ml

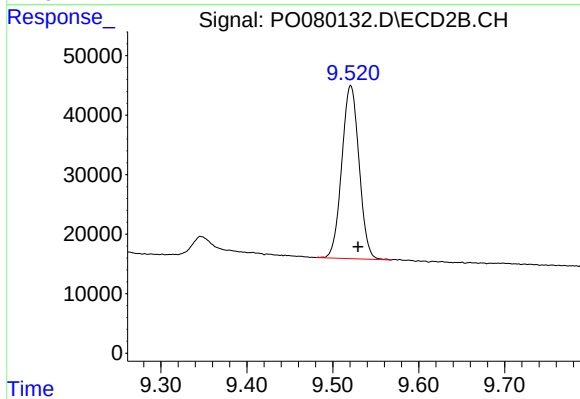

#2 Decachlorobiphenyl

R.T.: 9.521 min
Delta R.T.: -0.008 min
Response: 406064
Conc: 19.54 ng/ml