

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080421\
 Data File : P0080148.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Aug 2021 17:41
 Operator : DD\AJ
 Sample : M3271-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

mohammad
 8/5/2021 12:38:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:30:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.996	4.114	1564391	586304	25.962	25.602
2) SA Decachlor...	11.100	9.520	1030689	460279	21.972	22.148
Target Compounds						
26) L6 AR-1254-1	7.240	6.276	58957	39882	26.990m	29.410
27) L6 AR-1254-2	7.471	6.436	128378	49639	39.095	41.398
28) L6 AR-1254-3	7.854	6.864	193015	133202	56.058	71.190 #
29) L6 AR-1254-4	8.151	7.105	114947	72685	45.194	61.395 #
30) L6 AR-1254-5	8.581	7.541	241372	288950	90.760	180.380 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080421\
Data File : PO080148.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Aug 2021 17:41
Operator : DD\AJ
Sample : M3271-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-3


Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:30:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

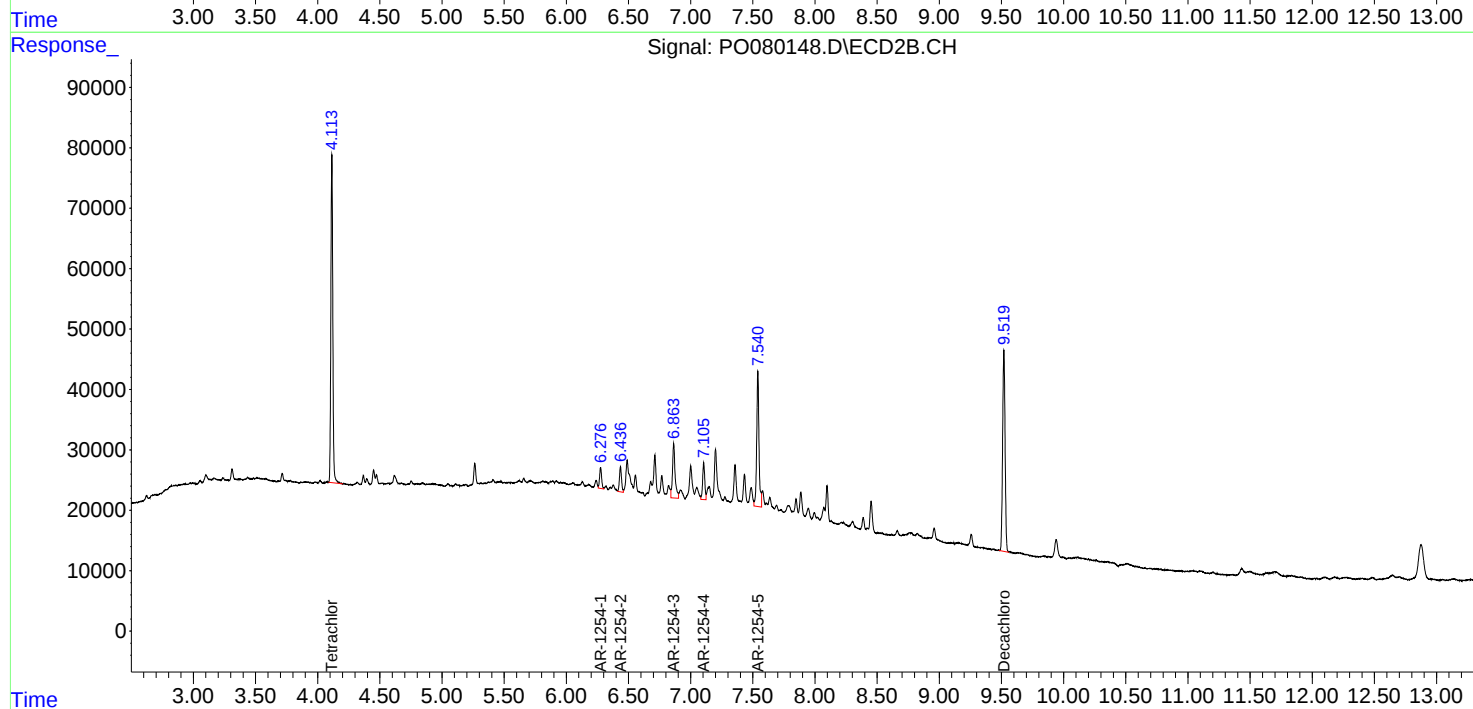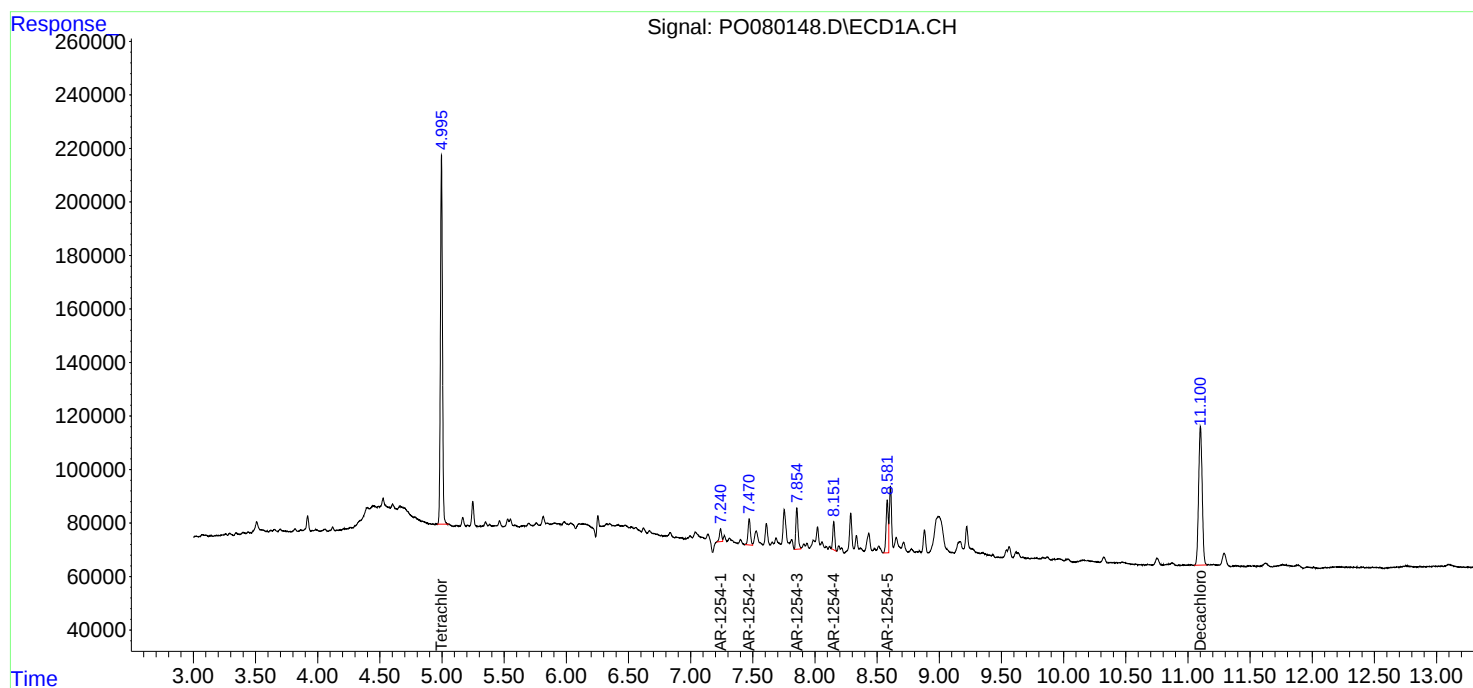

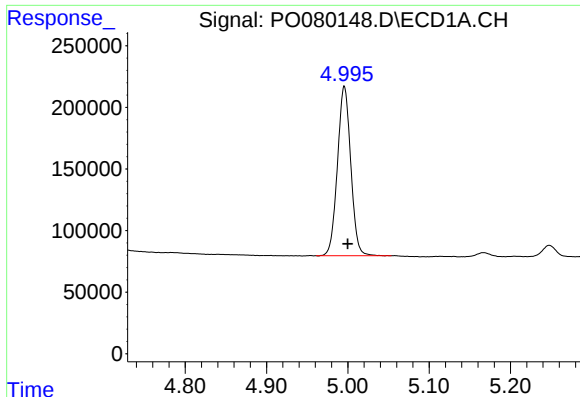


#1 Tetrachloro-m-xylene

R.T.: 4.996 min
Delta R.T.: -0.004 min
Response: 1564391
Conc: 25.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:45 PM

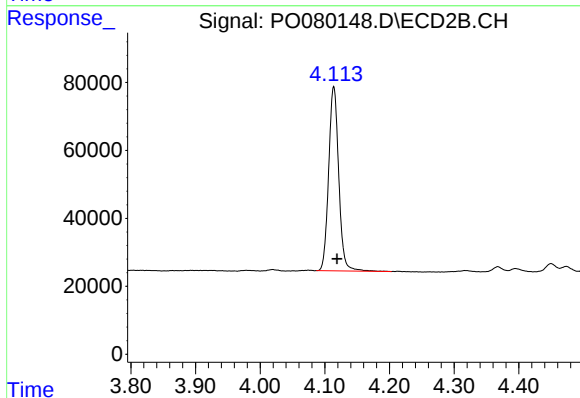


#1 Tetrachloro-m-xylene

R.T.: 4.114 min
Delta R.T.: -0.005 min
Response: 586304
Conc: 25.60 ng/ml

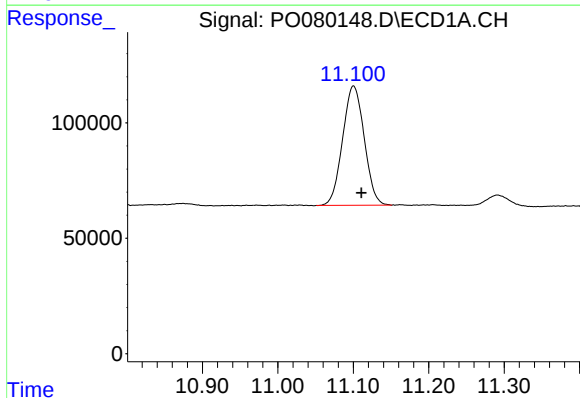


#2 Decachlorobiphenyl

R.T.: 11.100 min
Delta R.T.: -0.010 min
Response: 1030689
Conc: 21.97 ng/ml

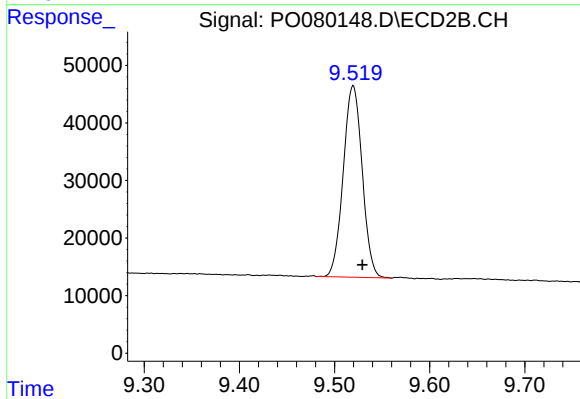

#2 Decachlorobiphenyl

R.T.: 9.520 min
Delta R.T.: -0.010 min
Response: 460279
Conc: 22.15 ng/ml

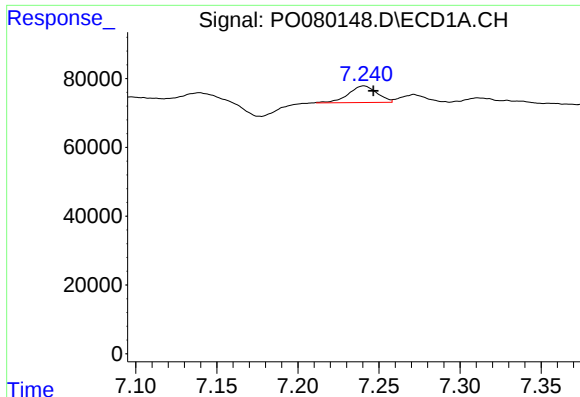


#26 AR-1254-1

R.T.: 7.240 min
Delta R.T.: -0.006 min
Response: 58957
Conc: 26.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:45 PM

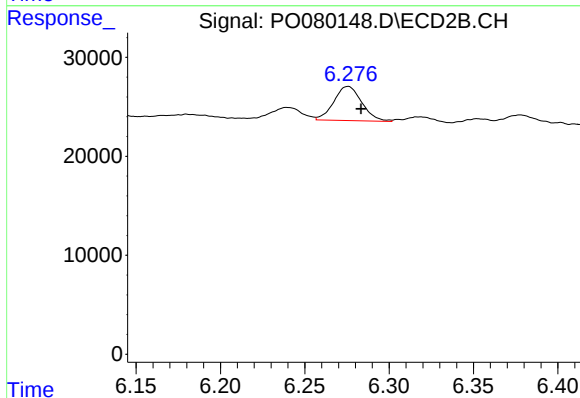


#26 AR-1254-1

R.T.: 6.276 min
Delta R.T.: -0.008 min
Response: 39882
Conc: 29.41 ng/ml

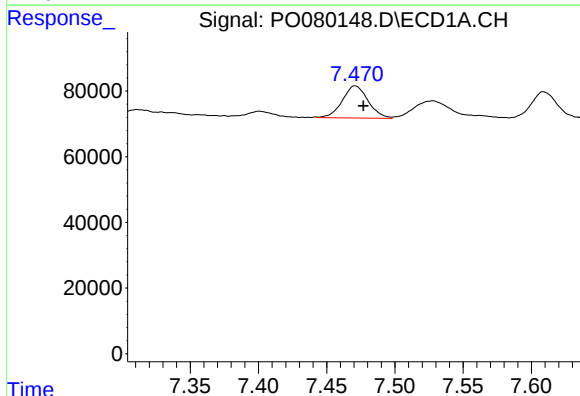


#27 AR-1254-2

R.T.: 7.471 min
Delta R.T.: -0.006 min
Response: 128378
Conc: 39.09 ng/ml

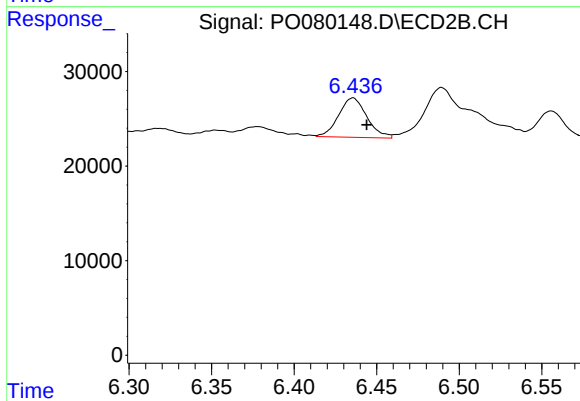

#27 AR-1254-2

R.T.: 6.436 min
Delta R.T.: -0.008 min
Response: 49639
Conc: 41.40 ng/ml

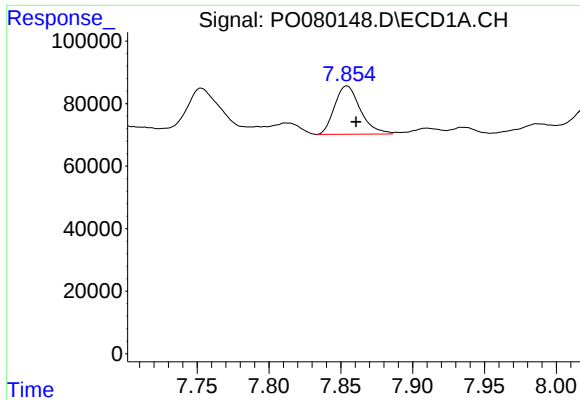


#28 AR-1254-3

R.T.: 7.854 min
Delta R.T.: -0.006 min
Response: 193015
Conc: 56.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:45 PM

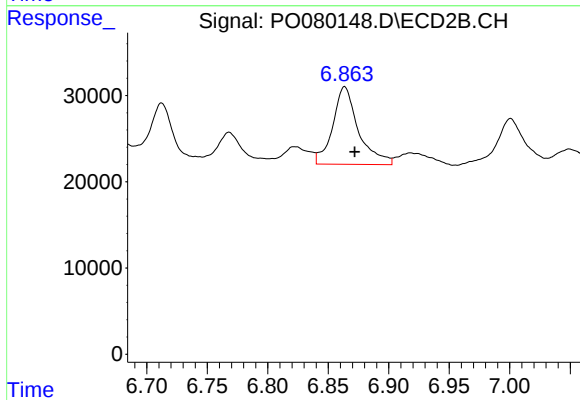


#28 AR-1254-3

R.T.: 6.864 min
Delta R.T.: -0.008 min
Response: 133202
Conc: 71.19 ng/ml

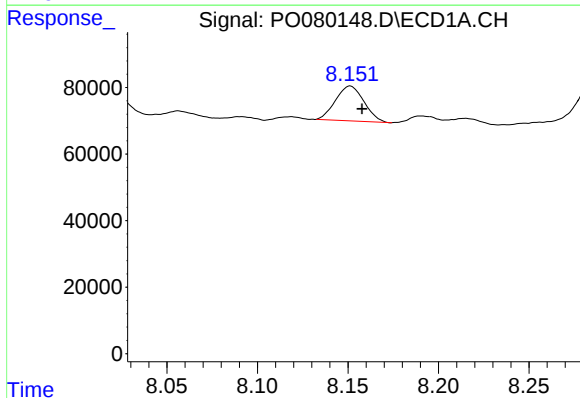


#29 AR-1254-4

R.T.: 8.151 min
Delta R.T.: -0.006 min
Response: 114947
Conc: 45.19 ng/ml

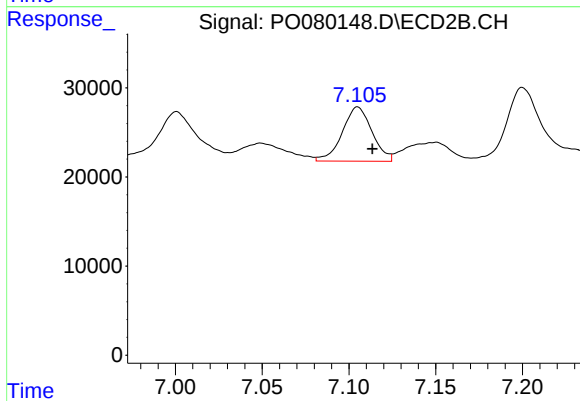

#29 AR-1254-4

R.T.: 7.105 min
Delta R.T.: -0.008 min
Response: 72685
Conc: 61.40 ng/ml

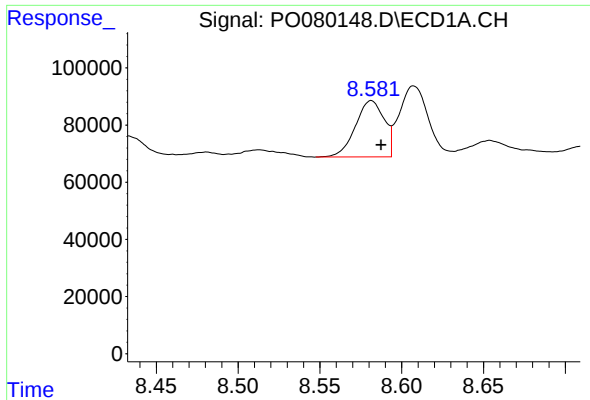


#30 AR-1254-5

R.T.: 8.581 min
Delta R.T.: -0.006 min
Response: 241372
Conc: 90.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3

Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:45 PM

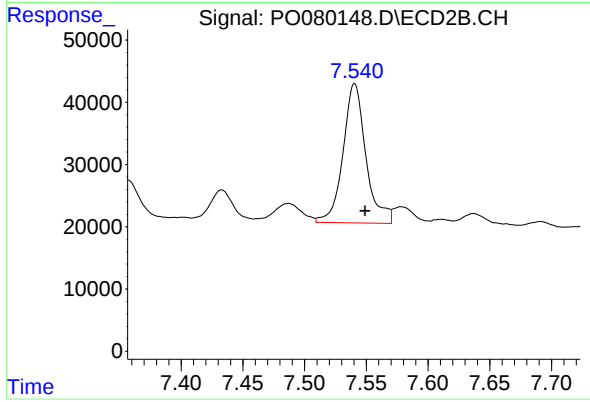

#30 AR-1254-5

R.T.: 7.541 min
Delta R.T.: -0.008 min
Response: 288950
Conc: 180.38 ng/ml