

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080421\
 Data File : P0080174.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2021 1:45
 Operator : DD\AJ
 Sample : M3272-03 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AFL05145-END-1-1

Manual Integrations
 APPROVED

mohammad
 8/5/2021 12:38:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:45:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.997	4.113	94519	45699	1.569	1.995m#
2) SA Decachlor...	11.101	9.519	102315	37574	2.181	1.808

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080421\
Data File : PO080174.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2021 1:45
Operator : DD\AJ
Sample : M3272-03 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AFL05145-END-1-1


Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:45:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

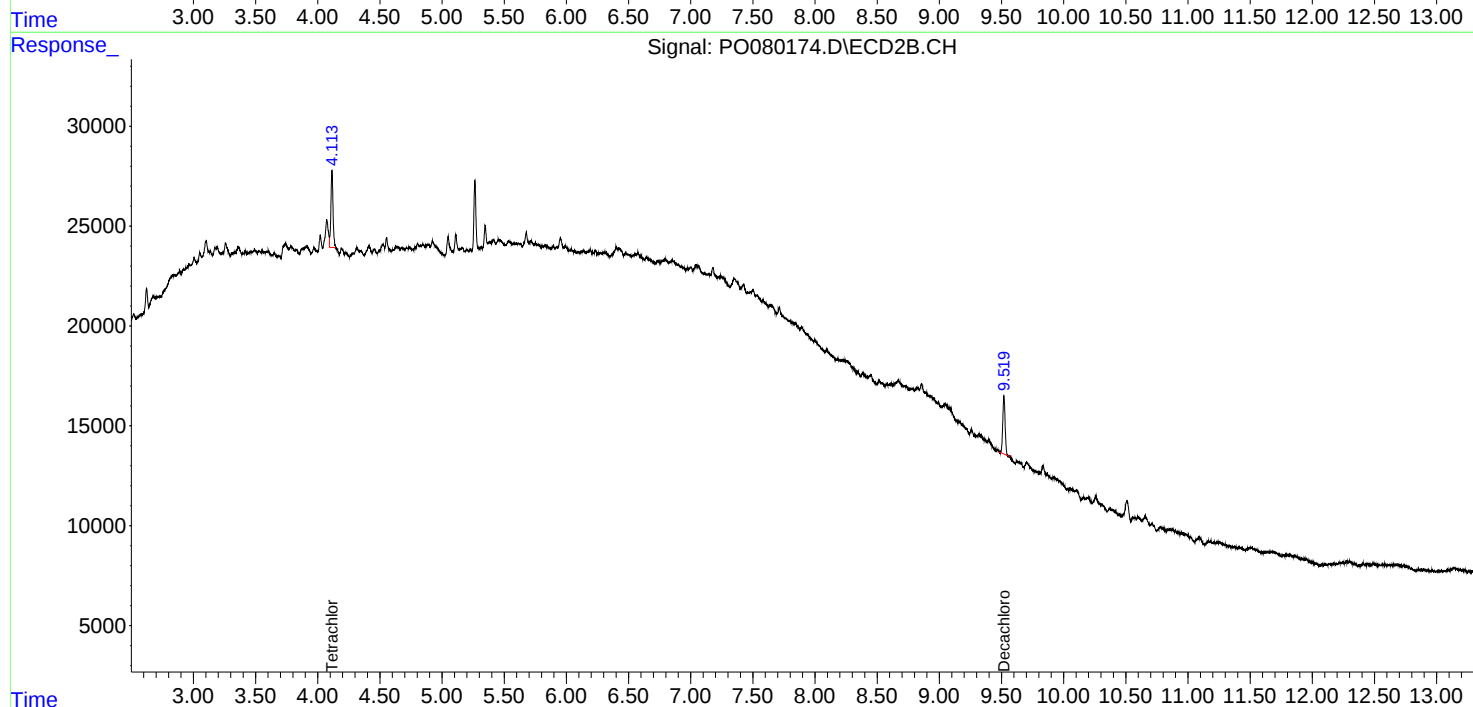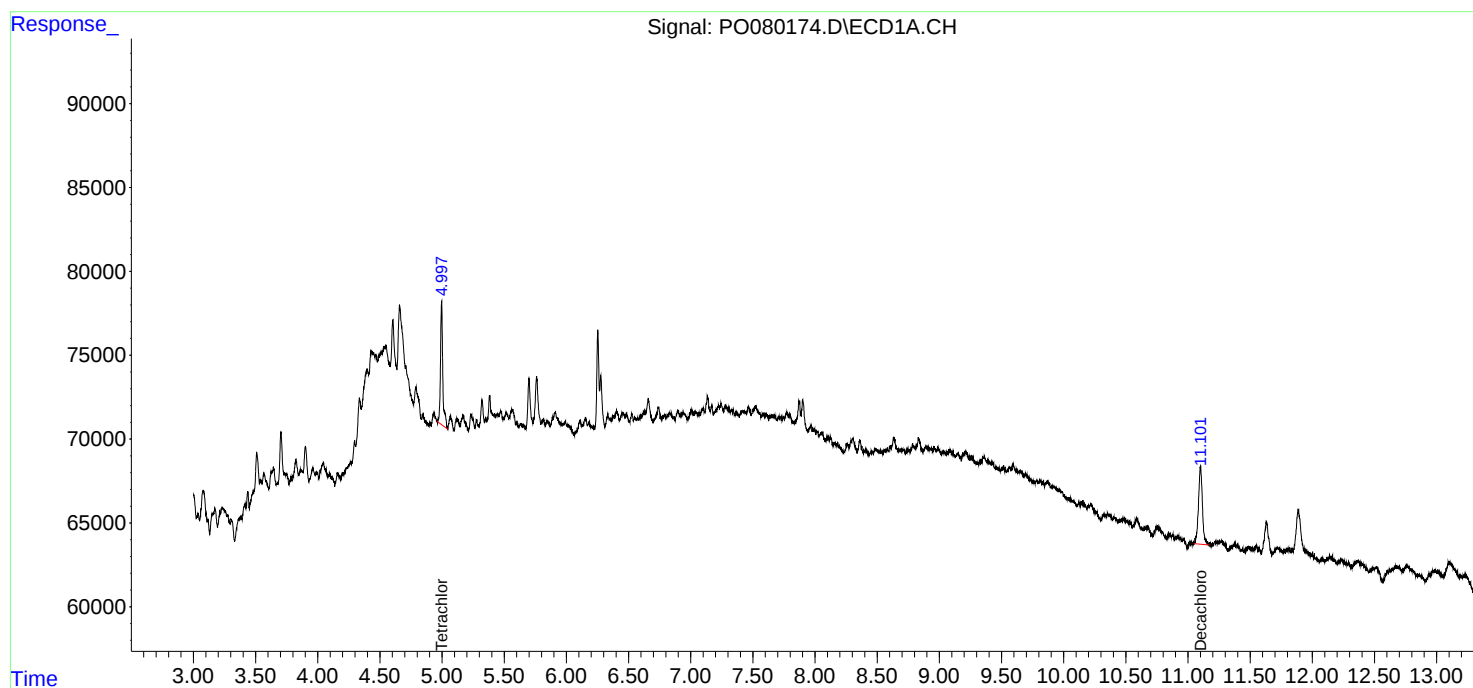

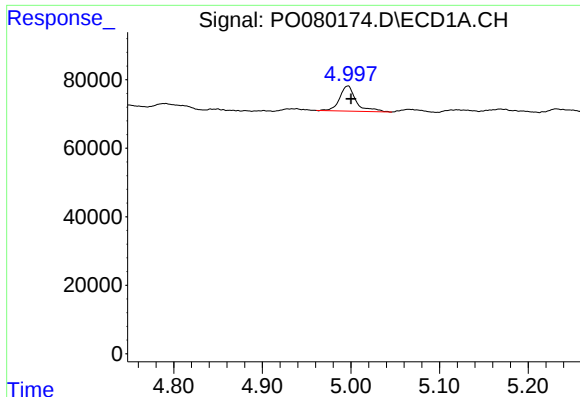


#1 Tetrachloro-m-xylene

R.T.: 4.997 min
Delta R.T.: -0.003 min
Response: 94519
Conc: 1.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
AFL05145-END-1-1


Manual Integrations
APPROVED

mohammad
8/5/2021 12:38:58 PM

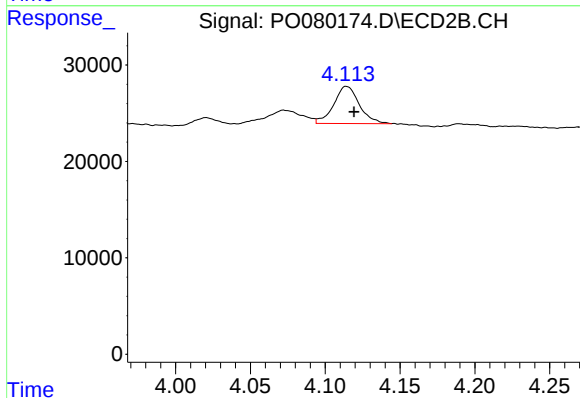


#1 Tetrachloro-m-xylene

R.T.: 4.113 min
Delta R.T.: -0.006 min
Response: 45699
Conc: 2.00 ng/ml m

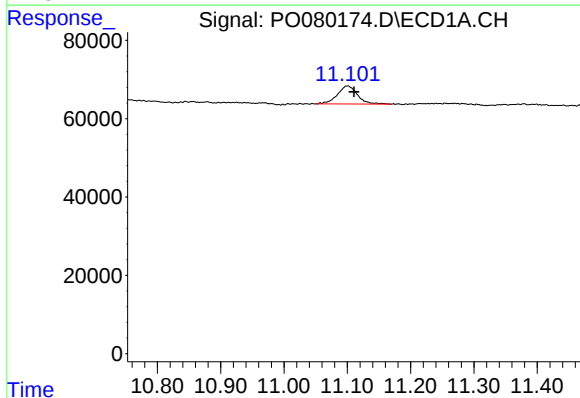

#2 Decachlorobiphenyl

R.T.: 11.101 min
Delta R.T.: -0.010 min
Response: 102315
Conc: 2.18 ng/ml

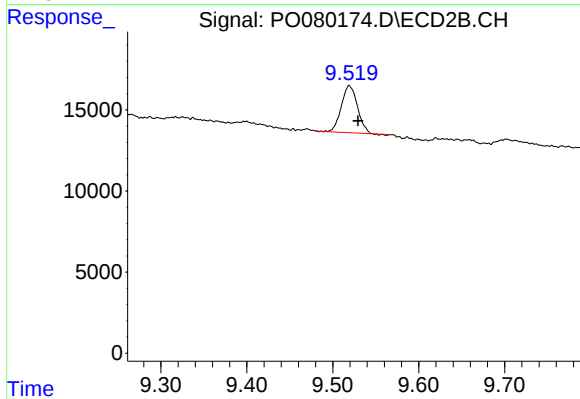

#2 Decachlorobiphenyl

R.T.: 9.519 min
Delta R.T.: -0.010 min
Response: 37574
Conc: 1.81 ng/ml