

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080423\
 Data File : P0096703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2023 17:24
 Operator : YP/AJ
 Sample : 03893-08 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC136902LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/07/2023
 Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:29:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 28 01:38:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.620	4448156	1680452	1.331	1.186m
2) SA Decachlor...	10.309f	8.643	3791671	1767731	1.714m	1.503

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080423\
Data File : PO096703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2023 17:24
Operator : YP/AJ
Sample : 03893-08 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC136902LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:29:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072723.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 28 01:38:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

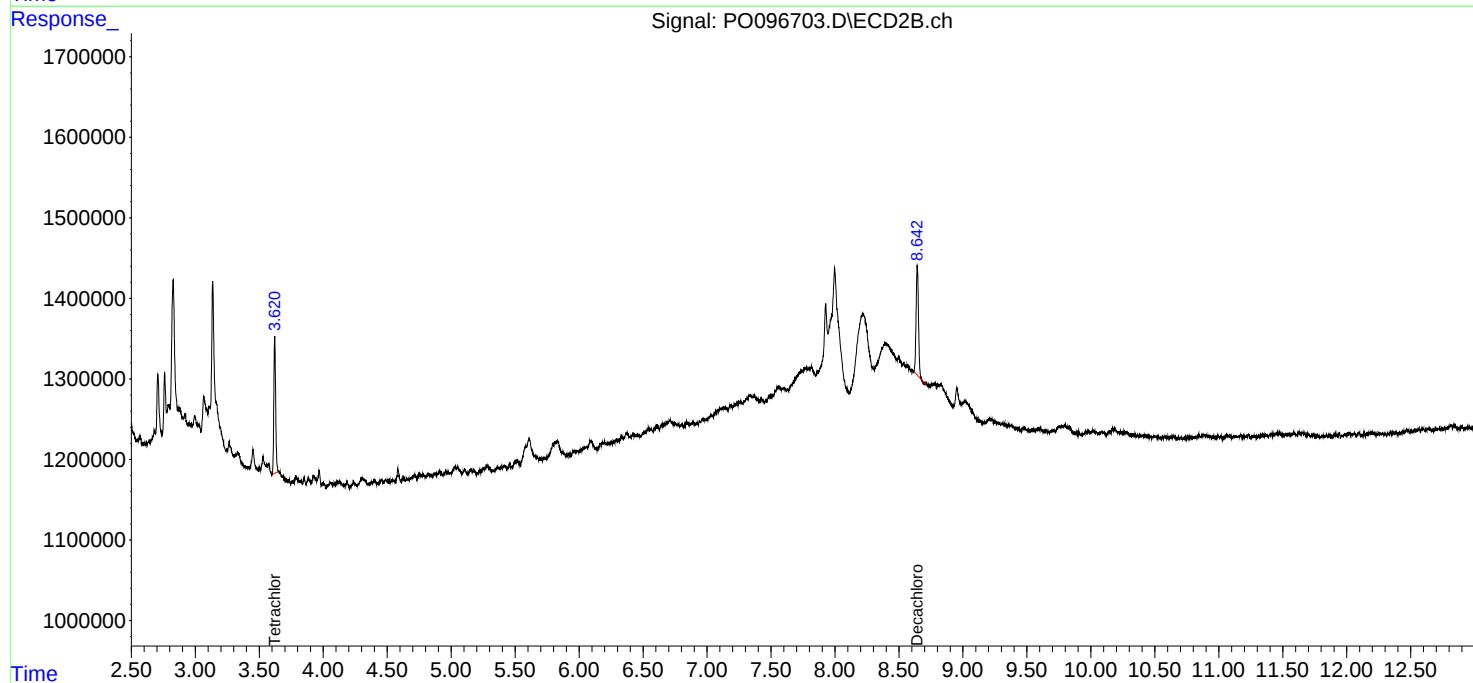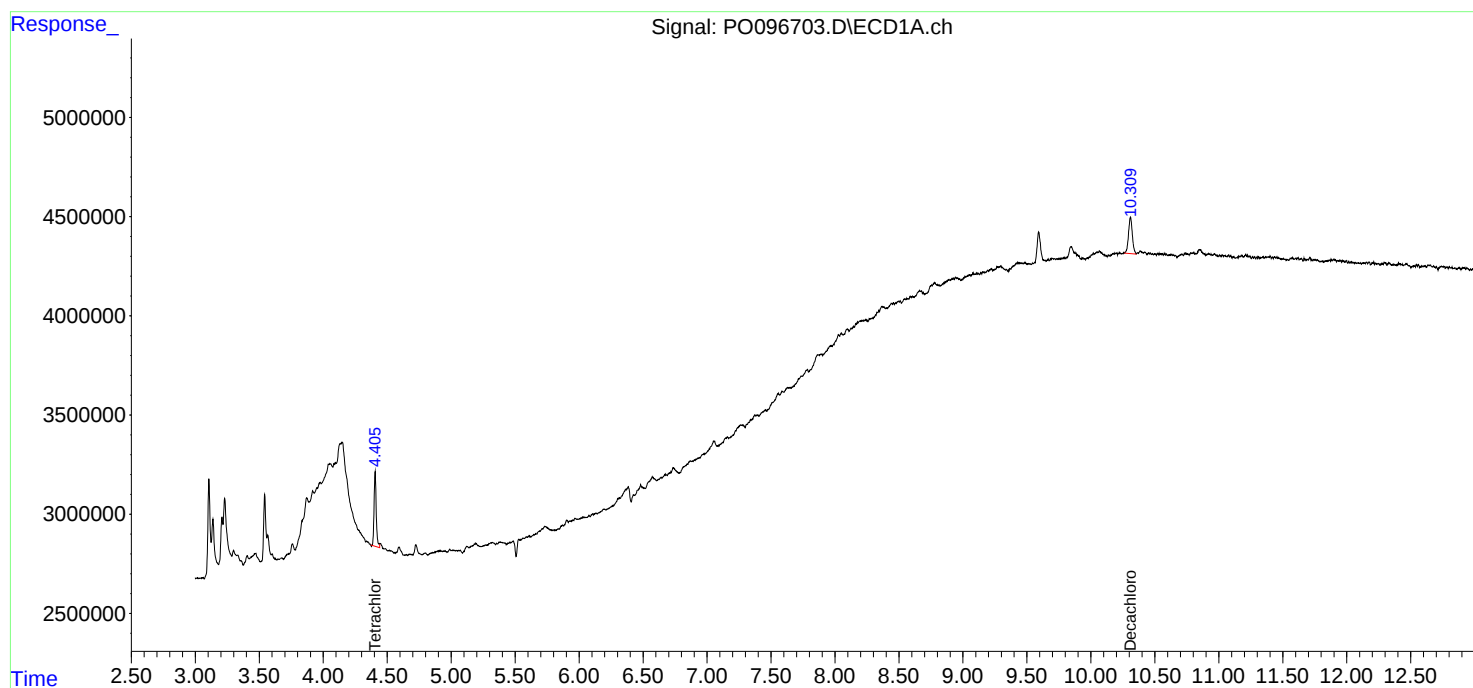

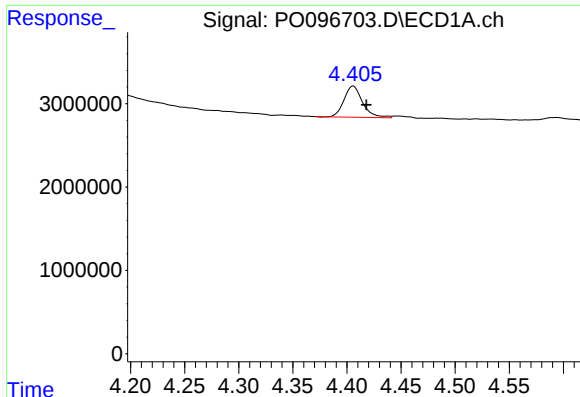


#1 Tetrachloro-m-xylene

R.T.: 4.406 min
Delta R.T.: -0.012 min
Response: 4448156
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC136902LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/07/2023
Supervised By :Ankita Jodhani 08/07/2023

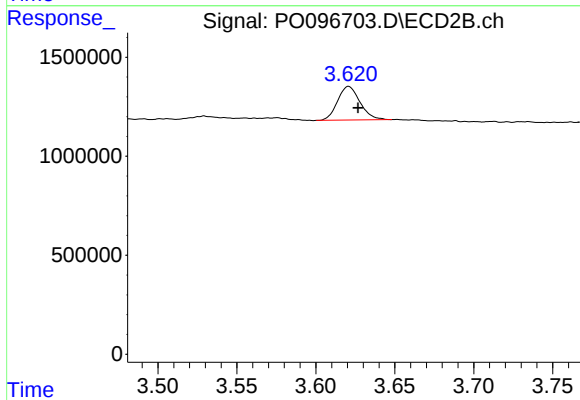


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.006 min
Response: 1680452
Conc: 1.19 ng/ml m

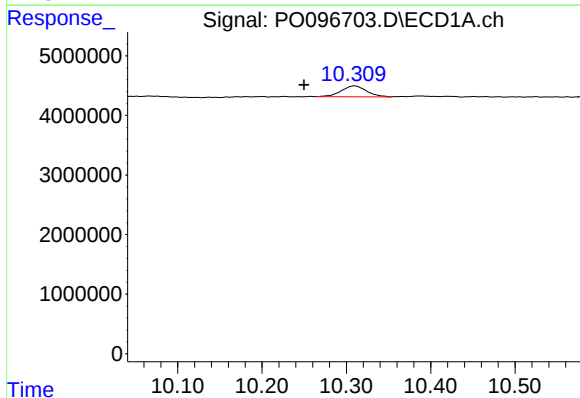

#2 Decachlorobiphenyl

R.T.: 10.309 min
Delta R.T.: 0.059 min
Response: 3791671
Conc: 1.71 ng/ml m

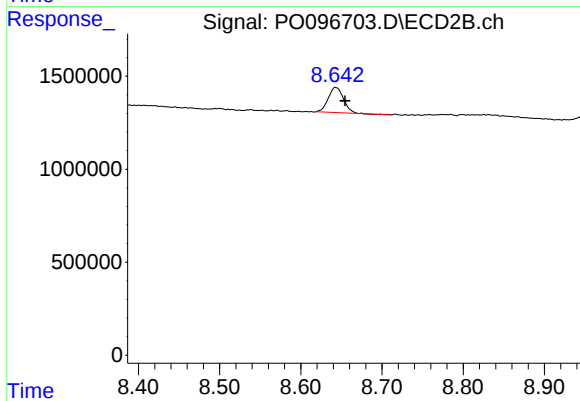

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.012 min
Response: 1767731
Conc: 1.50 ng/ml