

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080425\
 Data File : P0112714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2025 10:21
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 12:18:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.674	3.664	377905	36771	0.046	0.007 #
2)	SA Decachlor...	8.689	8.641	434422	31778	0.059	0.018 #
Target Compounds							
3)	L1 AR-1016-1	4.782	4.737	898553	181769	3.348	1.039 #
4)	L1 AR-1016-2	4.782	4.760	898553	143981	2.213	0.553 #
5)	L1 AR-1016-3	4.864	4.933	1267823	904656	4.845	6.654 #
6)	L1 AR-1016-4	4.956	4.977	3638190	1157698	17.174	10.422 #
7)	L1 AR-1016-5	5.200	5.186	3407505	485159	15.526	3.386 #
8)	L2 AR-1221-1	0.000	3.874	0	69884	N.D.	1.039 #
9)	L2 AR-1221-2	4.025f	3.959	58381	64122	0.812	1.264 #
10)	L2 AR-1221-3	4.025	4.023	58381	100125	0.246	0.632 #
11)	L3 AR-1232-1	4.025	4.023	58381	100125	0.312	0.791 #
12)	L3 AR-1232-2	4.527	4.760	1472816	143981	13.685	1.098 #
13)	L3 AR-1232-3	4.782	4.933	898553	904656	4.345	13.463 #
14)	L3 AR-1232-4	4.956	5.019	3638190	691695	34.735	11.561 #
15)	L3 AR-1232-5	5.013	5.186	5163140	485159	76.062	7.441 #
16)	L4 AR-1242-1	4.782	4.737	898553	181769	3.629	1.148 #
17)	L4 AR-1242-2	4.782	4.760	898553	143981	2.430	0.616 #
18)	L4 AR-1242-3	4.864	4.933	1267823	904656	5.357	7.465 #
19)	L4 AR-1242-4	4.956	5.019	3638190	691695	18.727	5.635 #
20)	L4 AR-1242-5	5.613	5.531	9244770	520943	43.217	3.236 #
21)	L5 AR-1248-1	4.782	4.737	898553	181769	4.800	1.496 #
22)	L5 AR-1248-2	5.013	4.977	5163140	1157698	20.239	6.839 #
23)	L5 AR-1248-3	5.200	5.019	3407505	691695	9.914	3.894 #
24)	L5 AR-1248-4	5.576	5.186	7683857	485159	15.123	2.329 #
25)	L5 AR-1248-5	5.613	5.581	9244770	1036767	26.445	4.827 #
26)	L6 AR-1254-1	5.576	5.531	7683857	520943	13.997	1.585 #
27)	L6 AR-1254-2	5.728	5.670	32738562	535095	67.375	1.848 #
28)	L6 AR-1254-3	6.128	6.074	10058596	642647	13.514	1.503 #
29)	L6 AR-1254-4	6.356	6.302	3399032	395194	6.183	1.448 #
30)	L6 AR-1254-5	6.757	6.721	3424.1E6	1571.2E6	4837.430	4704.010
31)	L7 AR-1260-1	6.248	6.212	170698	559347	0.389	2.251 #
32)	L7 AR-1260-2	6.435	6.400	11805465	6681039	17.162	20.277
33)	L7 AR-1260-3	6.757f	6.592f	3424.1E6	51729	5823.021	0.201 #
34)	L7 AR-1260-4	7.050	7.028	6127111	84352	13.585	0.441 #
35)	L7 AR-1260-5	7.294	7.271	3821836	109874	3.084	0.267 #
36)	L8 AR-1262-1	6.757f	6.721f	3424.1E6	1571.2E6	3684.913	3787.671
37)	L8 AR-1262-2	7.294	7.271	3821836	109874	2.570	0.213 #
38)	L8 AR-1262-3	7.589	7.542	485460	133083	0.822	0.713
39)	L8 AR-1262-4	7.641	7.613	669017	116060	0.673	0.403 #
40)	L8 AR-1262-5	8.146	8.102	160000	126330	0.369	1.270 #
41)	L9 AR-1268-1	7.589	7.542	485460	133083	0.277	0.257

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080425\
Data File : P0112714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2025 10:21
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 12:18:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.641	7.613	669017	116060	0.454	0.273 #
43)	L9 AR-1268-3	7.860	7.818	170928	15247	0.136	0.047 #
44)	L9 AR-1268-4	8.146	8.102	160000	126330	0.332	1.135 #
45)	L9 AR-1268-5	8.439	8.394	163492	61440	0.049	0.084 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080425\
Data File : PO112714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2025 10:21
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 12:18:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

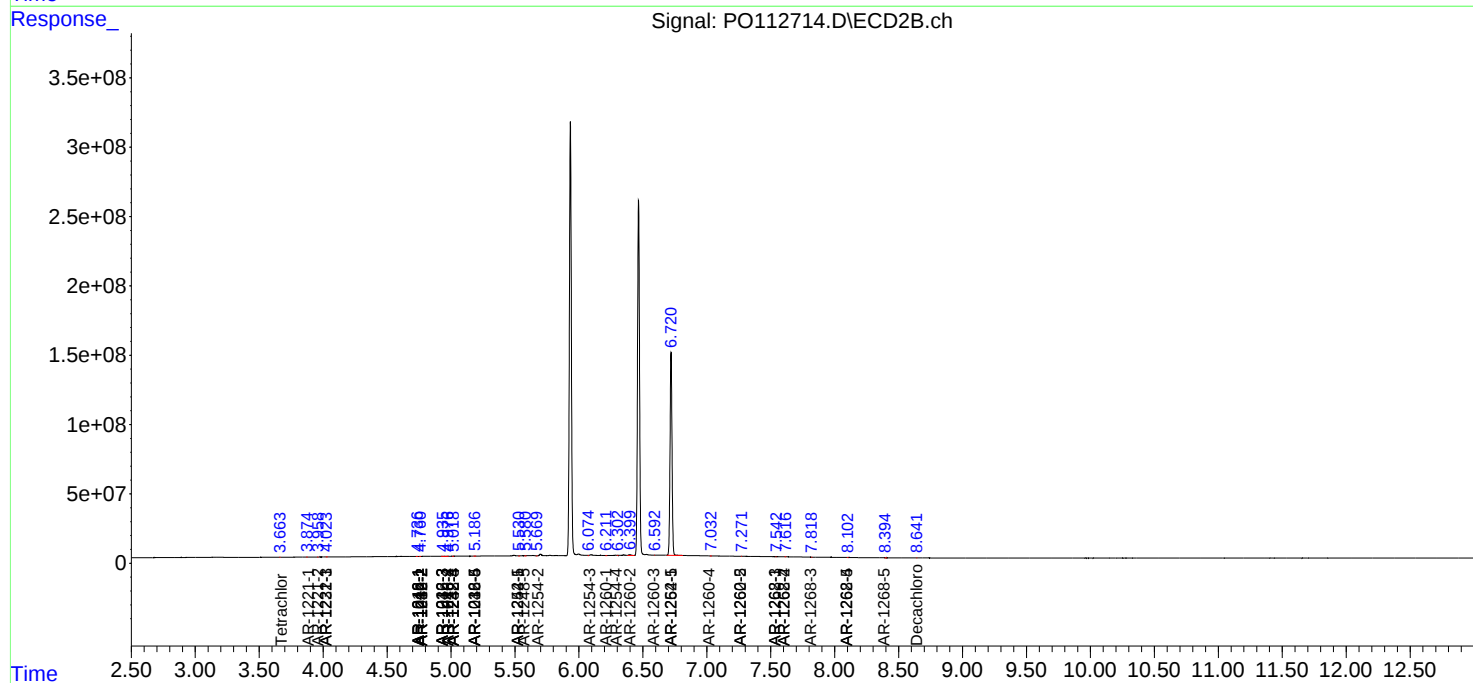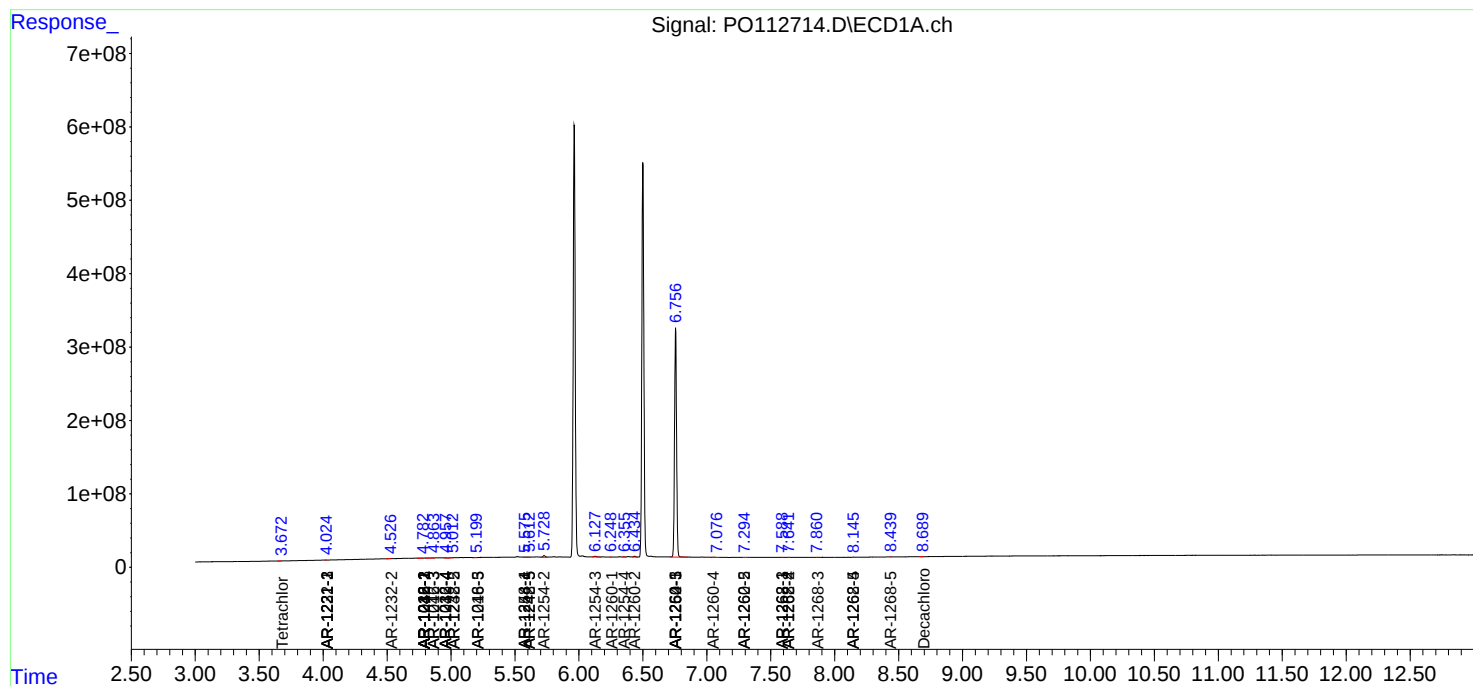


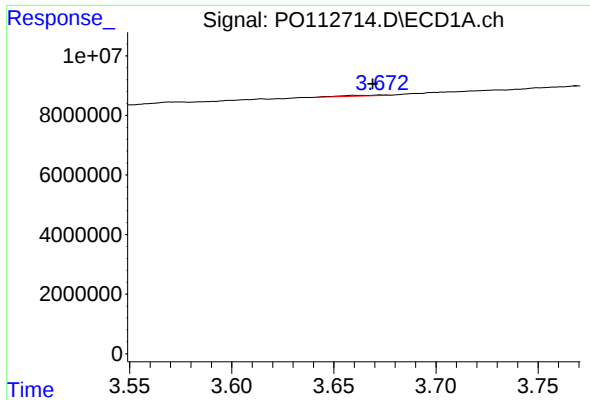

#1 Tetrachloro-m-xylene


R.T.: 3.674 min
Delta R.T.: 0.005 min
Response: 377905
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

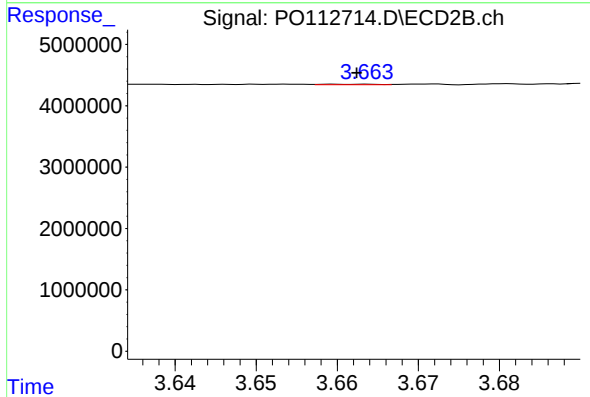


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: 0.001 min
Response: 36771
Conc: 0.01 ng/ml

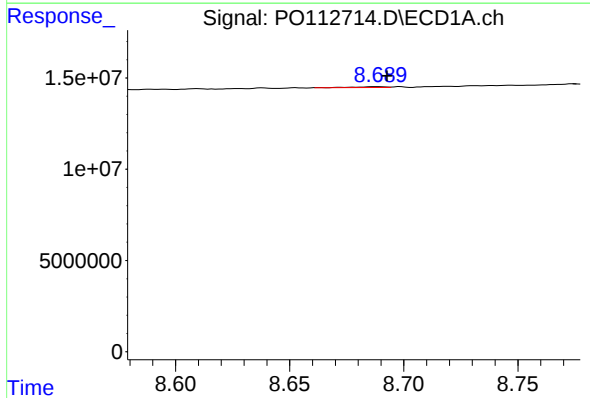


#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.004 min
Response: 434422
Conc: 0.06 ng/ml

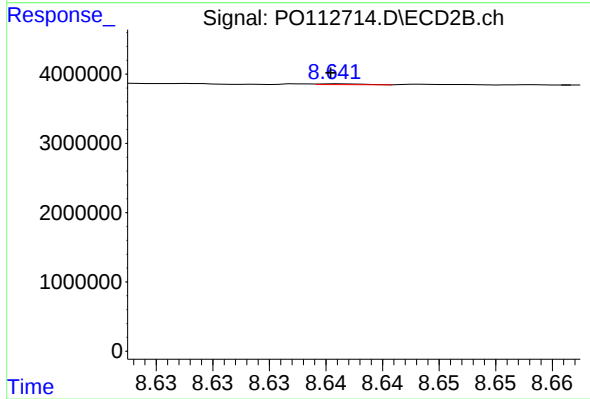

#2 Decachlorobiphenyl


R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 31778
Conc: 0.02 ng/ml

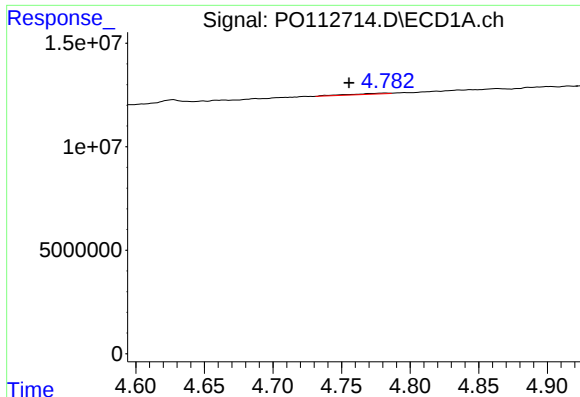

#3 AR-1016-1


R.T.: 4.782 min
Delta R.T.: 0.026 min
Response: 898553
Conc: 3.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

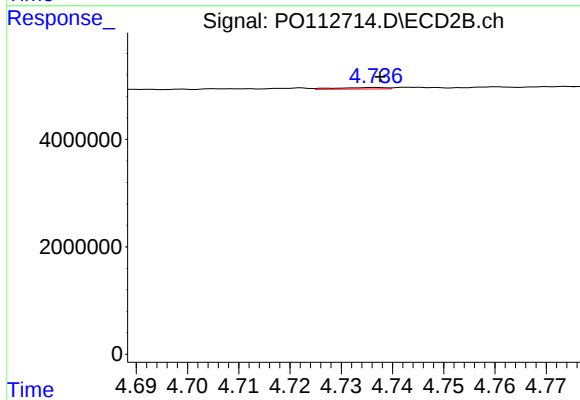


#3 AR-1016-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 181769
Conc: 1.04 ng/ml

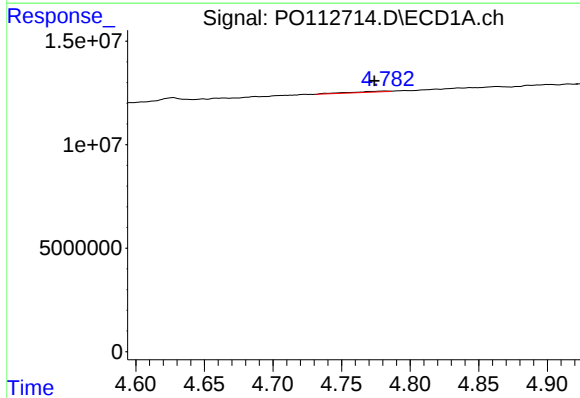


#4 AR-1016-2

R.T.: 4.782 min
Delta R.T.: 0.008 min
Response: 898553
Conc: 2.21 ng/ml

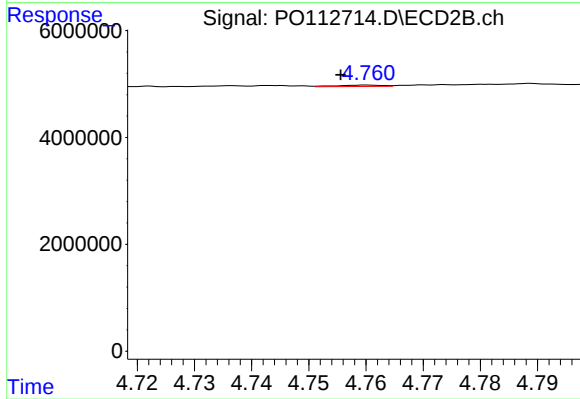

#4 AR-1016-2


R.T.: 4.760 min
Delta R.T.: 0.005 min
Response: 143981
Conc: 0.55 ng/ml

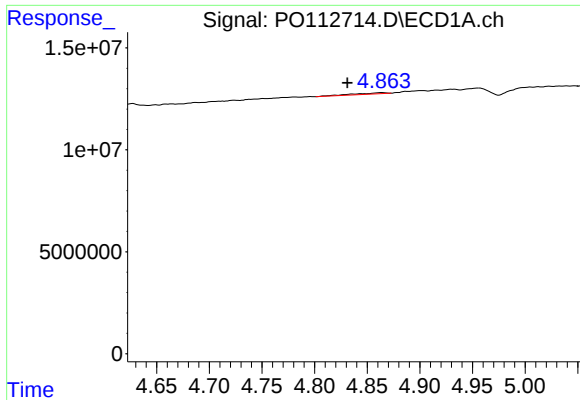

#5 AR-1016-3


R.T.: 4.864 min
Delta R.T.: 0.032 min
Response: 1267823
Conc: 4.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

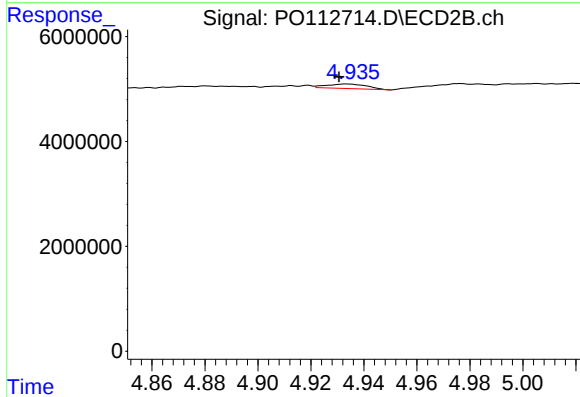


#5 AR-1016-3

R.T.: 4.933 min
Delta R.T.: 0.003 min
Response: 904656
Conc: 6.65 ng/ml

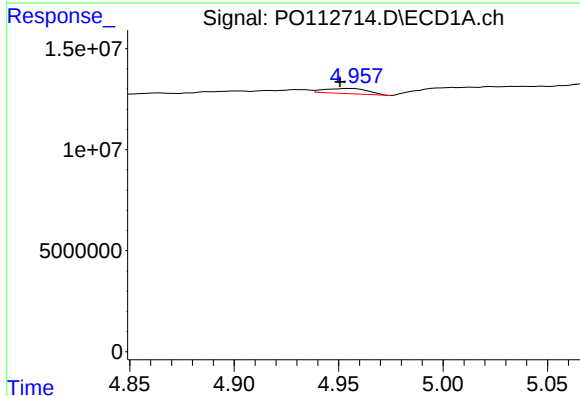


#6 AR-1016-4

R.T.: 4.956 min
Delta R.T.: 0.006 min
Response: 3638190
Conc: 17.17 ng/ml

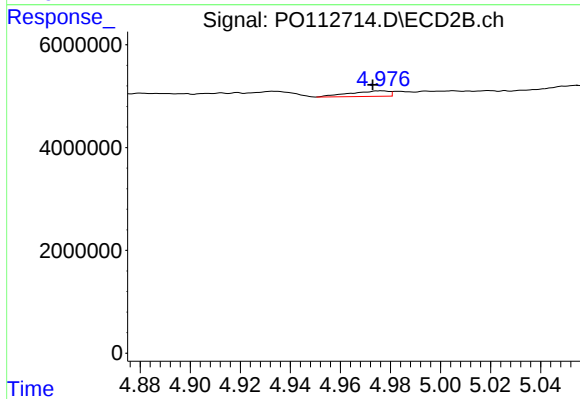

#6 AR-1016-4


R.T.: 4.977 min
Delta R.T.: 0.004 min
Response: 1157698
Conc: 10.42 ng/ml

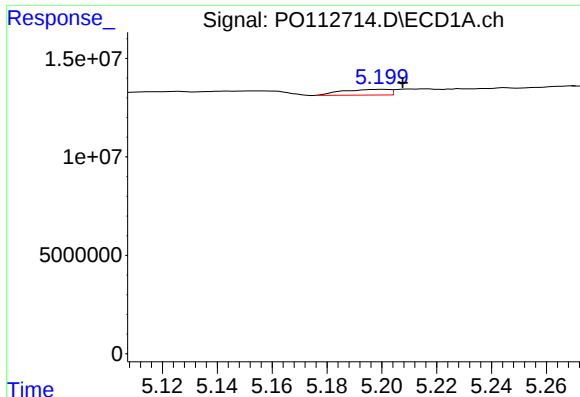

#7 AR-1016-5


R.T.: 5.200 min
Delta R.T.: -0.008 min
Response: 3407505
Conc: 15.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

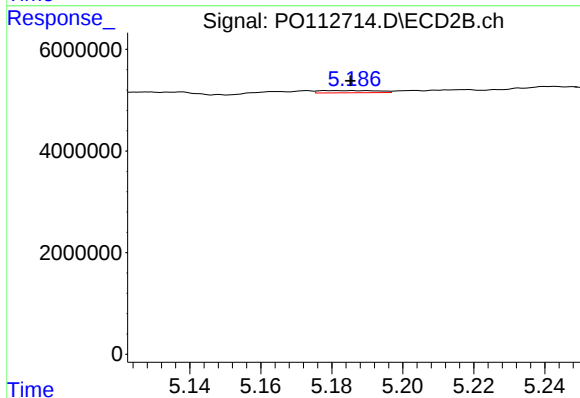


#7 AR-1016-5

R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 485159
Conc: 3.39 ng/ml

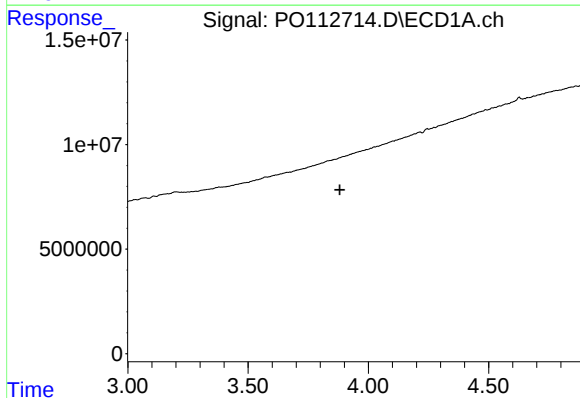


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.882 min
Response: 0
Conc: N.D.

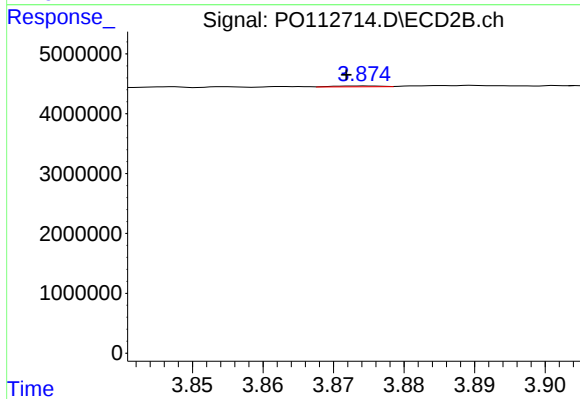

#8 AR-1221-1


R.T.: 3.874 min
Delta R.T.: 0.002 min
Response: 69884
Conc: 1.04 ng/ml

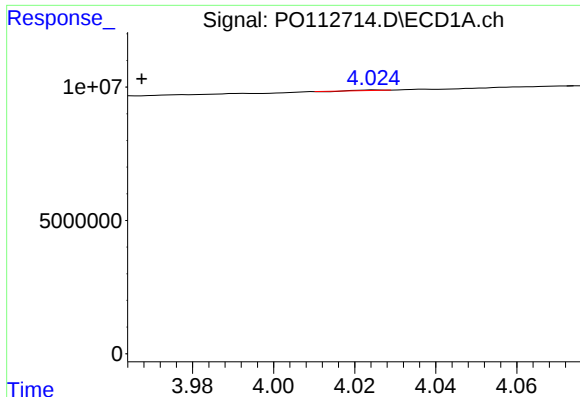

#9 AR-1221-2


R.T.: 4.025 min
Delta R.T.: 0.058 min
Response: 58381
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

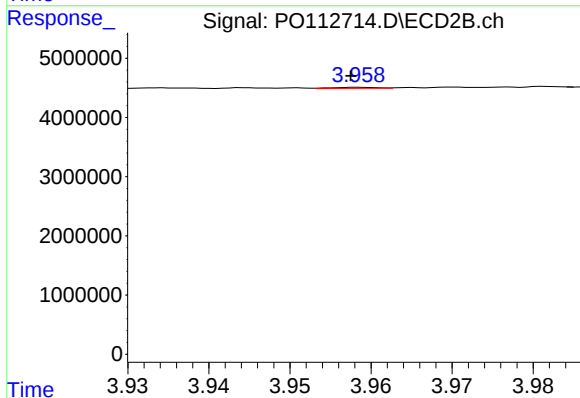


#9 AR-1221-2

R.T.: 3.959 min
Delta R.T.: 0.001 min
Response: 64122
Conc: 1.26 ng/ml

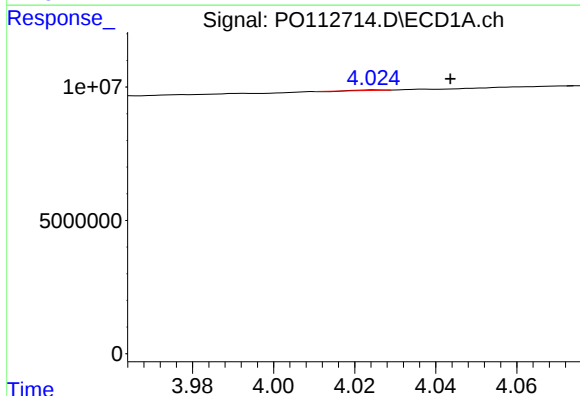


#10 AR-1221-3

R.T.: 4.025 min
Delta R.T.: -0.018 min
Response: 58381
Conc: 0.25 ng/ml

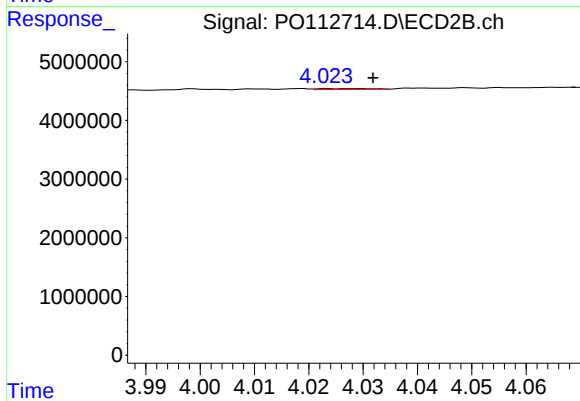

#10 AR-1221-3


R.T.: 4.023 min
Delta R.T.: -0.008 min
Response: 100125
Conc: 0.63 ng/ml

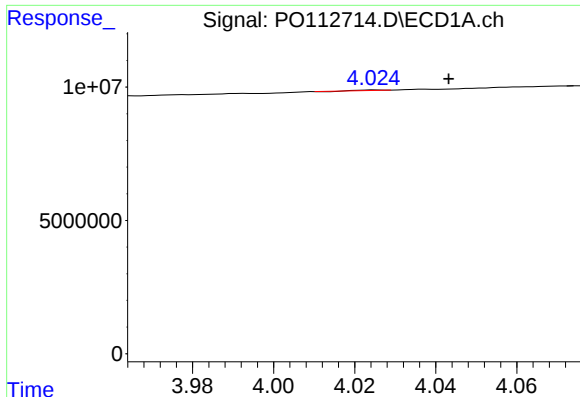

#11 AR-1232-1


R.T.: 4.025 min
Delta R.T.: -0.018 min
Response: 58381
Conc: 0.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

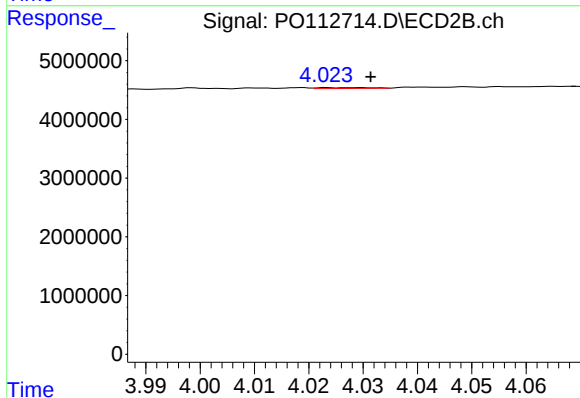


#11 AR-1232-1

R.T.: 4.023 min
Delta R.T.: -0.008 min
Response: 100125
Conc: 0.79 ng/ml

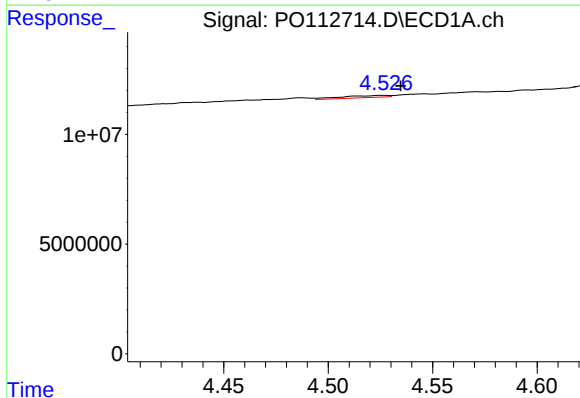


#12 AR-1232-2

R.T.: 4.527 min
Delta R.T.: -0.008 min
Response: 1472816
Conc: 13.68 ng/ml

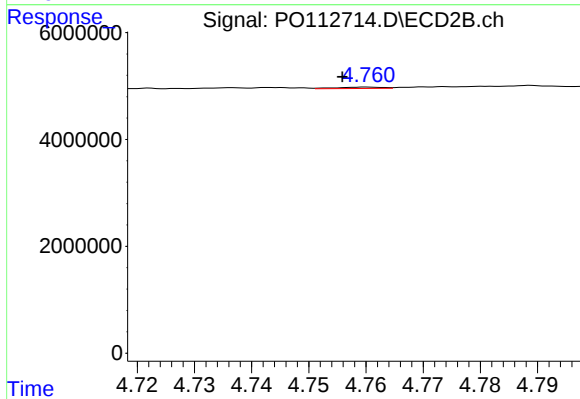

#12 AR-1232-2


R.T.: 4.760 min
Delta R.T.: 0.005 min
Response: 143981
Conc: 1.10 ng/ml

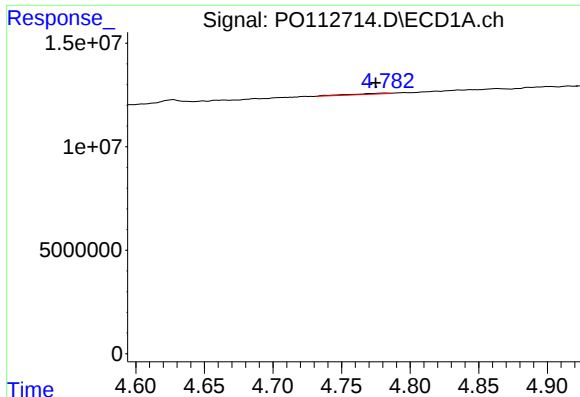

#13 AR-1232-3


R.T.: 4.782 min
Delta R.T.: 0.007 min
Response: 898553
Conc: 4.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

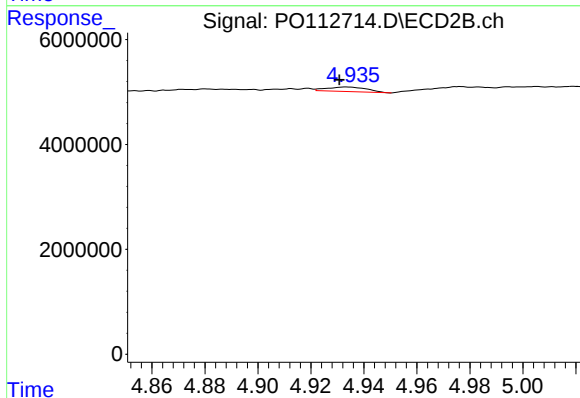


#13 AR-1232-3

R.T.: 4.933 min
Delta R.T.: 0.003 min
Response: 904656
Conc: 13.46 ng/ml

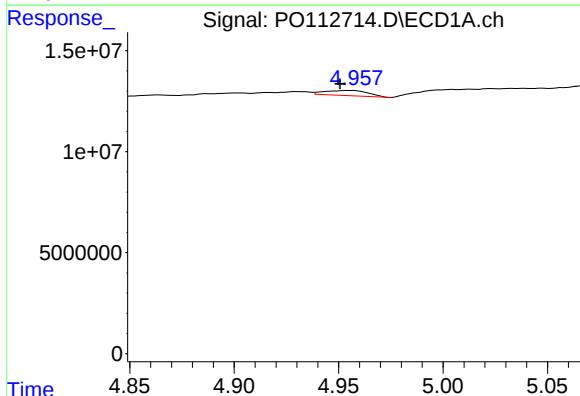


#14 AR-1232-4

R.T.: 4.956 min
Delta R.T.: 0.005 min
Response: 3638190
Conc: 34.74 ng/ml

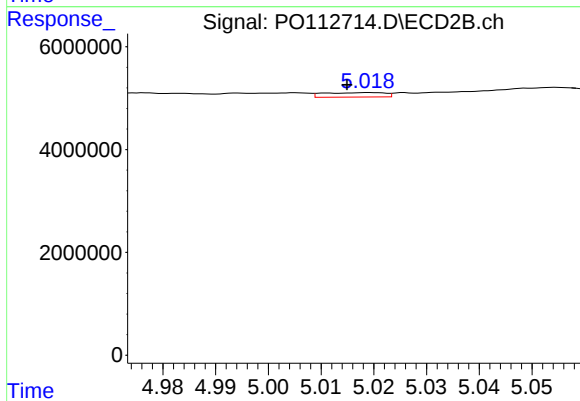

#14 AR-1232-4


R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 691695
Conc: 11.56 ng/ml

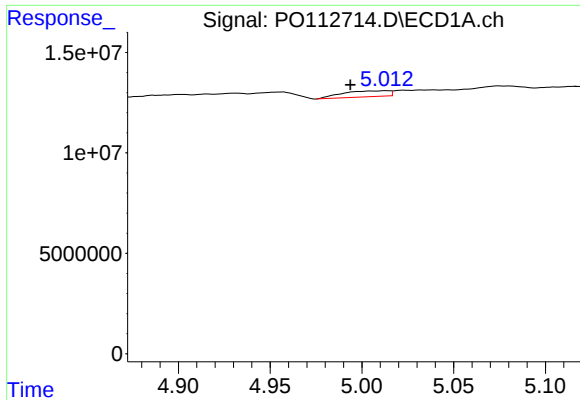

#15 AR-1232-5


R.T.: 5.013 min
Delta R.T.: 0.019 min
Response: 5163140
Conc: 76.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

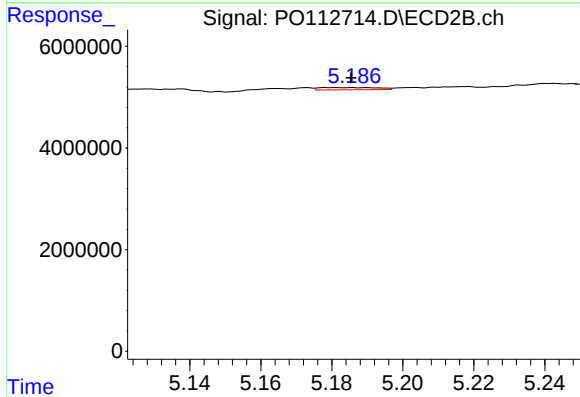


#15 AR-1232-5

R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 485159
Conc: 7.44 ng/ml

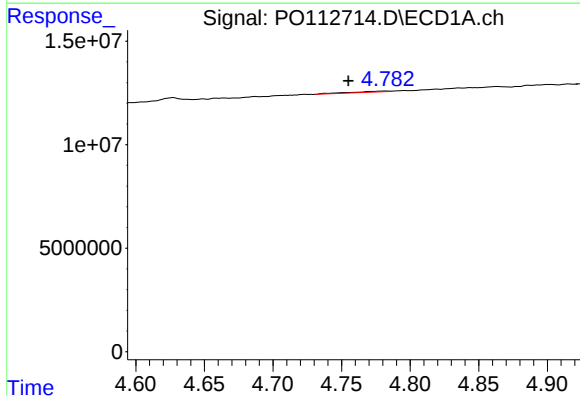


#16 AR-1242-1

R.T.: 4.782 min
Delta R.T.: 0.027 min
Response: 898553
Conc: 3.63 ng/ml

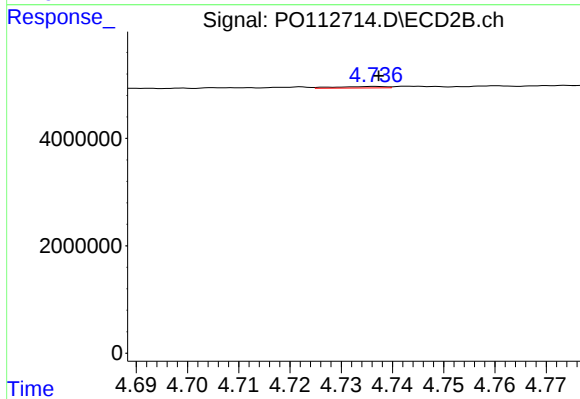

#16 AR-1242-1


R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 181769
Conc: 1.15 ng/ml

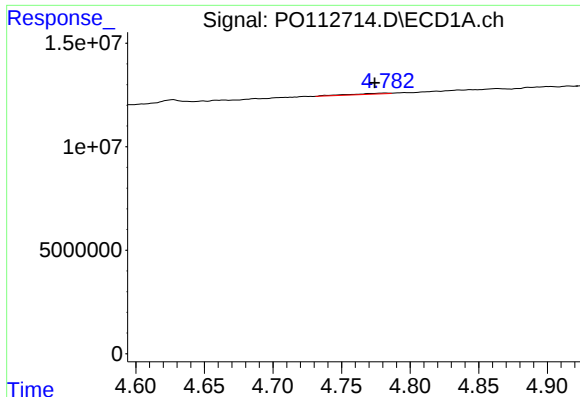

#17 AR-1242-2


R.T.: 4.782 min
Delta R.T.: 0.008 min
Response: 898553
Conc: 2.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

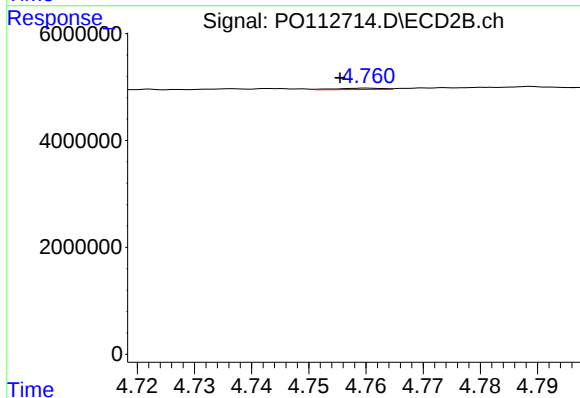


#17 AR-1242-2

R.T.: 4.760 min
Delta R.T.: 0.005 min
Response: 143981
Conc: 0.62 ng/ml

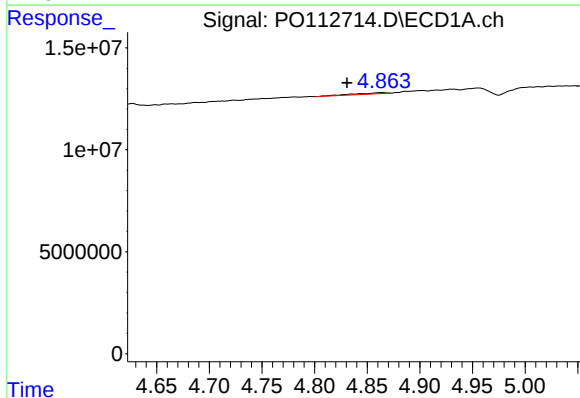


#18 AR-1242-3

R.T.: 4.864 min
Delta R.T.: 0.033 min
Response: 1267823
Conc: 5.36 ng/ml

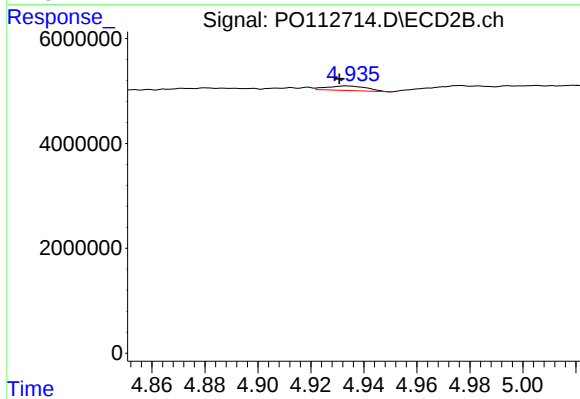

#18 AR-1242-3


R.T.: 4.933 min
Delta R.T.: 0.003 min
Response: 904656
Conc: 7.46 ng/ml

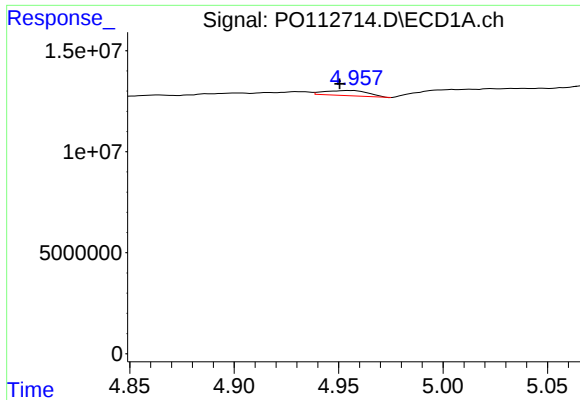

#19 AR-1242-4


R.T.: 4.956 min
Delta R.T.: 0.006 min
Response: 3638190
Conc: 18.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

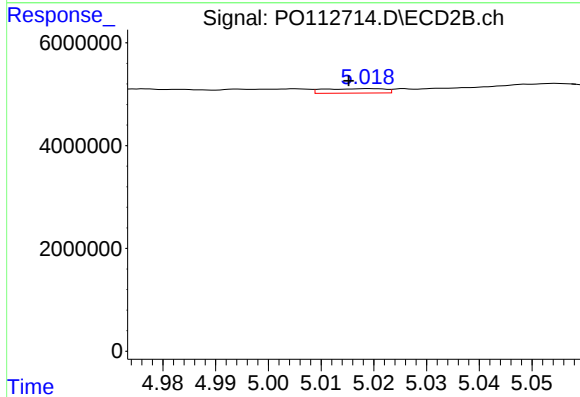


#19 AR-1242-4

R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 691695
Conc: 5.64 ng/ml

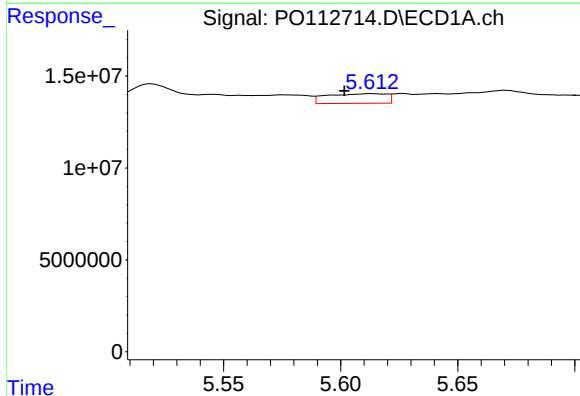


#20 AR-1242-5

R.T.: 5.613 min
Delta R.T.: 0.012 min
Response: 9244770
Conc: 43.22 ng/ml

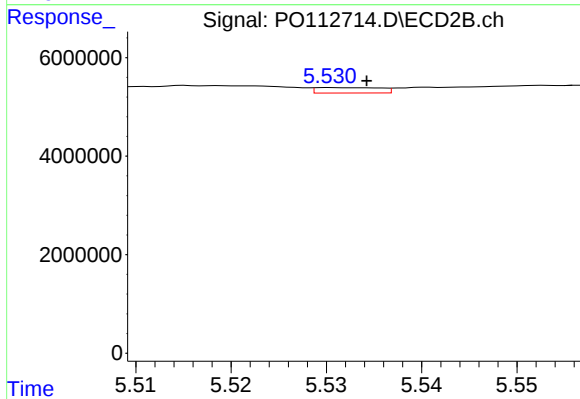

#20 AR-1242-5


R.T.: 5.531 min
Delta R.T.: -0.004 min
Response: 520943
Conc: 3.24 ng/ml

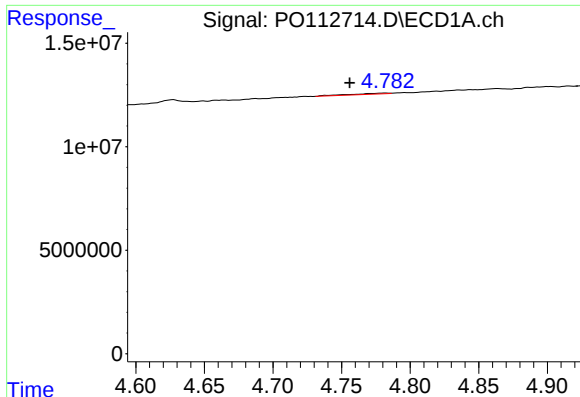

#21 AR-1248-1


R.T.: 4.782 min
Delta R.T.: 0.026 min
Response: 898553
Conc: 4.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

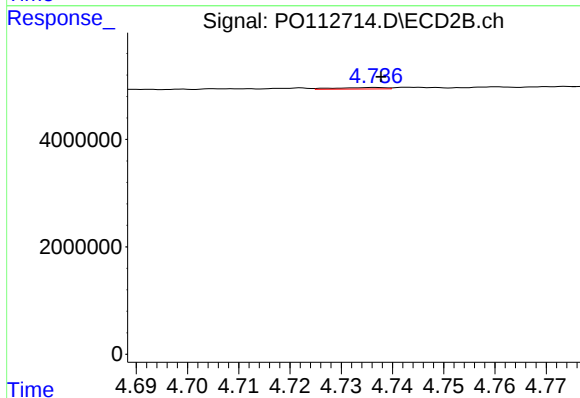


#21 AR-1248-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 181769
Conc: 1.50 ng/ml

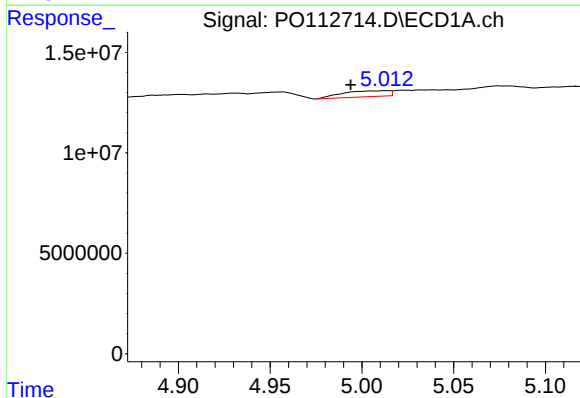


#22 AR-1248-2

R.T.: 5.013 min
Delta R.T.: 0.019 min
Response: 5163140
Conc: 20.24 ng/ml

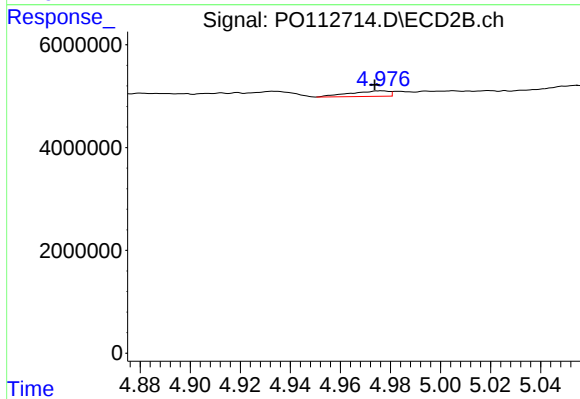

#22 AR-1248-2


R.T.: 4.977 min
Delta R.T.: 0.003 min
Response: 1157698
Conc: 6.84 ng/ml

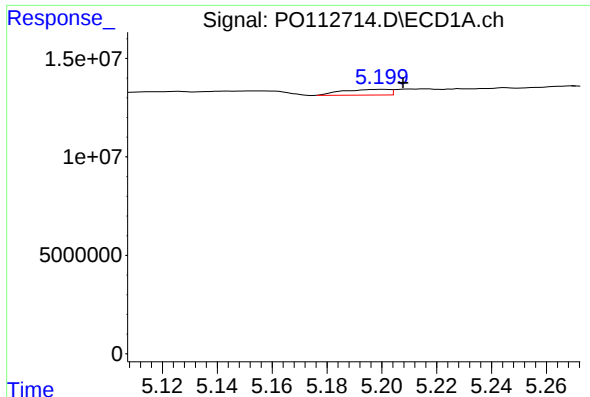

#23 AR-1248-3


R.T.: 5.200 min
Delta R.T.: -0.008 min
Response: 3407505
Conc: 9.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

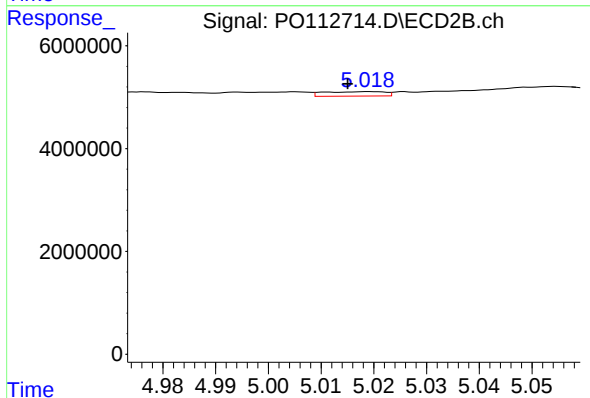


#23 AR-1248-3

R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 691695
Conc: 3.89 ng/ml

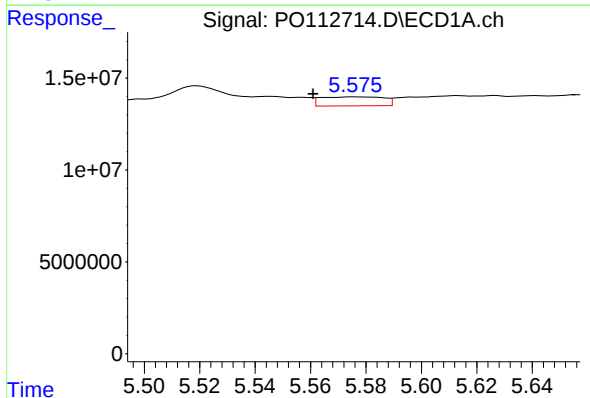


#24 AR-1248-4

R.T.: 5.576 min
Delta R.T.: 0.015 min
Response: 7683857
Conc: 15.12 ng/ml

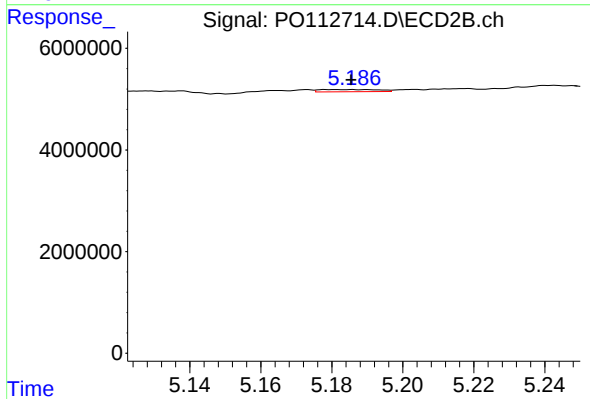

#24 AR-1248-4


R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 485159
Conc: 2.33 ng/ml

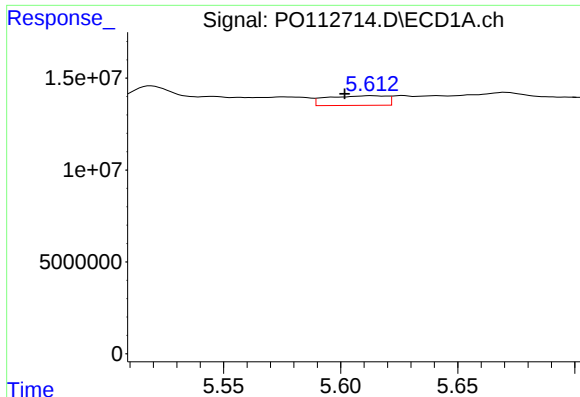

#25 AR-1248-5


R.T.: 5.613 min
Delta R.T.: 0.012 min
Response: 9244770
Conc: 26.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

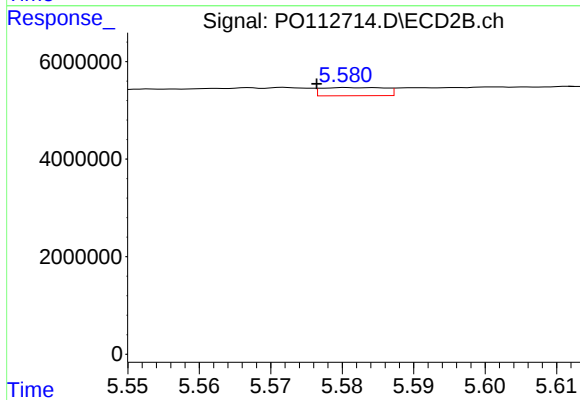


#25 AR-1248-5

R.T.: 5.581 min
Delta R.T.: 0.004 min
Response: 1036767
Conc: 4.83 ng/ml

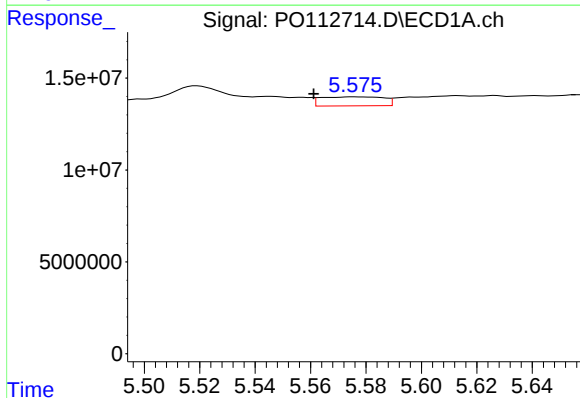


#26 AR-1254-1

R.T.: 5.576 min
Delta R.T.: 0.015 min
Response: 7683857
Conc: 14.00 ng/ml

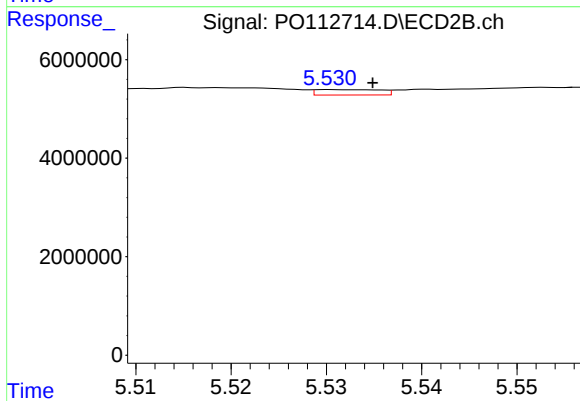

#26 AR-1254-1


R.T.: 5.531 min
Delta R.T.: -0.004 min
Response: 520943
Conc: 1.59 ng/ml

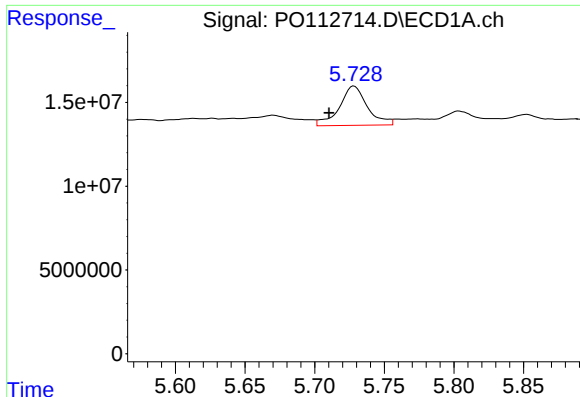

#27 AR-1254-2


R.T.: 5.728 min
Delta R.T.: 0.018 min
Response: 32738562
Conc: 67.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

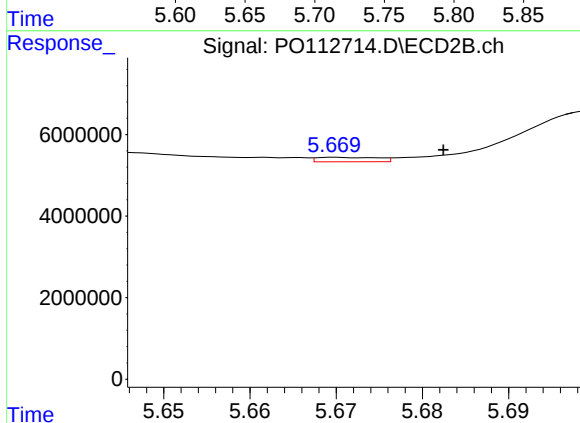


#27 AR-1254-2

R.T.: 5.670 min
Delta R.T.: -0.013 min
Response: 535095
Conc: 1.85 ng/ml

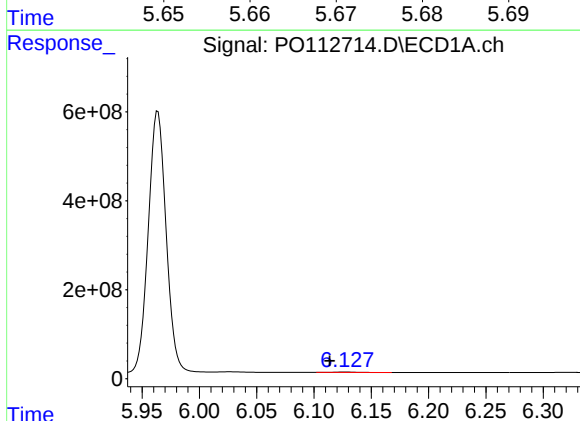


#28 AR-1254-3

R.T.: 6.128 min
Delta R.T.: 0.014 min
Response: 10058596
Conc: 13.51 ng/ml

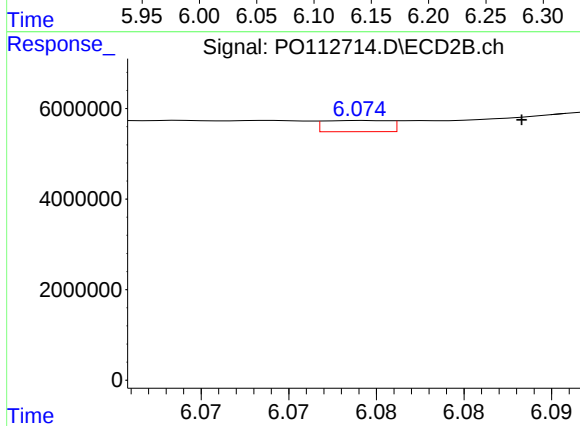

#28 AR-1254-3


R.T.: 6.074 min
Delta R.T.: -0.009 min
Response: 642647
Conc: 1.50 ng/ml

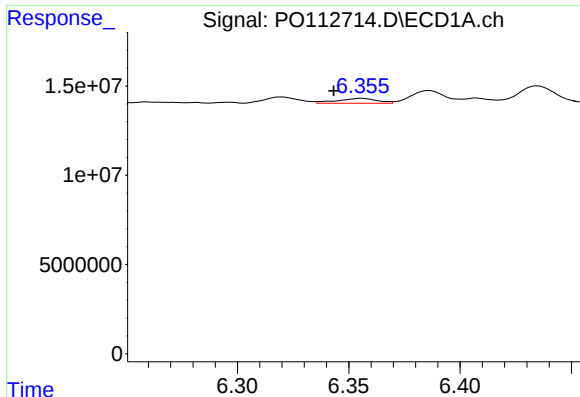

#29 AR-1254-4


R.T.: 6.356 min
Delta R.T.: 0.013 min
Response: 3399032
Conc: 6.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

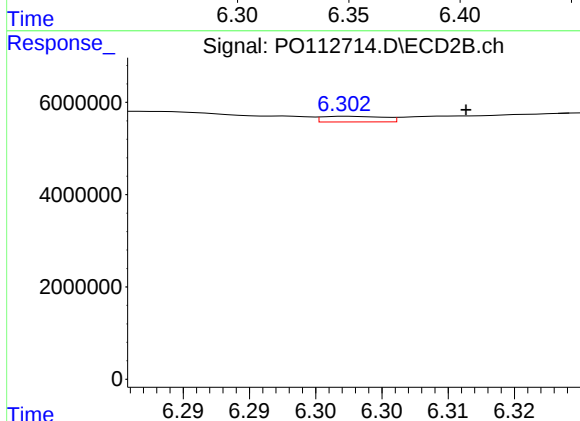


#29 AR-1254-4

R.T.: 6.302 min
Delta R.T.: -0.009 min
Response: 395194
Conc: 1.45 ng/ml

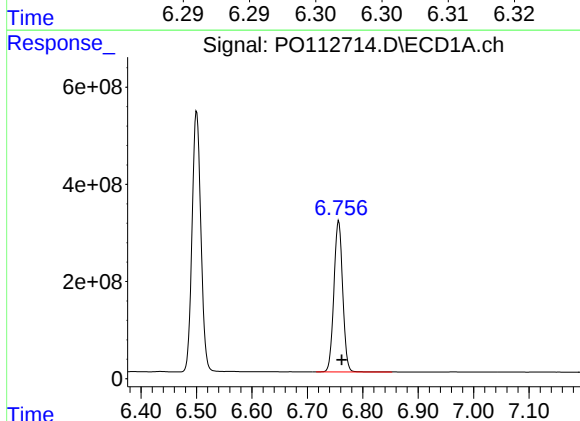


#30 AR-1254-5

R.T.: 6.757 min
Delta R.T.: -0.006 min
Response: 3424050125
Conc: 4837.43 ng/ml

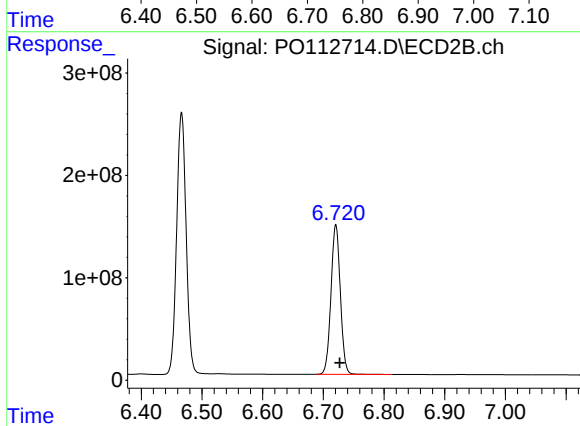

#30 AR-1254-5


R.T.: 6.721 min
Delta R.T.: -0.007 min
Response: 1571231876
Conc: 4704.01 ng/ml

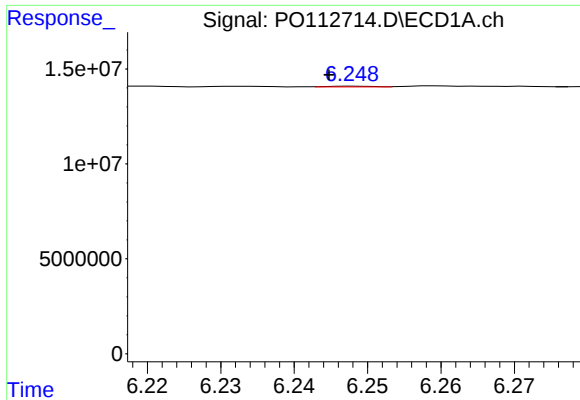

#31 AR-1260-1


R.T.: 6.248 min
Delta R.T.: 0.003 min
Response: 170698
Conc: 0.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

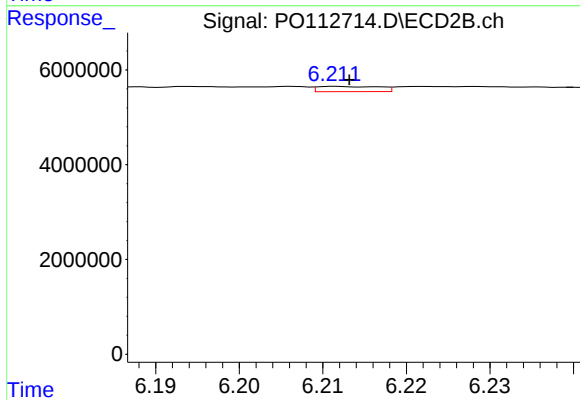


#31 AR-1260-1

R.T.: 6.212 min
Delta R.T.: -0.002 min
Response: 559347
Conc: 2.25 ng/ml

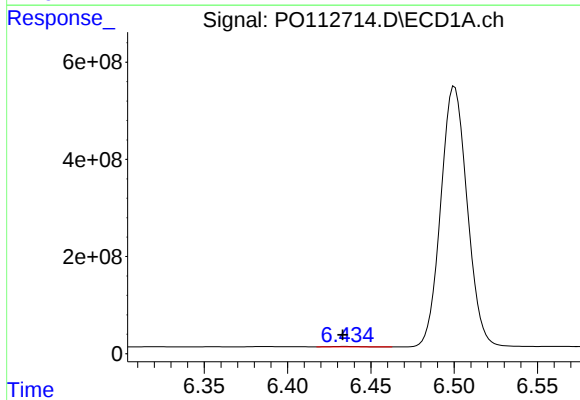


#32 AR-1260-2

R.T.: 6.435 min
Delta R.T.: 0.002 min
Response: 11805465
Conc: 17.16 ng/ml

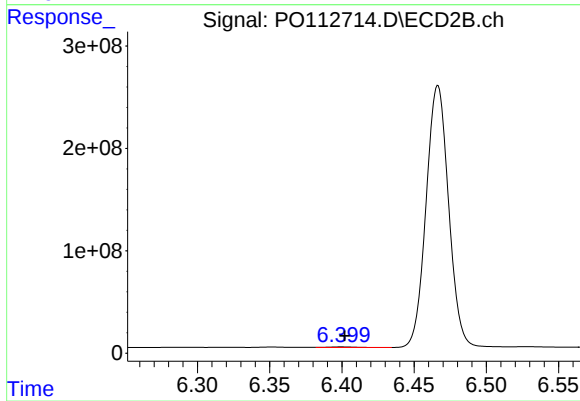

#32 AR-1260-2


R.T.: 6.400 min
Delta R.T.: -0.002 min
Response: 6681039
Conc: 20.28 ng/ml

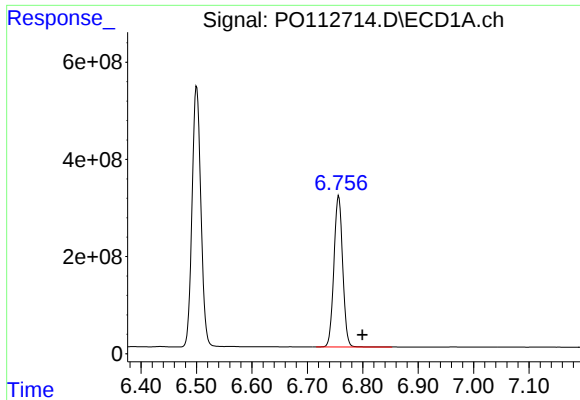

#33 AR-1260-3


R.T.: 6.757 min
Delta R.T.: -0.043 min
Response: 3424050125
Conc: 5823.02 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

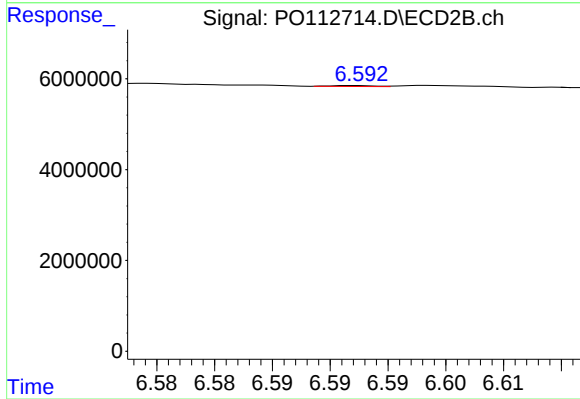


#33 AR-1260-3

R.T.: 6.592 min
Delta R.T.: 0.039 min
Response: 51729
Conc: 0.20 ng/ml

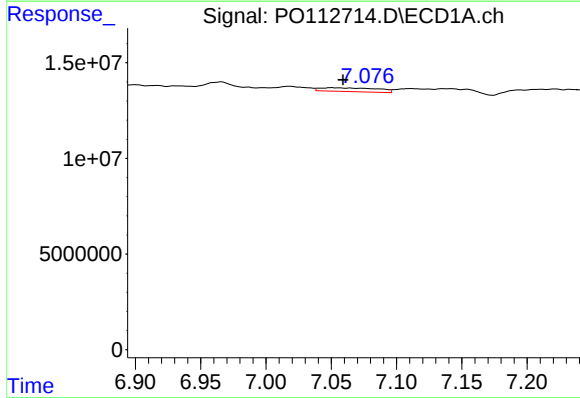


#34 AR-1260-4

R.T.: 7.050 min
Delta R.T.: -0.009 min
Response: 6127111
Conc: 13.59 ng/ml

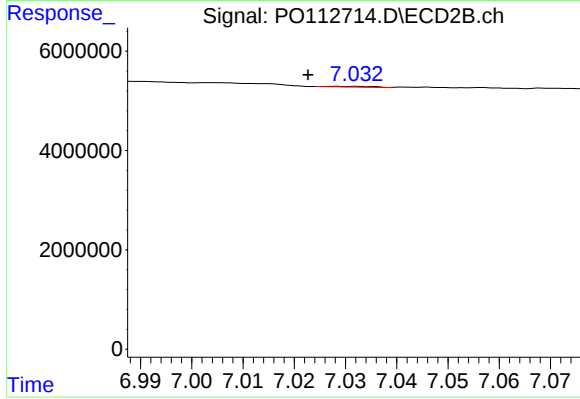

#34 AR-1260-4


R.T.: 7.028 min
Delta R.T.: 0.006 min
Response: 84352
Conc: 0.44 ng/ml

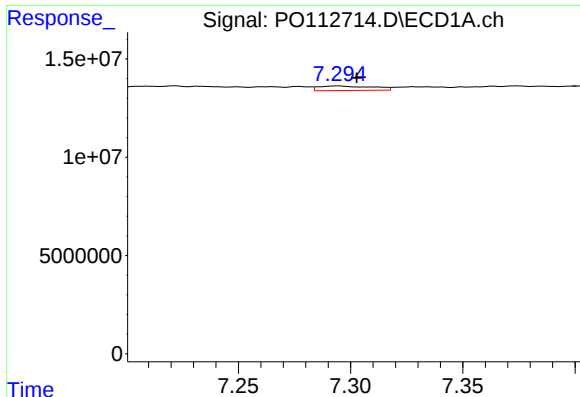

#35 AR-1260-5


R.T.: 7.294 min
Delta R.T.: -0.008 min
Response: 3821836
Conc: 3.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

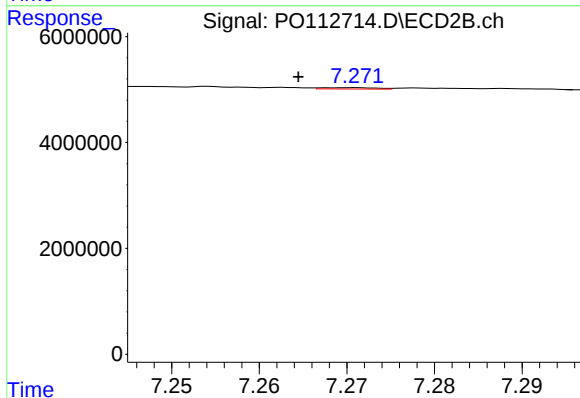


#35 AR-1260-5

R.T.: 7.271 min
Delta R.T.: 0.007 min
Response: 109874
Conc: 0.27 ng/ml

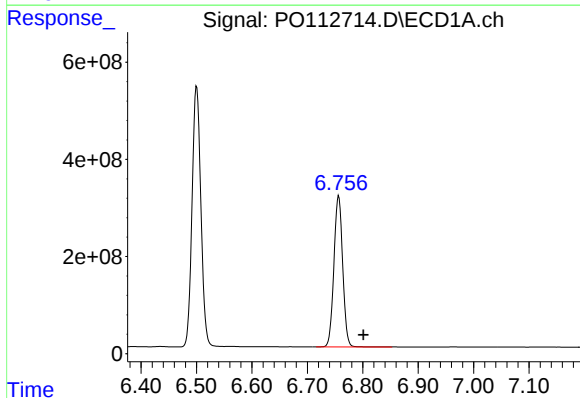


#36 AR-1262-1

R.T.: 6.757 min
Delta R.T.: -0.045 min
Response: 3424050125
Conc: 3684.91 ng/ml

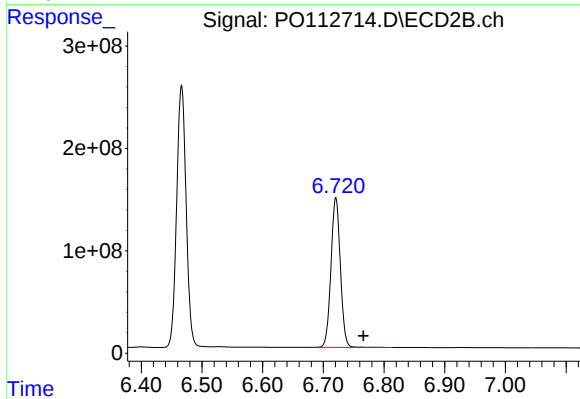

#36 AR-1262-1


R.T.: 6.721 min
Delta R.T.: -0.045 min
Response: 1571231876
Conc: 3787.67 ng/ml

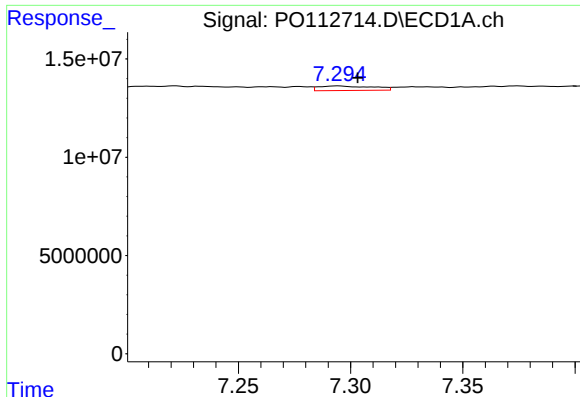

#37 AR-1262-2


R.T.: 7.294 min
Delta R.T.: -0.009 min
Response: 3821836
Conc: 2.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

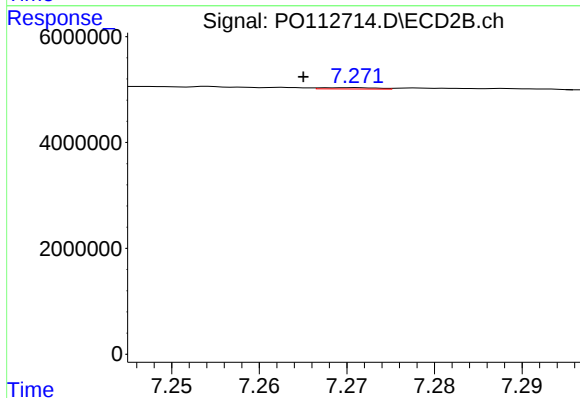


#37 AR-1262-2

R.T.: 7.271 min
Delta R.T.: 0.006 min
Response: 109874
Conc: 0.21 ng/ml

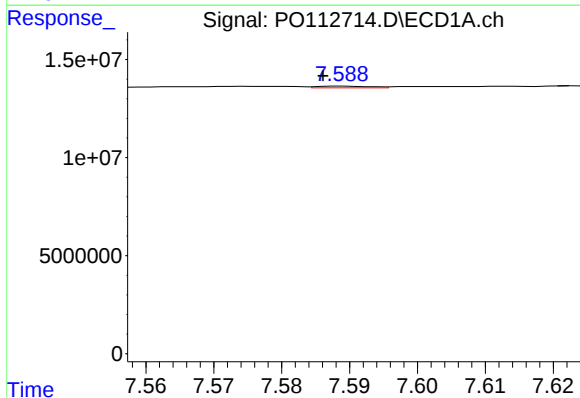


#38 AR-1262-3

R.T.: 7.589 min
Delta R.T.: 0.003 min
Response: 485460
Conc: 0.82 ng/ml

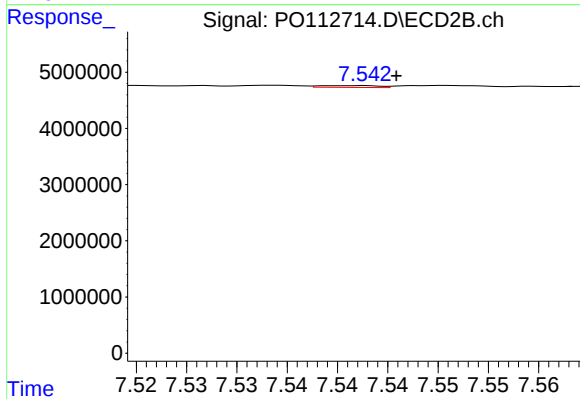

#38 AR-1262-3


R.T.: 7.542 min
Delta R.T.: -0.003 min
Response: 133083
Conc: 0.71 ng/ml

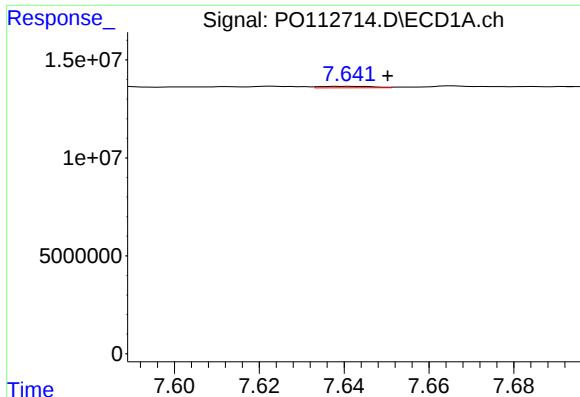

#39 AR-1262-4


R.T.: 7.641 min
Delta R.T.: -0.009 min
Response: 669017
Conc: 0.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

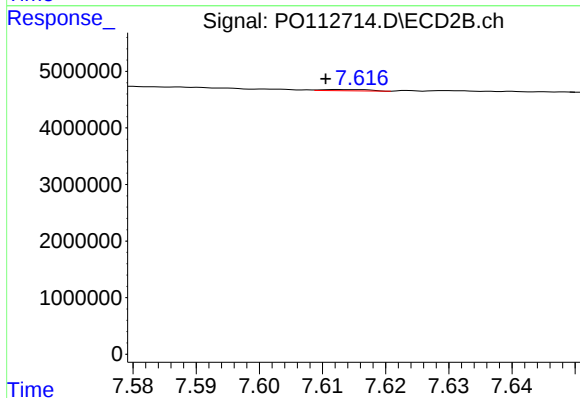


#39 AR-1262-4

R.T.: 7.613 min
Delta R.T.: 0.002 min
Response: 116060
Conc: 0.40 ng/ml

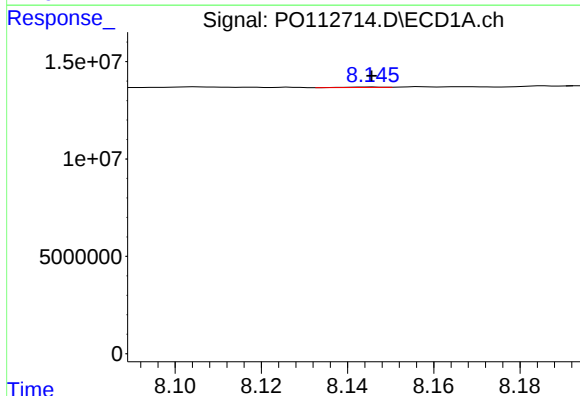


#40 AR-1262-5

R.T.: 8.146 min
Delta R.T.: 0.000 min
Response: 160000
Conc: 0.37 ng/ml

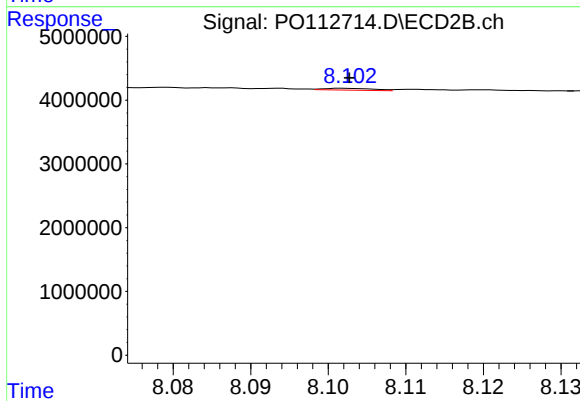

#40 AR-1262-5


R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 126330
Conc: 1.27 ng/ml

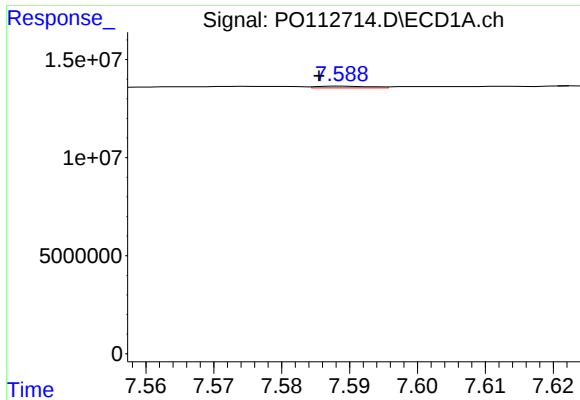

#41 AR-1268-1


R.T.: 7.589 min
Delta R.T.: 0.003 min
Response: 485460
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

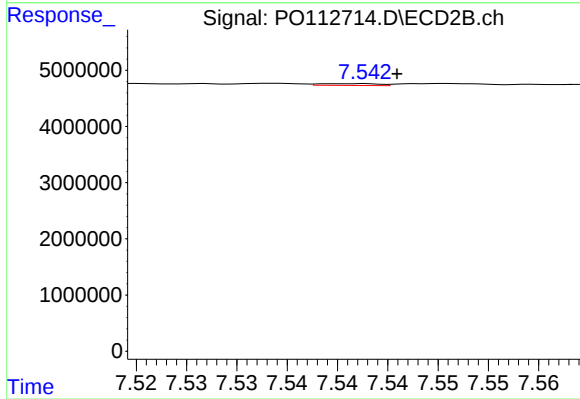


#41 AR-1268-1

R.T.: 7.542 min
Delta R.T.: -0.004 min
Response: 133083
Conc: 0.26 ng/ml

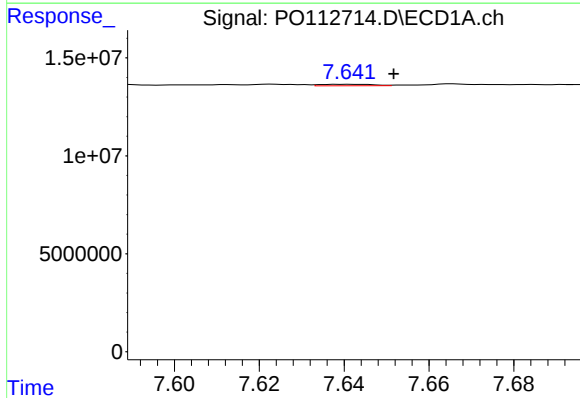


#42 AR-1268-2

R.T.: 7.641 min
Delta R.T.: -0.011 min
Response: 669017
Conc: 0.45 ng/ml

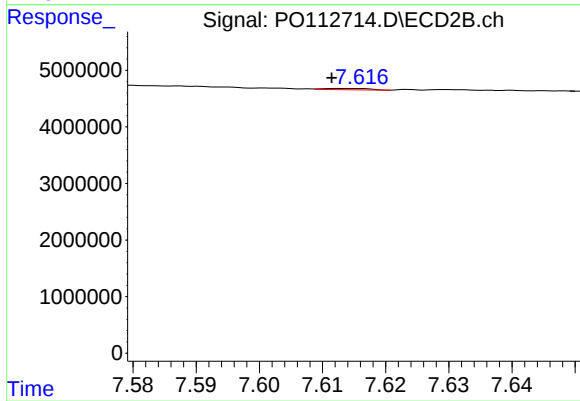

#42 AR-1268-2


R.T.: 7.613 min
Delta R.T.: 0.001 min
Response: 116060
Conc: 0.27 ng/ml

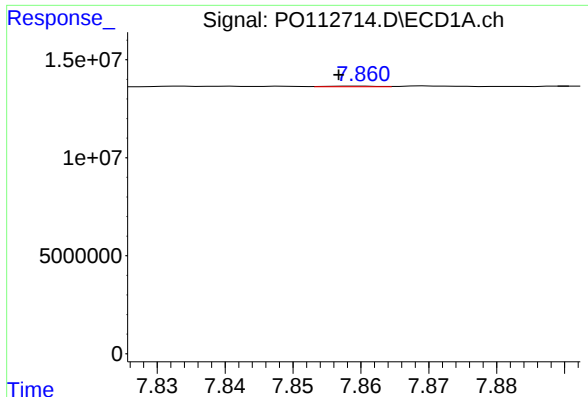

#43 AR-1268-3


R.T.: 7.860 min
Delta R.T.: 0.003 min
Response: 170928
Conc: 0.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

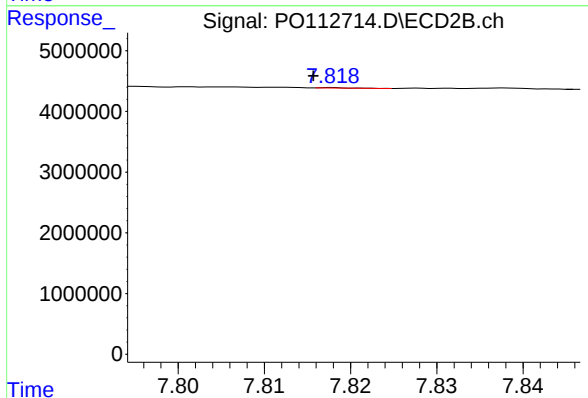


#43 AR-1268-3

R.T.: 7.818 min
Delta R.T.: 0.002 min
Response: 15247
Conc: 0.05 ng/ml

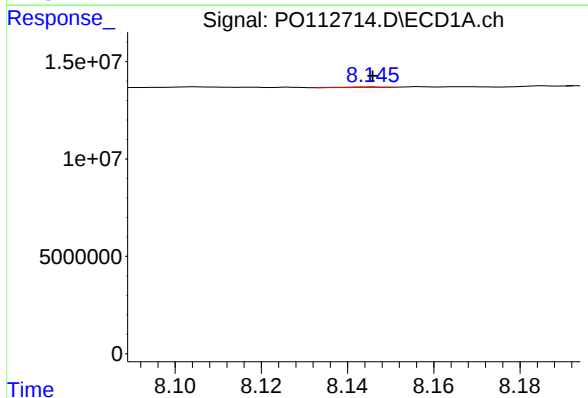


#44 AR-1268-4

R.T.: 8.146 min
Delta R.T.: 0.000 min
Response: 160000
Conc: 0.33 ng/ml

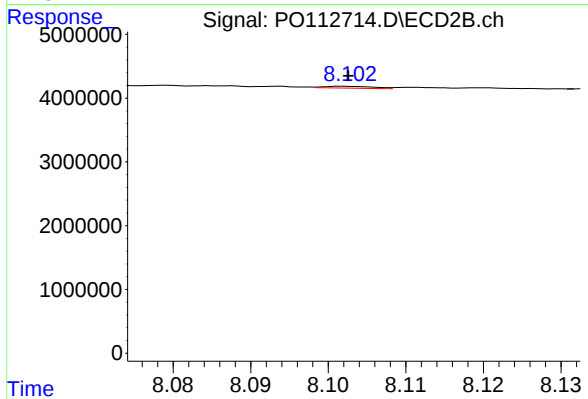

#44 AR-1268-4


R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 126330
Conc: 1.14 ng/ml

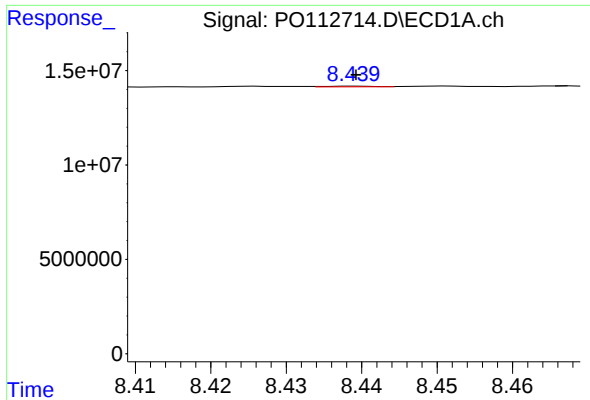

#45 AR-1268-5

R.T.: 8.439 min
Delta R.T.: 0.000 min
Response: 163492
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

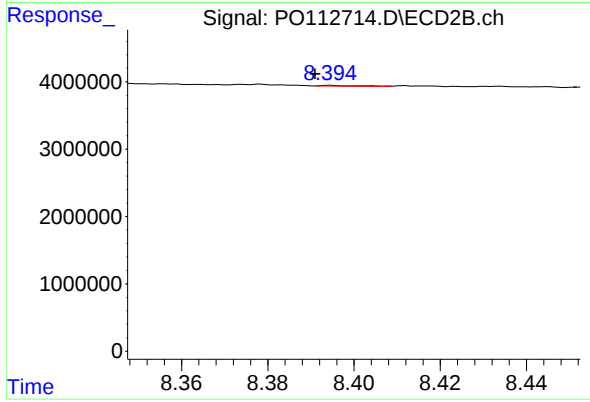

#45 AR-1268-5

R.T.: 8.394 min
Delta R.T.: 0.003 min
Response: 61440
Conc: 0.08 ng/ml