

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080425\
Data File : P0112726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2025 14:38
Operator : YP/AJ
Sample : Q2747-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 14:53:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.668	3.659	109.9E6	65715585	13.512	13.225
2) SA Decachlor...	8.690	8.634	72206399	18429278	9.875	10.429

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080425\
Data File : PO112726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2025 14:38
Operator : YP/AJ
Sample : Q2747-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 14:53:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

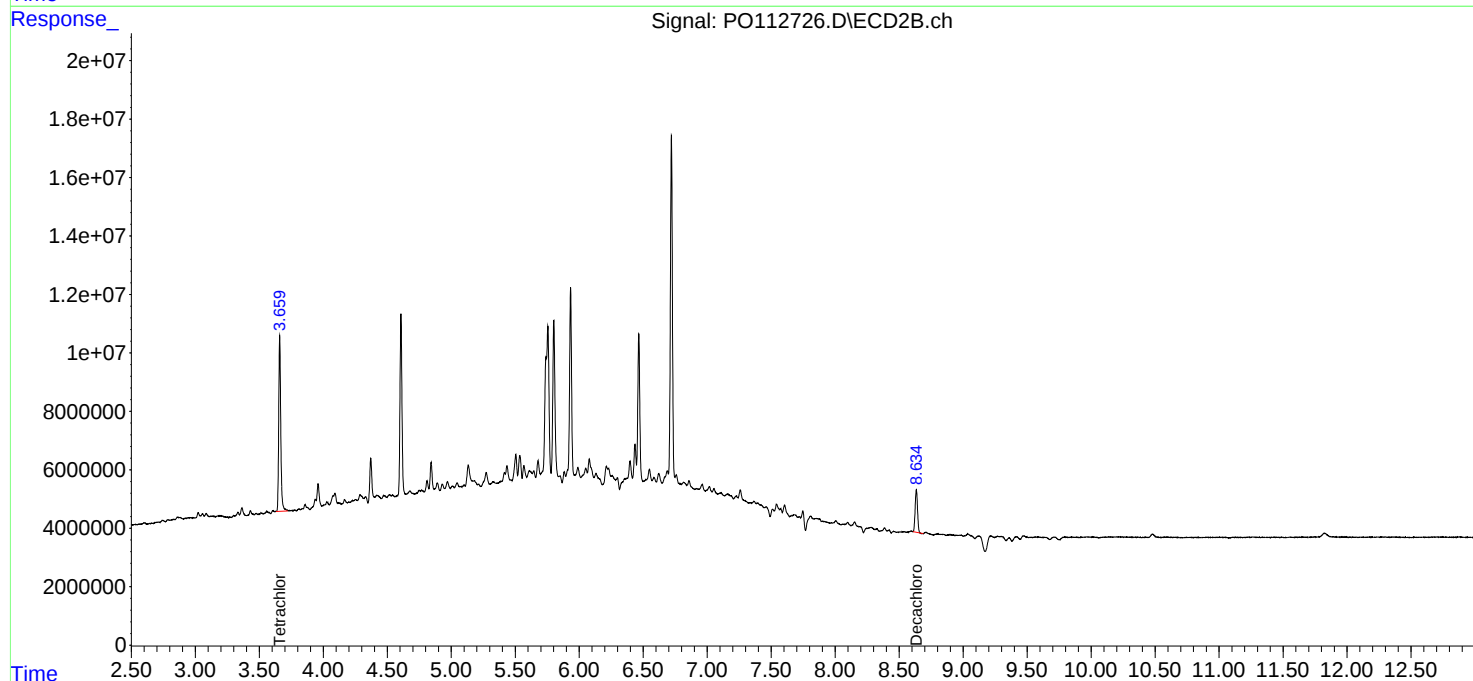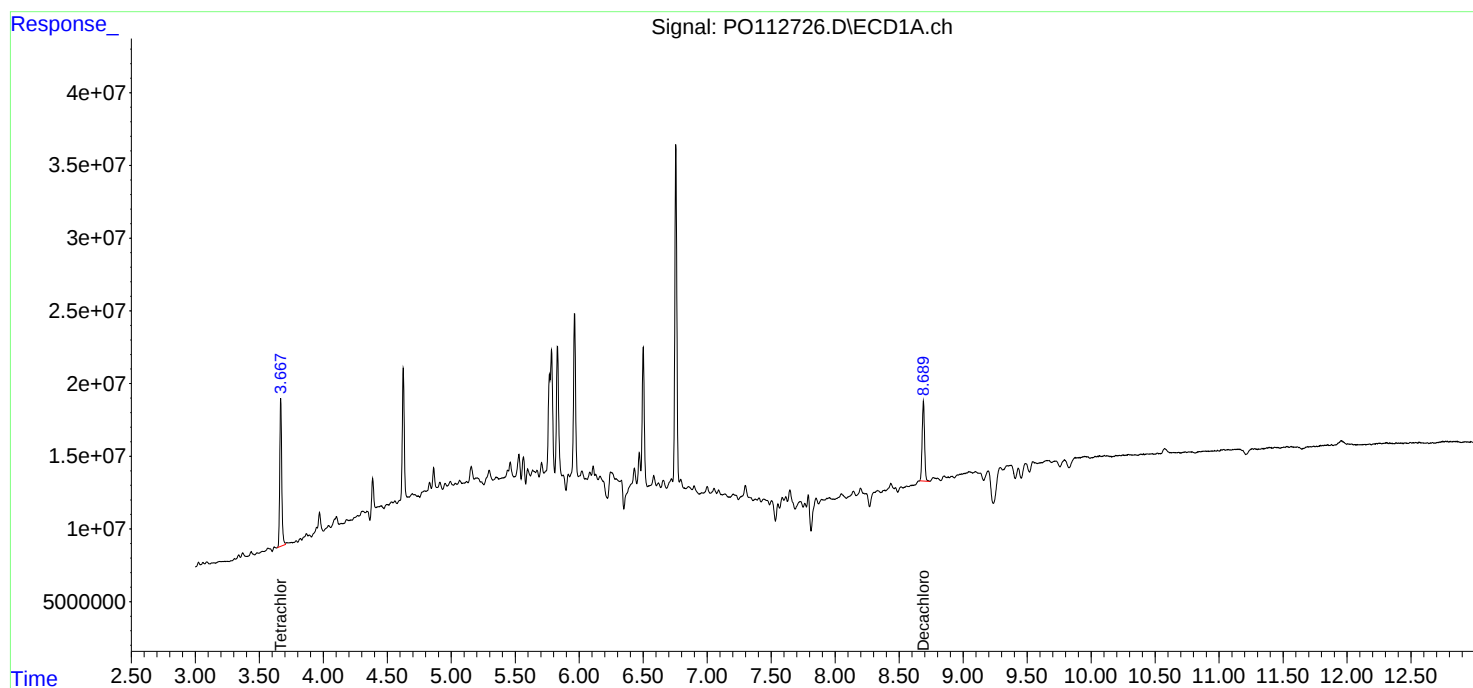


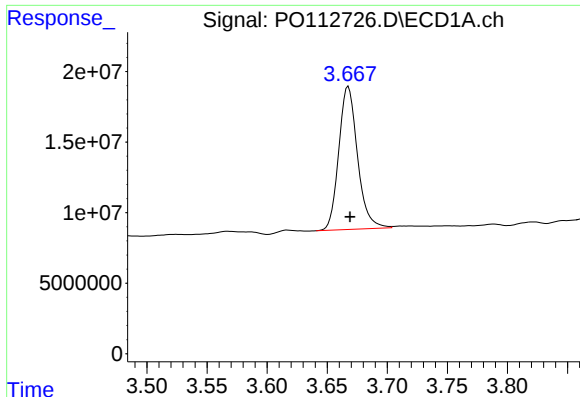

#1 Tetrachloro-m-xylene


R.T.: 3.668 min
Delta R.T.: -0.001 min
Response: 109874293
Conc: 13.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

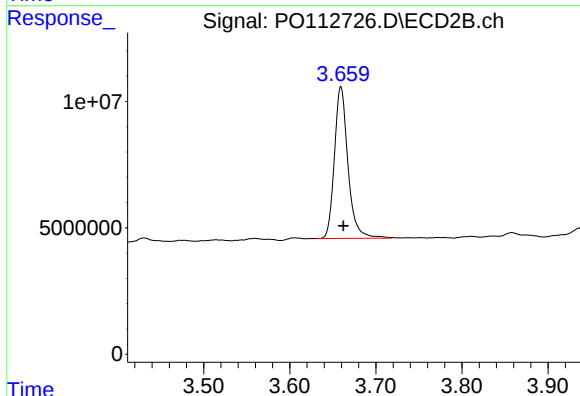


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.003 min
Response: 65715585
Conc: 13.22 ng/ml

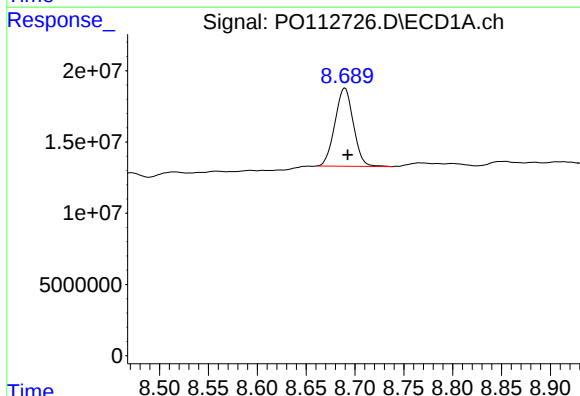

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.003 min
Response: 72206399
Conc: 9.88 ng/ml

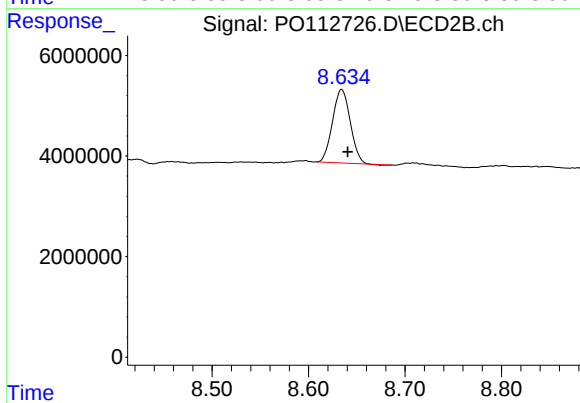

#2 Decachlorobiphenyl

R.T.: 8.634 min
Delta R.T.: -0.006 min
Response: 18429278
Conc: 10.43 ng/ml