

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080425\
Data File : P0112727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2025 14:56
Operator : YP/AJ
Sample : Q2747-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 17:33:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.667	3.659	91863937	54316163	11.297	10.931
2) SA Decachlor...	8.689	8.634	56492045	14643336	7.726	8.287

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080425\
Data File : PO112727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2025 14:56
Operator : YP/AJ
Sample : Q2747-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 17:33:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

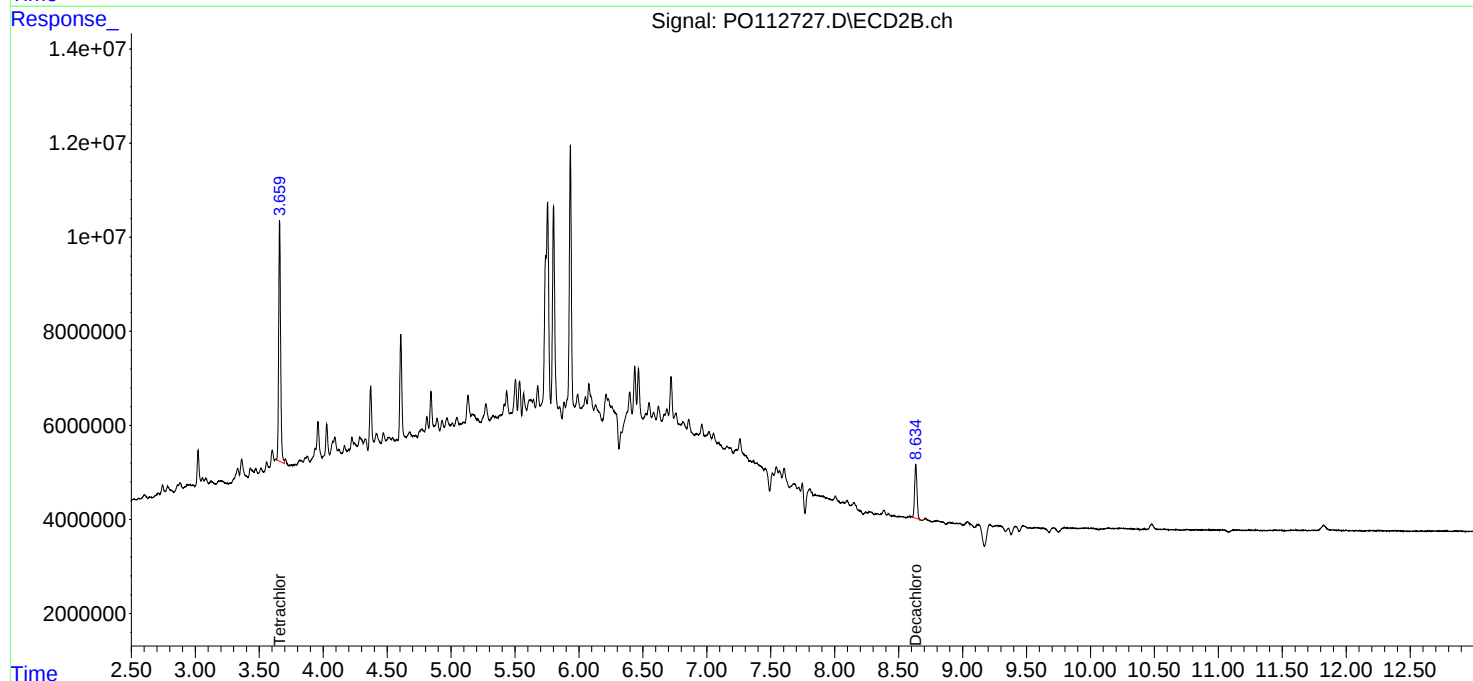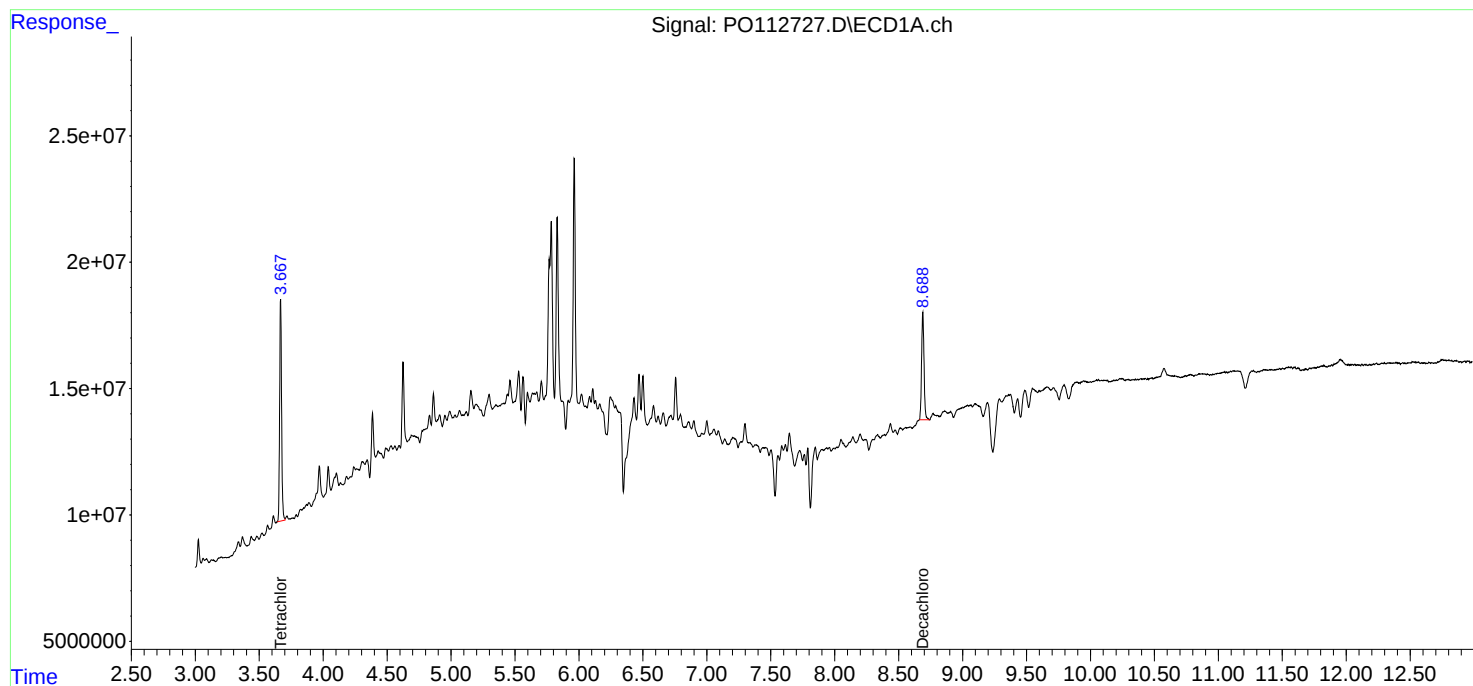


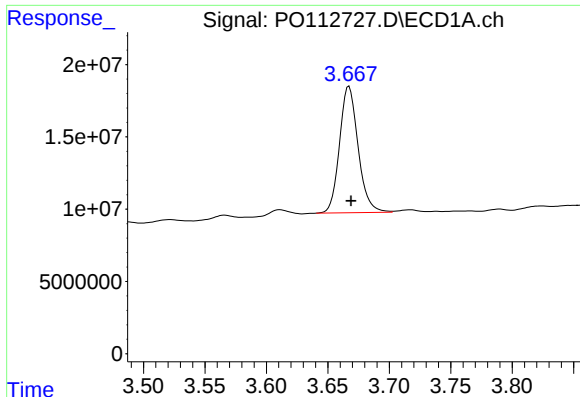

#1 Tetrachloro-m-xylene


R.T.: 3.667 min
Delta R.T.: -0.002 min
Response: 91863937
Conc: 11.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

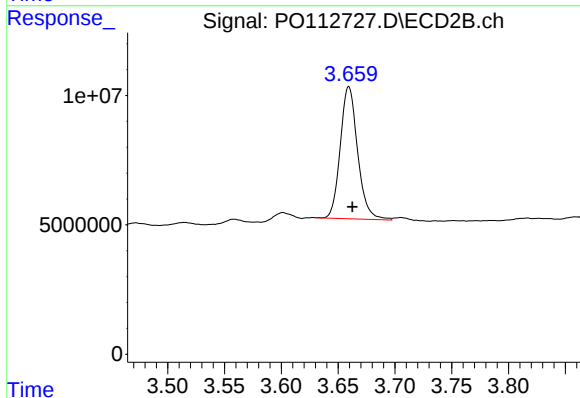


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.003 min
Response: 54316163
Conc: 10.93 ng/ml

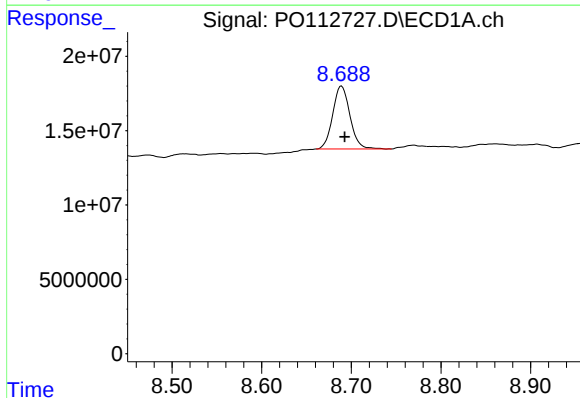

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: -0.004 min
Response: 56492045
Conc: 7.73 ng/ml

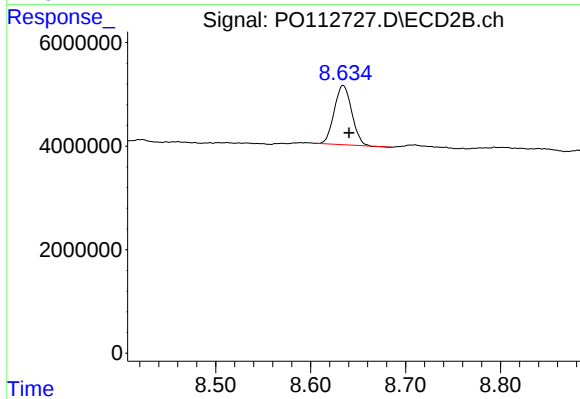

#2 Decachlorobiphenyl

R.T.: 8.634 min
Delta R.T.: -0.006 min
Response: 14643336
Conc: 8.29 ng/ml