

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
 Data File : P0058881.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2019 20:18
 Operator : SM/AJ
 Sample : K4156-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RT3380

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:12:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.156	3.515	847918	710273	20.091	17.779
2)	SA Decachlor...	9.664	8.399	486929	375253	8.991	9.507
Target Compounds							
7)	L1 AR-1016-5	0.000	4.960	0	154869	N.D.	125.763 #
15)	L3 AR-1232-5	0.000	4.960	0	154869	N.D.	351.775 #
20)	L4 AR-1242-5	0.000	5.353	0	17349	N.D.	16.174 #
24)	L5 AR-1248-4	0.000	4.960	0	154869	N.D.	110.859 #
25)	L5 AR-1248-5	0.000	5.353	0	17349	N.D.	12.524 #
26)	L6 AR-1254-1	0.000	5.353	0	17349	N.D.	6.697 #
27)	L6 AR-1254-2	0.000	5.558	0	40338	N.D.	17.619 #
30)	L6 AR-1254-5	0.000	6.501	0	19291	N.D.	5.592 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080519\
Data File : PO058881.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2019 20:18
Operator : SM/AJ
Sample : K4156-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RT3380

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:12:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

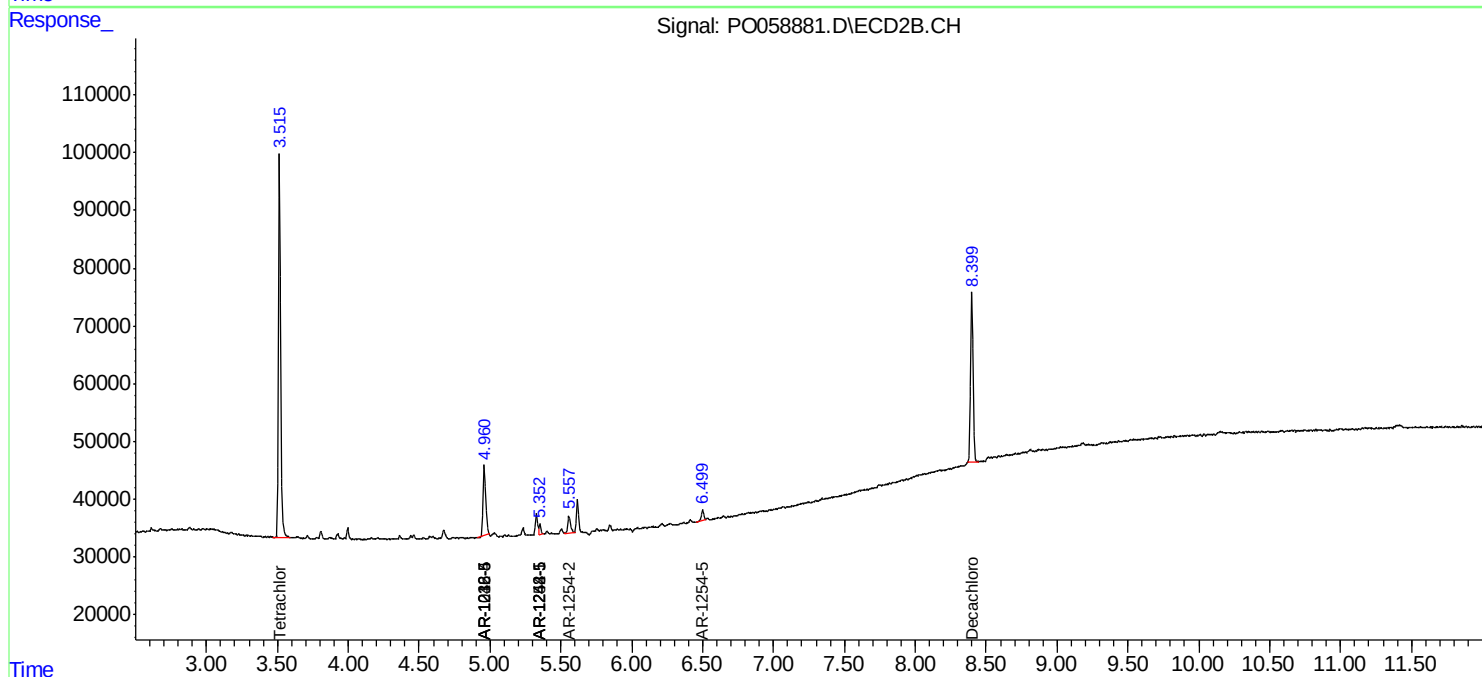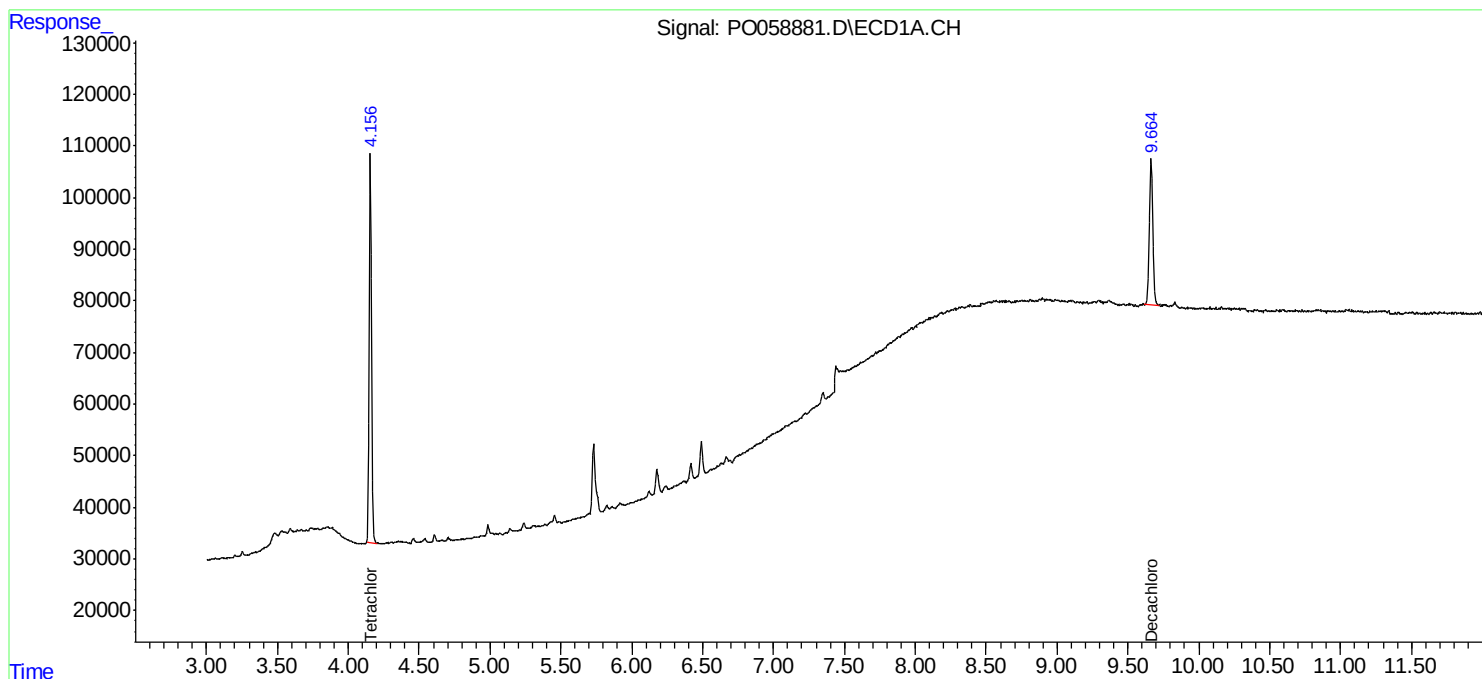


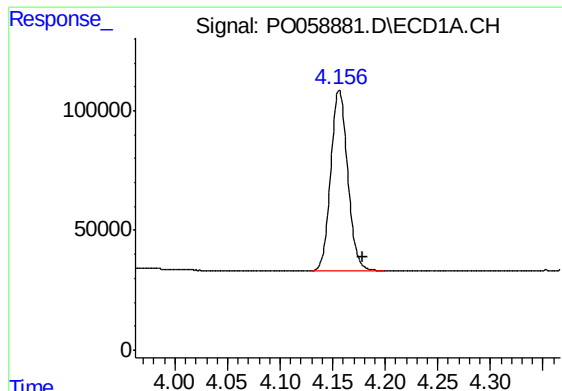

#1 Tetrachloro-m-xylene


R.T.: 4.156 min
Delta R.T.: -0.023 min
Response: 847918
Conc: 20.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT3380

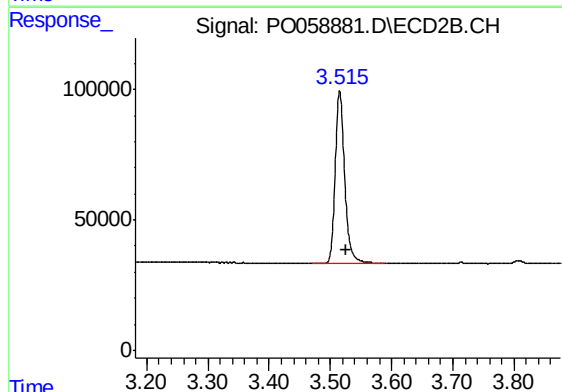


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: -0.010 min
Response: 710273
Conc: 17.78 ng/ml

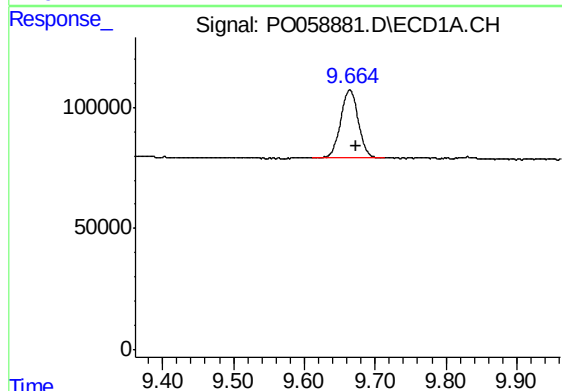


#2 Decachlorobiphenyl

R.T.: 9.664 min
Delta R.T.: -0.008 min
Response: 486929
Conc: 8.99 ng/ml

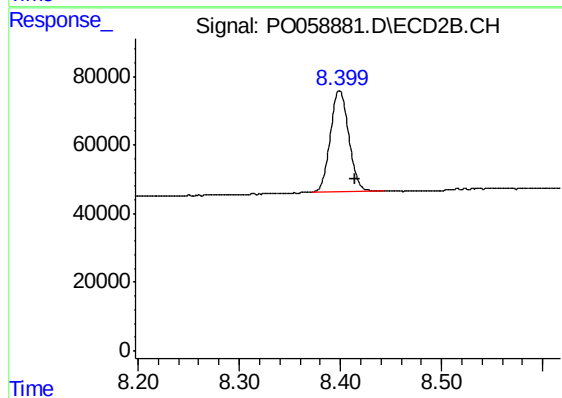

#2 Decachlorobiphenyl


R.T.: 8.399 min
Delta R.T.: -0.015 min
Response: 375253
Conc: 9.51 ng/ml

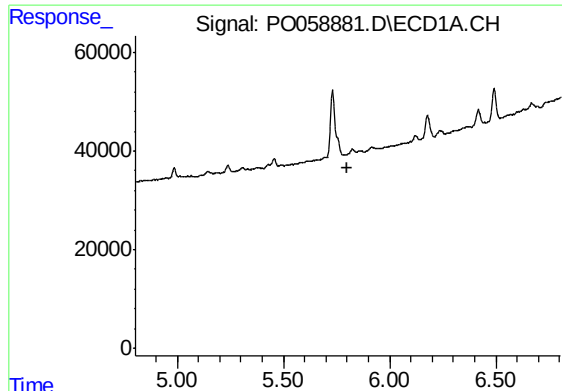

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.803 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
RT3380

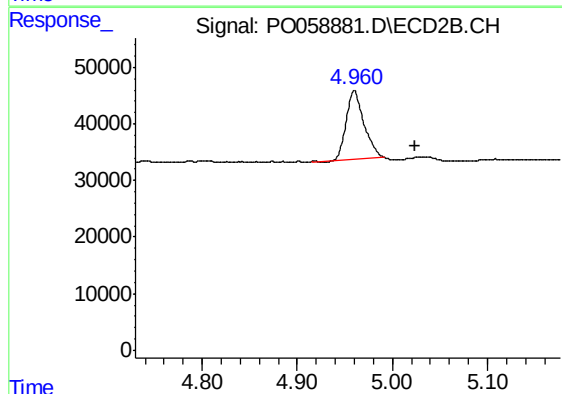


#7 AR-1016-5

R.T.: 4.960 min
Delta R.T.: -0.064 min
Response: 154869
Conc: 125.76 ng/ml

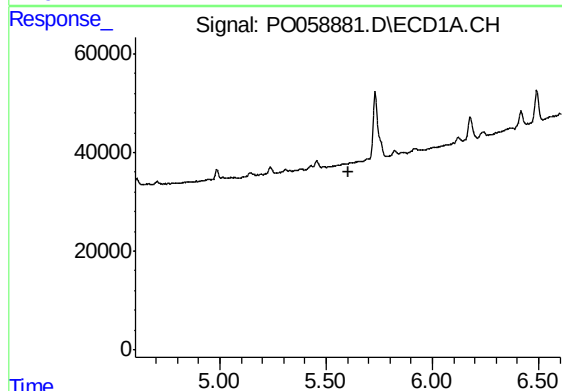


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

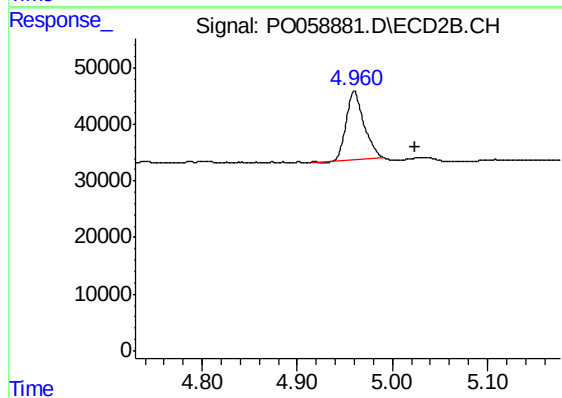

#15 AR-1232-5


R.T.: 4.960 min
Delta R.T.: -0.063 min
Response: 154869
Conc: 351.77 ng/ml

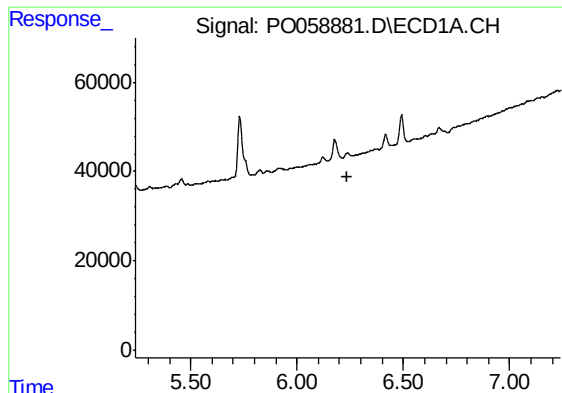

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
RT3380

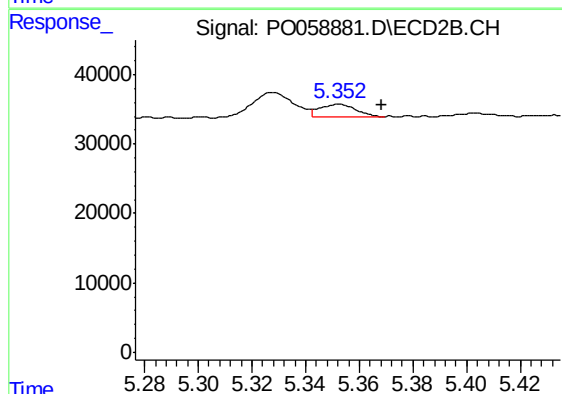


#20 AR-1242-5

R.T.: 5.353 min
Delta R.T.: -0.016 min
Response: 17349
Conc: 16.17 ng/ml

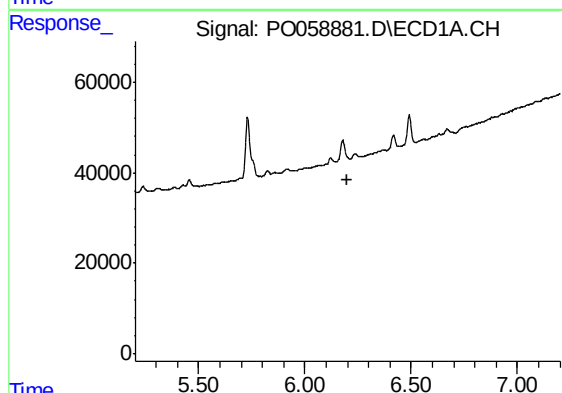


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.203 min
Response: 0
Conc: N.D.

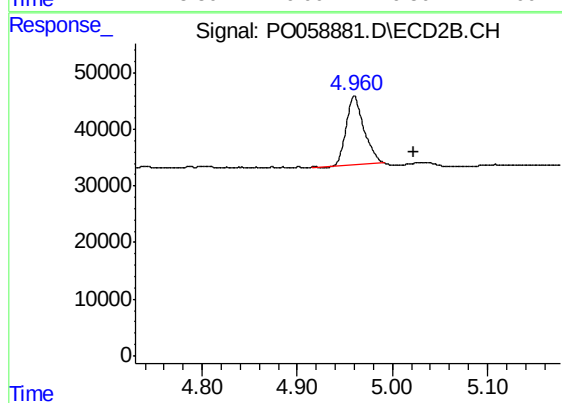

#24 AR-1248-4


R.T.: 4.960 min
Delta R.T.: -0.063 min
Response: 154869
Conc: 110.86 ng/ml

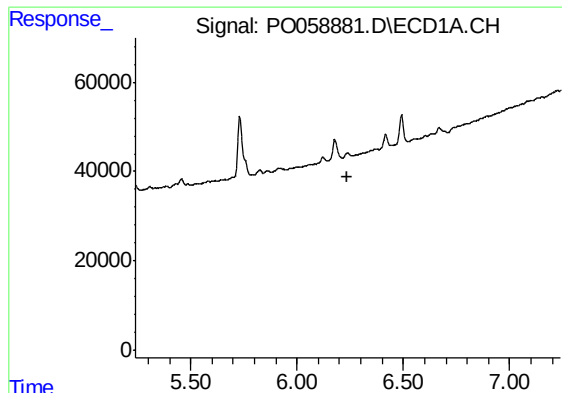

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
RT3380

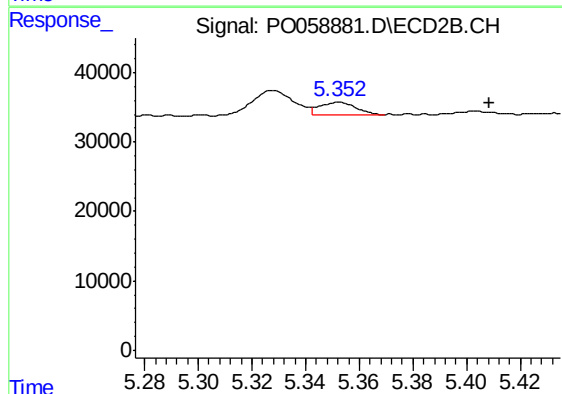


#25 AR-1248-5

R.T.: 5.353 min
Delta R.T.: -0.056 min
Response: 17349
Conc: 12.52 ng/ml

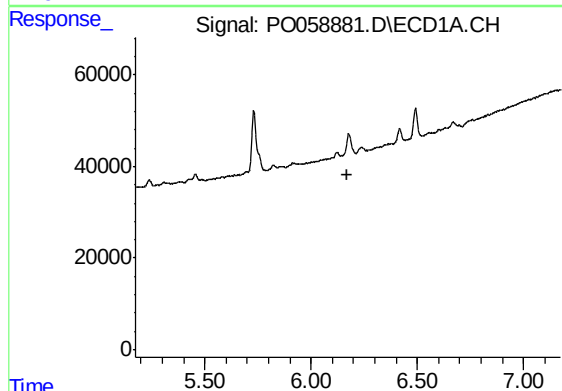


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.173 min
Response: 0
Conc: N.D.

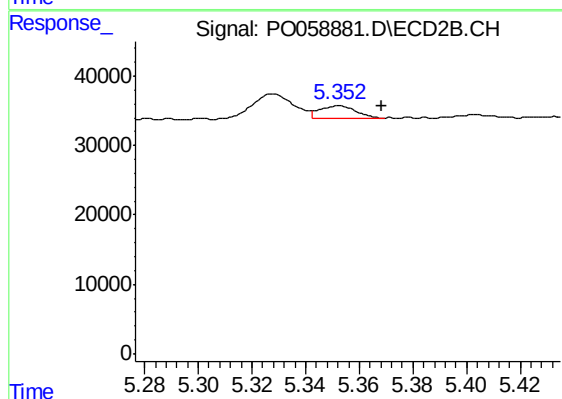

#26 AR-1254-1


R.T.: 5.353 min
Delta R.T.: -0.016 min
Response: 17349
Conc: 6.70 ng/ml

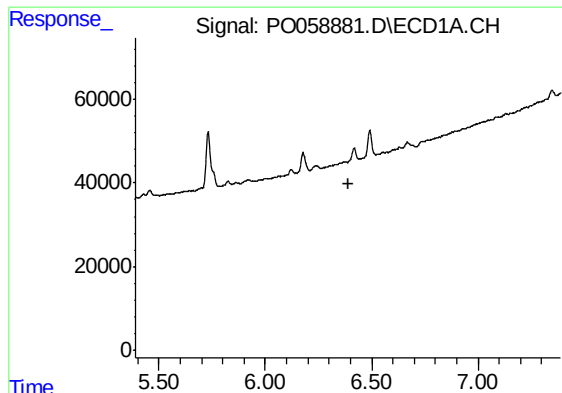

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
RT3380

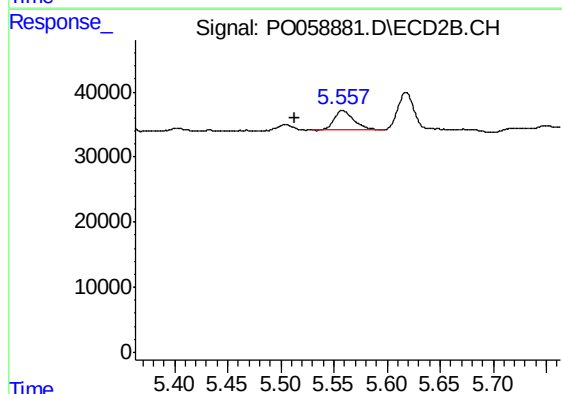


#27 AR-1254-2

R.T.: 5.558 min
Delta R.T.: 0.044 min
Response: 40338
Conc: 17.62 ng/ml

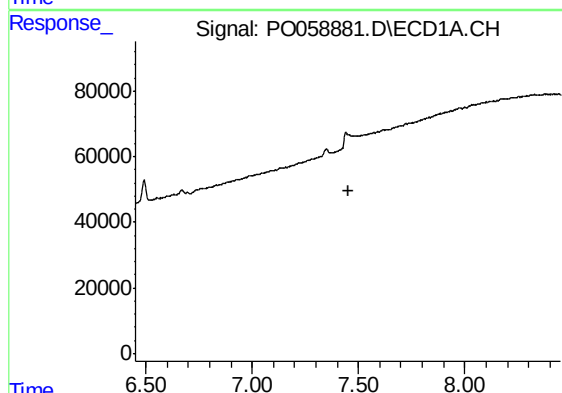

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.450 min
Response: 0
Conc: N.D.

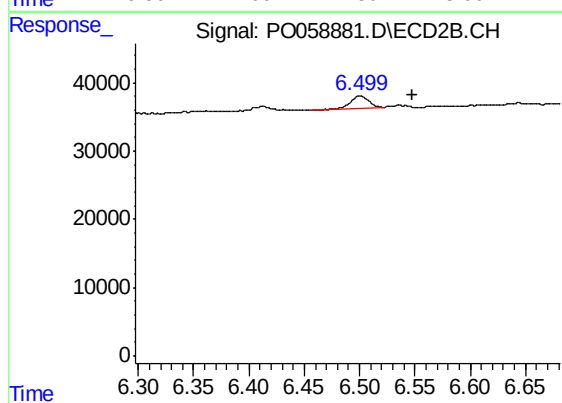

#30 AR-1254-5

R.T.: 6.501 min
Delta R.T.: -0.048 min
Response: 19291
Conc: 5.59 ng/ml