

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
 Data File : P0058850.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2019 10:21
 Operator : SM/AJ
 Sample : K4150-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-4

Manual Integrations
 APPROVED

Ankita
 8/6/2019 2:28:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 11:45:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.158	3.516	1182066	946570	28.009	23.694
2) SA Decachlor...	9.664	8.399	1098470	793195	20.284	20.095
Target Compounds						
31) L7 AR-1260-1	6.893	6.024	79872	64790	27.742m	27.222m
32) L7 AR-1260-2	7.150	6.212	122907	50286	29.545m	16.600 #
33) L7 AR-1260-3	7.503	6.361	94205	55550	25.297m	20.575m
34) L7 AR-1260-4	7.730	6.825	89376	48880	26.227m	21.633
35) L7 AR-1260-5	8.038	7.069	111394	101776	15.146m	18.899m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
Data File : P0058850.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2019 10:21
Operator : SM/AJ
Sample : K4150-10
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
8/6/2019 2:28:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 11:45:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

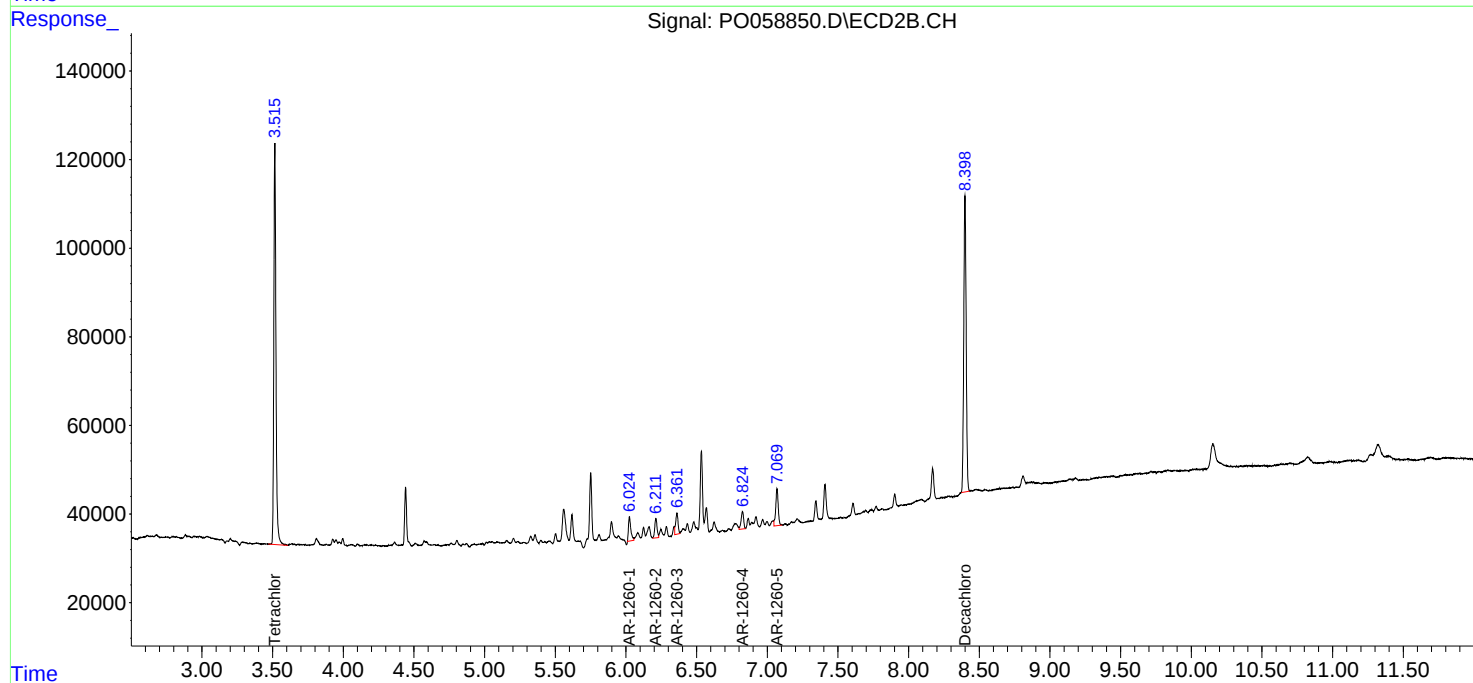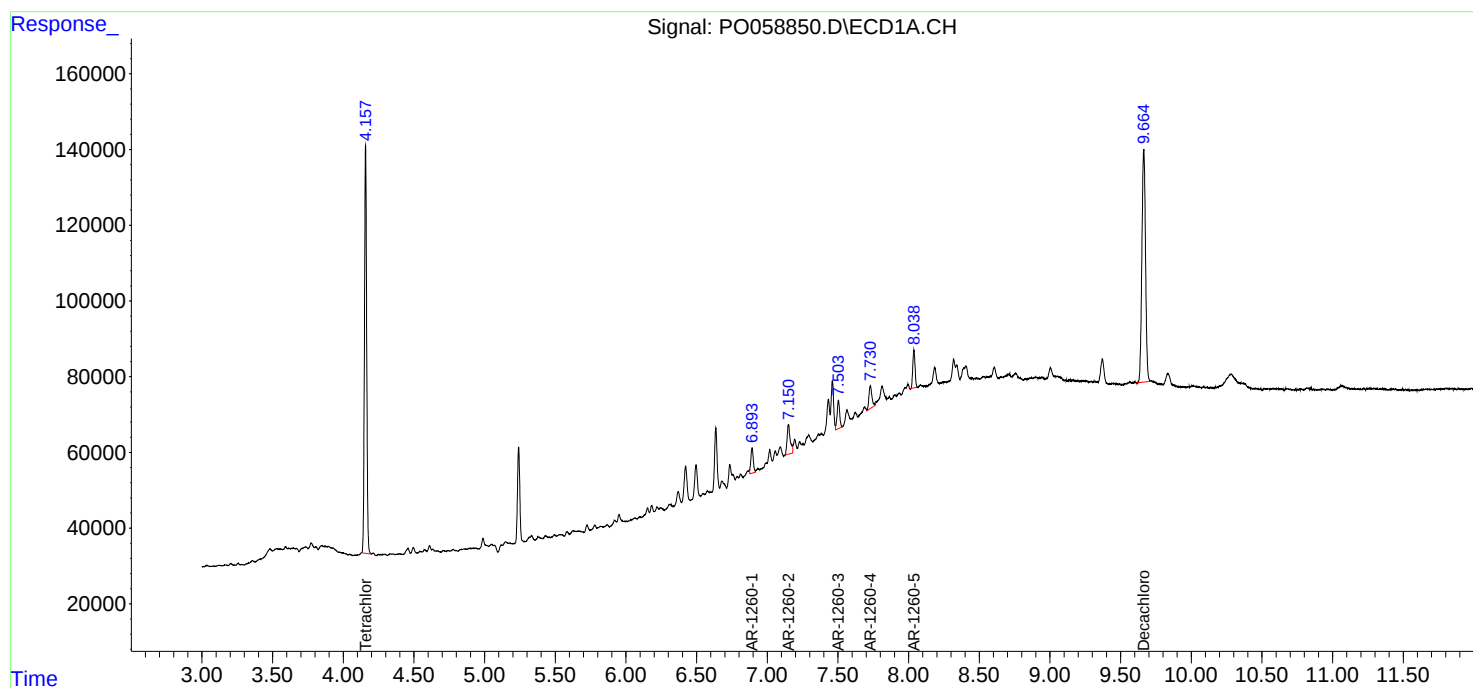

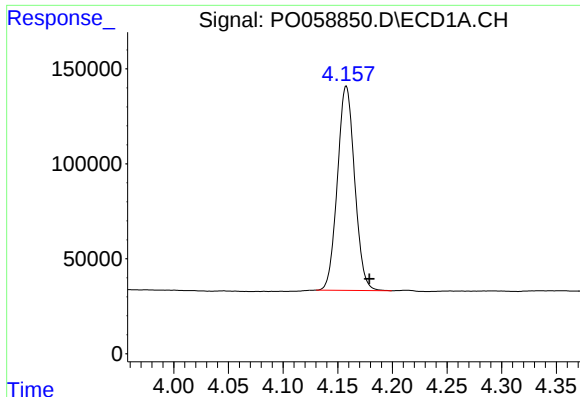


#1 Tetrachloro-m-xylene

R.T.: 4.158 min
Delta R.T.: -0.021 min
Response: 1182066
Conc: 28.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
8/6/2019 2:28:38 PM

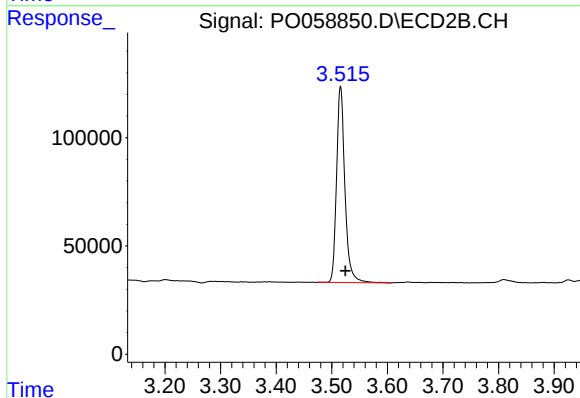


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 946570
Conc: 23.69 ng/ml

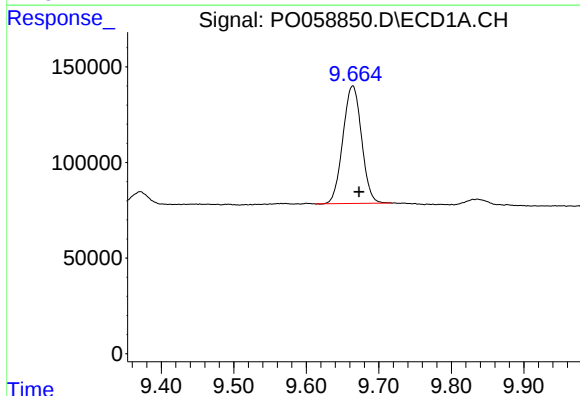


#2 Decachlorobiphenyl

R.T.: 9.664 min
Delta R.T.: -0.009 min
Response: 1098470
Conc: 20.28 ng/ml

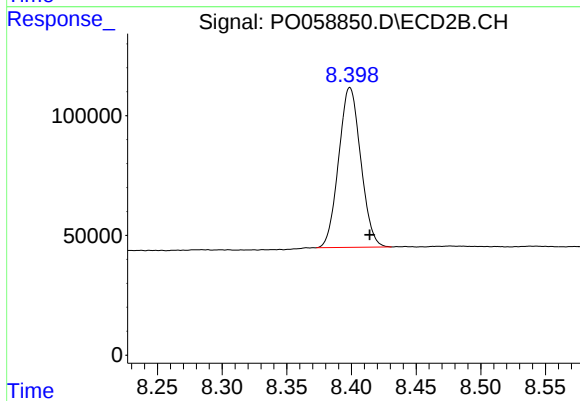

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.015 min
Response: 793195
Conc: 20.09 ng/ml

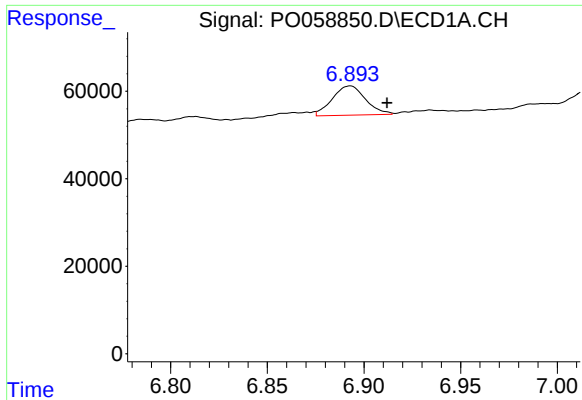


#31 AR-1260-1

R.T.: 6.893 min
Delta R.T.: -0.019 min
Response: 79872
Conc: 27.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
8/6/2019 2:28:38 PM

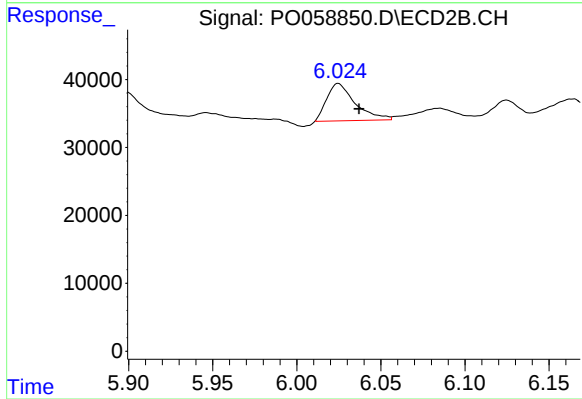


#31 AR-1260-1

R.T.: 6.024 min
Delta R.T.: -0.013 min
Response: 64790
Conc: 27.22 ng/ml m

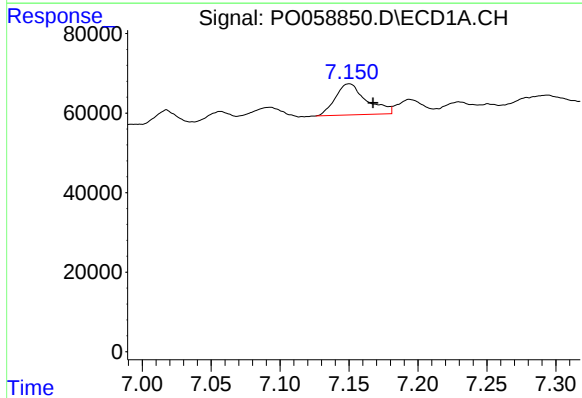


#32 AR-1260-2

R.T.: 7.150 min
Delta R.T.: -0.018 min
Response: 122907
Conc: 29.54 ng/ml m

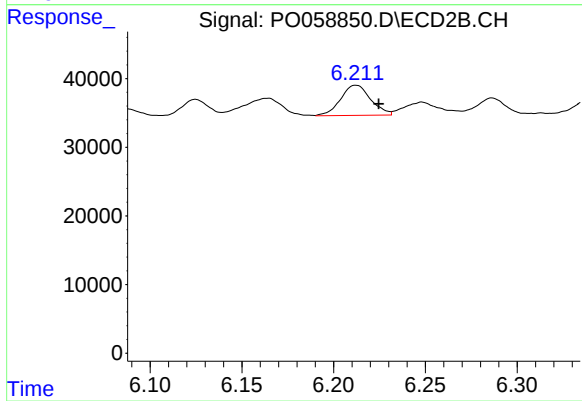

#32 AR-1260-2

R.T.: 6.212 min
Delta R.T.: -0.012 min
Response: 50286
Conc: 16.60 ng/ml

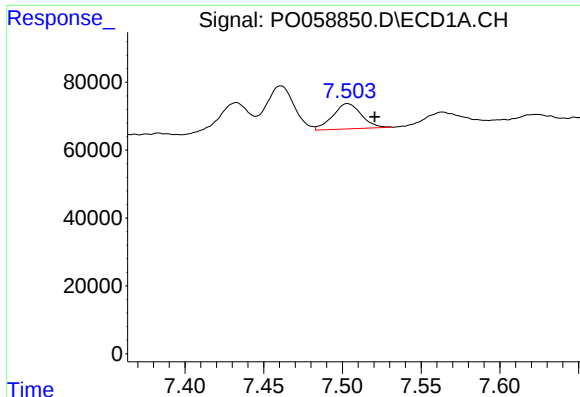


#33 AR-1260-3

R.T.: 7.503 min
Delta R.T.: -0.018 min
Response: 94205
Conc: 25.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
8/6/2019 2:28:38 PM

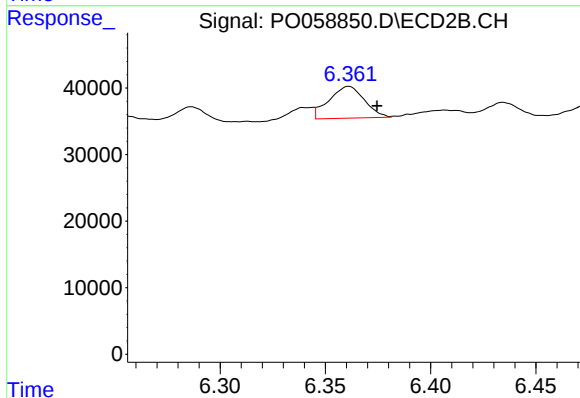


#33 AR-1260-3

R.T.: 6.361 min
Delta R.T.: -0.014 min
Response: 55550
Conc: 20.58 ng/ml m

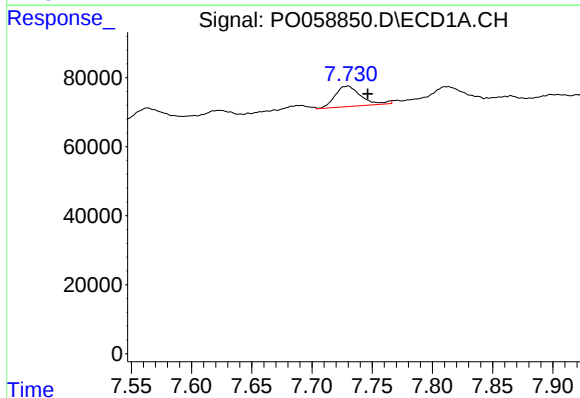


#34 AR-1260-4

R.T.: 7.730 min
Delta R.T.: -0.016 min
Response: 89376
Conc: 26.23 ng/ml m

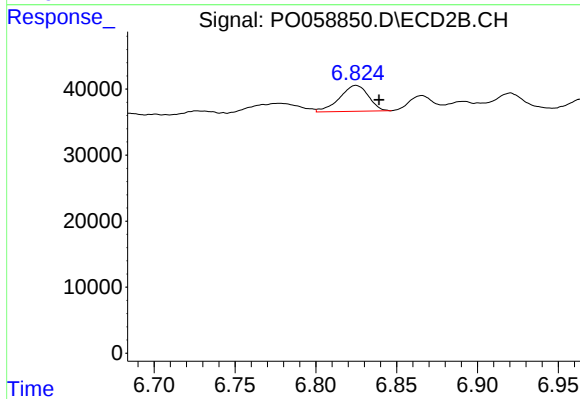

#34 AR-1260-4

R.T.: 6.825 min
Delta R.T.: -0.014 min
Response: 48880
Conc: 21.63 ng/ml

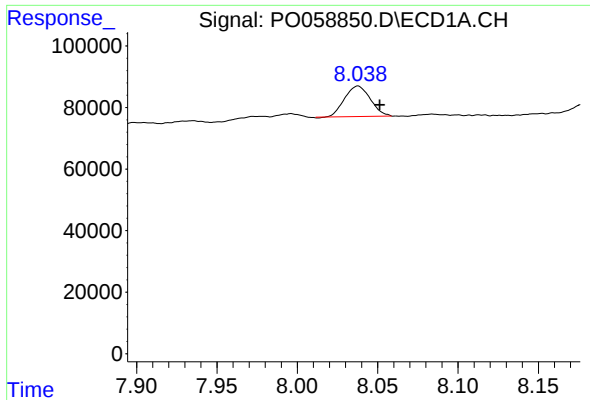


#35 AR-1260-5

R.T.: 8.038 min
Delta R.T.: -0.014 min
Response: 111394
Conc: 15.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-4

Manual Integrations
APPROVED

Ankita
8/6/2019 2:28:38 PM

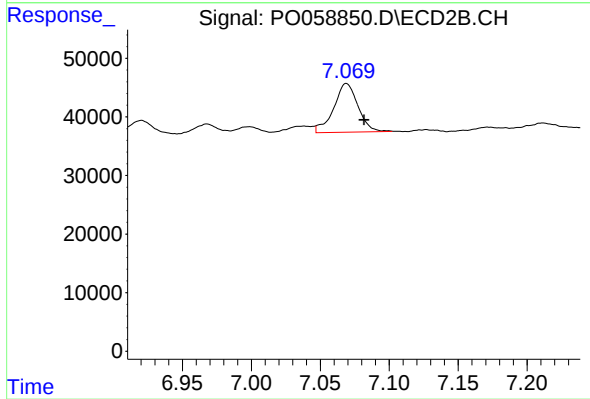

#35 AR-1260-5

R.T.: 7.069 min
Delta R.T.: -0.013 min
Response: 101776
Conc: 18.90 ng/ml m