

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
 Data File : P0058867.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2019 15:56
 Operator : SM/AJ
 Sample : K4135-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1S-A1-A4-COMP-(0-1)

Manual Integrations
 APPROVED

Ankita
 8/6/2019 2:29:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 18:31:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.157	3.516	958454	858628	22.711m	21.492
2) SA Decachlor...	9.631	8.399	880706	597194	16.263	15.129

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
Data File : P0058867.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2019 15:56
Operator : SM/AJ
Sample : K4135-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1S-A1-A4-COMP-(0-1)


Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 18:31:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

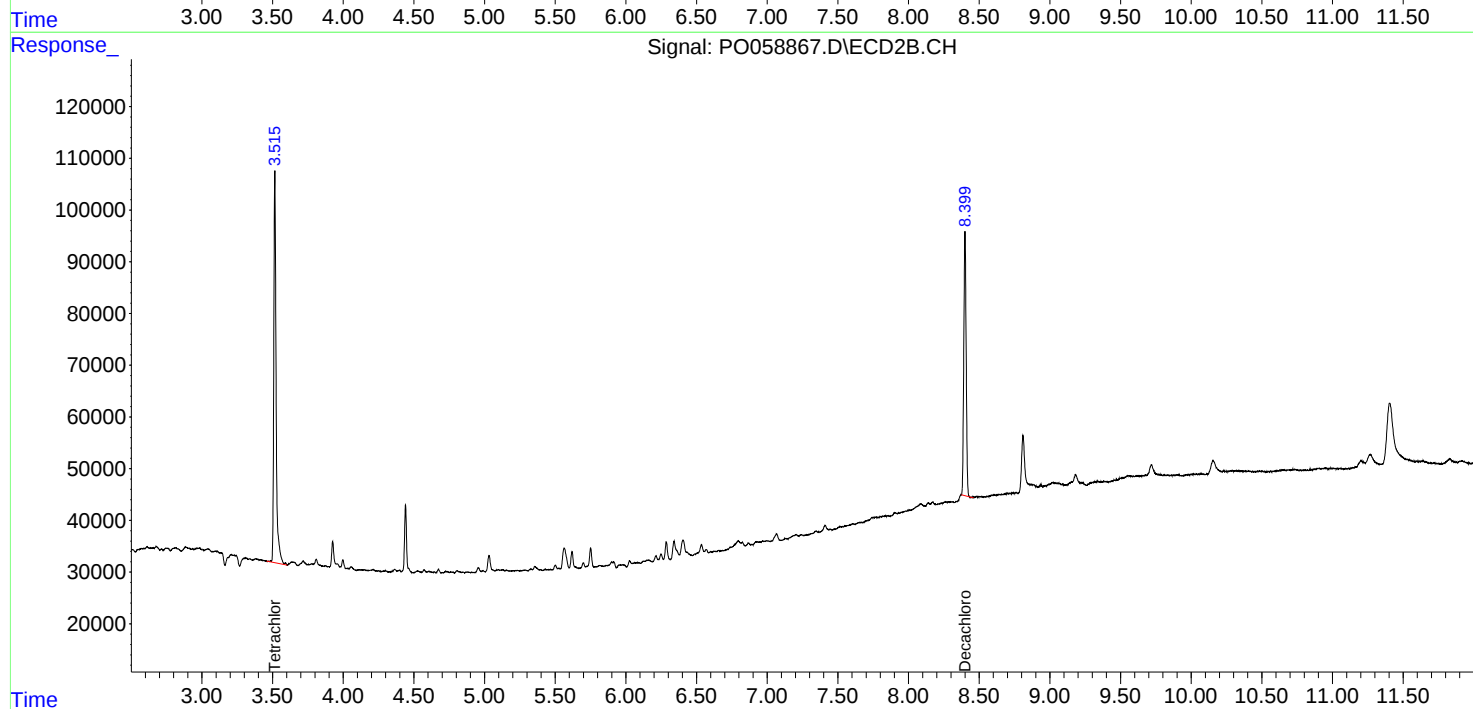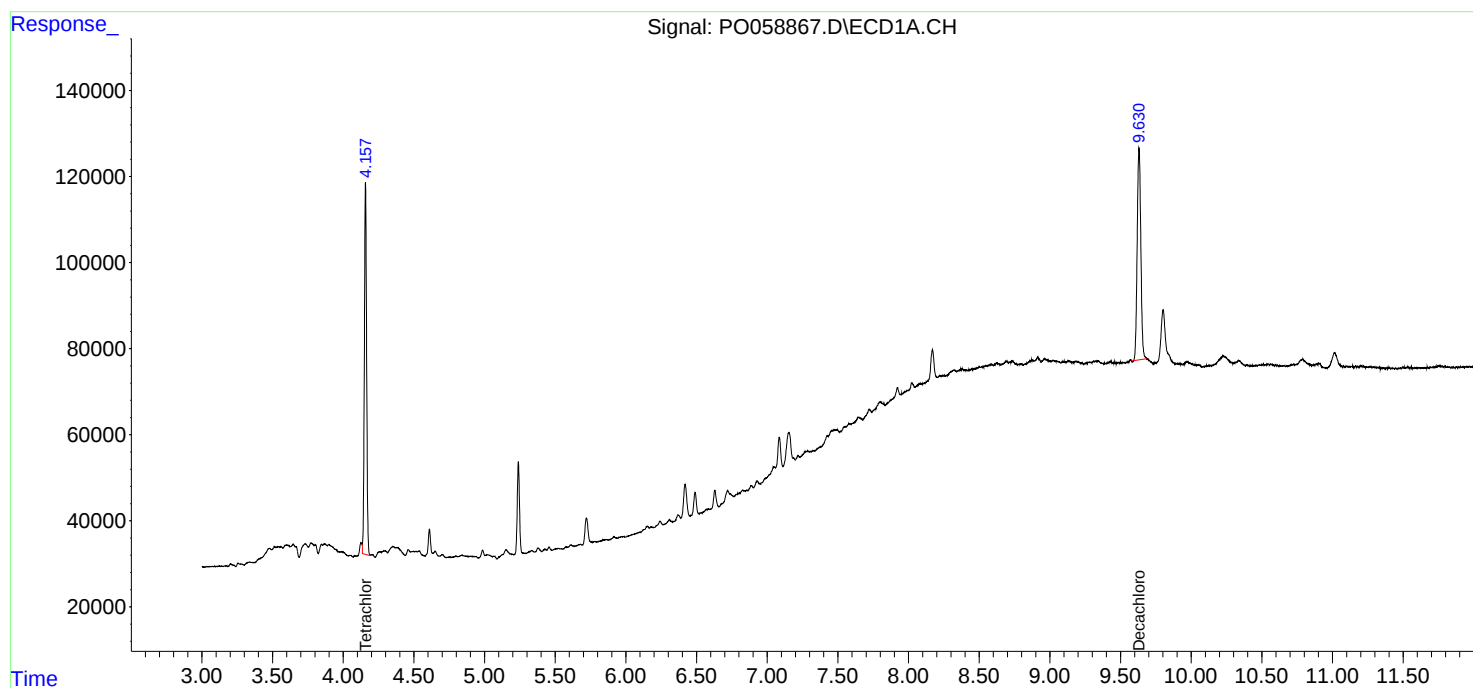

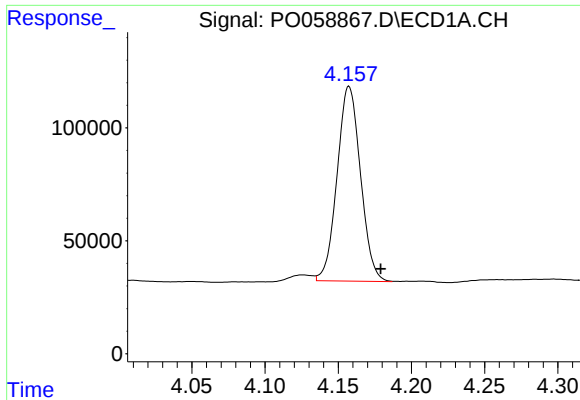


#1 Tetrachloro-m-xylene

R.T.: 4.157 min
Delta R.T.: -0.022 min
Response: 958454
Conc: 22.71 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1S-A1-A4-COMP-(0-1)


Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:17 PM

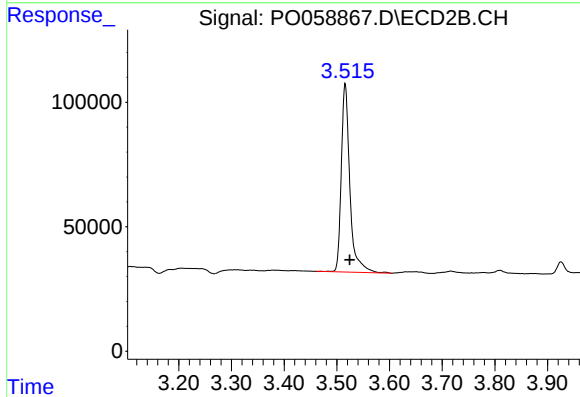


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 858628
Conc: 21.49 ng/ml

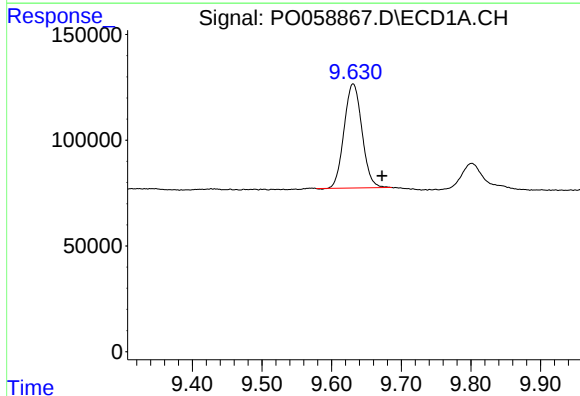

#2 Decachlorobiphenyl

R.T.: 9.631 min
Delta R.T.: -0.042 min
Response: 880706
Conc: 16.26 ng/ml

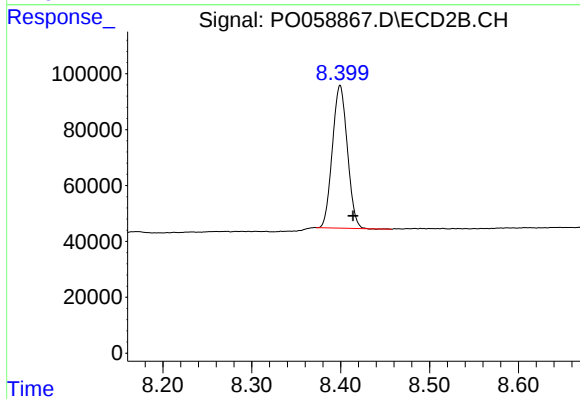

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.015 min
Response: 597194
Conc: 15.13 ng/ml