

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
 Data File : P0058890.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2019 22:51
 Operator : SM/AJ
 Sample : K4114-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-TEST-PIT

Manual Integrations
 APPROVED

Ankita
 8/6/2019 2:29:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 01:16:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.158	3.516	478143	374653	11.330	9.378
2) SA Decachlor...	9.670	8.399	356999	276789	6.592	7.012
Target Compounds						
31) L7 AR-1260-1	6.894	6.023	240757	178611	83.621	75.045
32) L7 AR-1260-2	7.148	6.214	565183	411358	135.860	135.793
33) L7 AR-1260-3	7.507	6.360	321088	157300	86.222	58.263m#
34) L7 AR-1260-4	7.733	6.824	267056	195695	78.367	86.609
35) L7 AR-1260-5	8.041	7.067	763234	640960	103.774	119.019

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080519\
Data File : PO058890.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2019 22:51
Operator : SM/AJ
Sample : K4114-01
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CS-TEST-PIT


Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 01:16:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

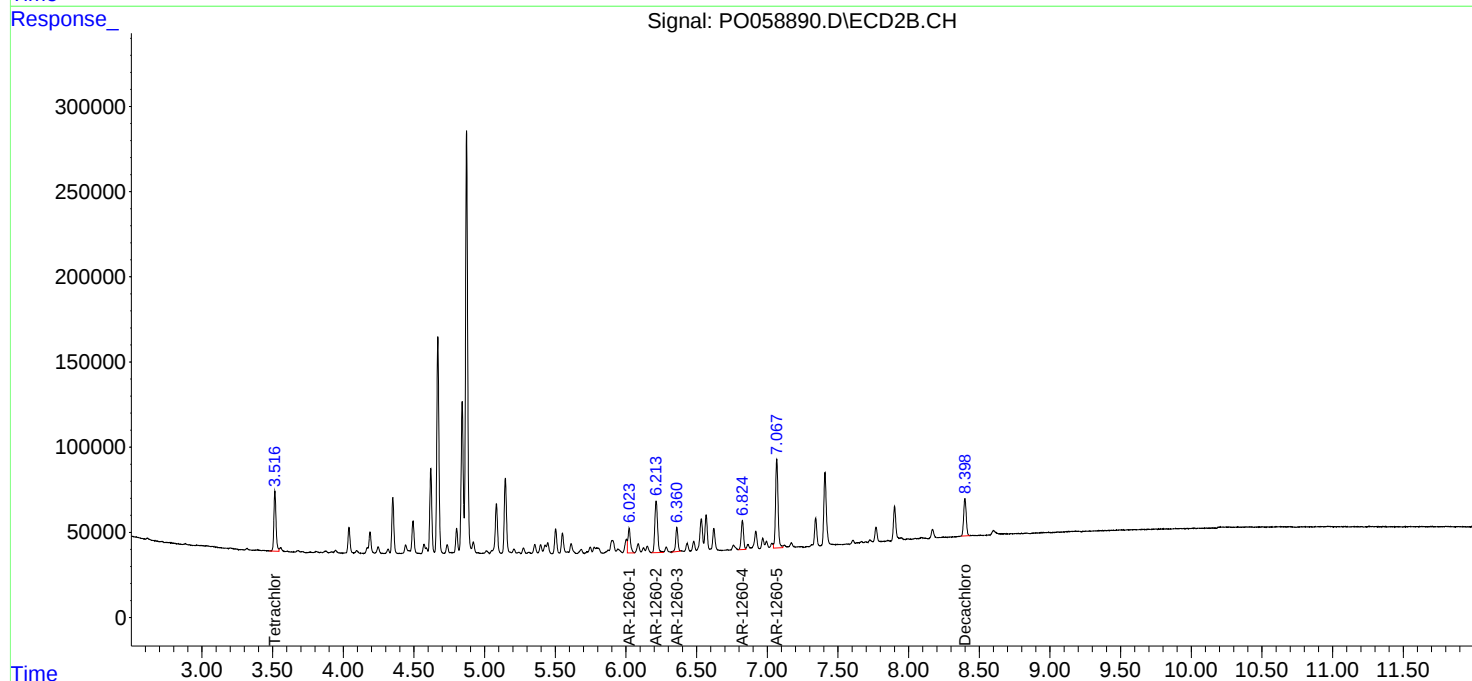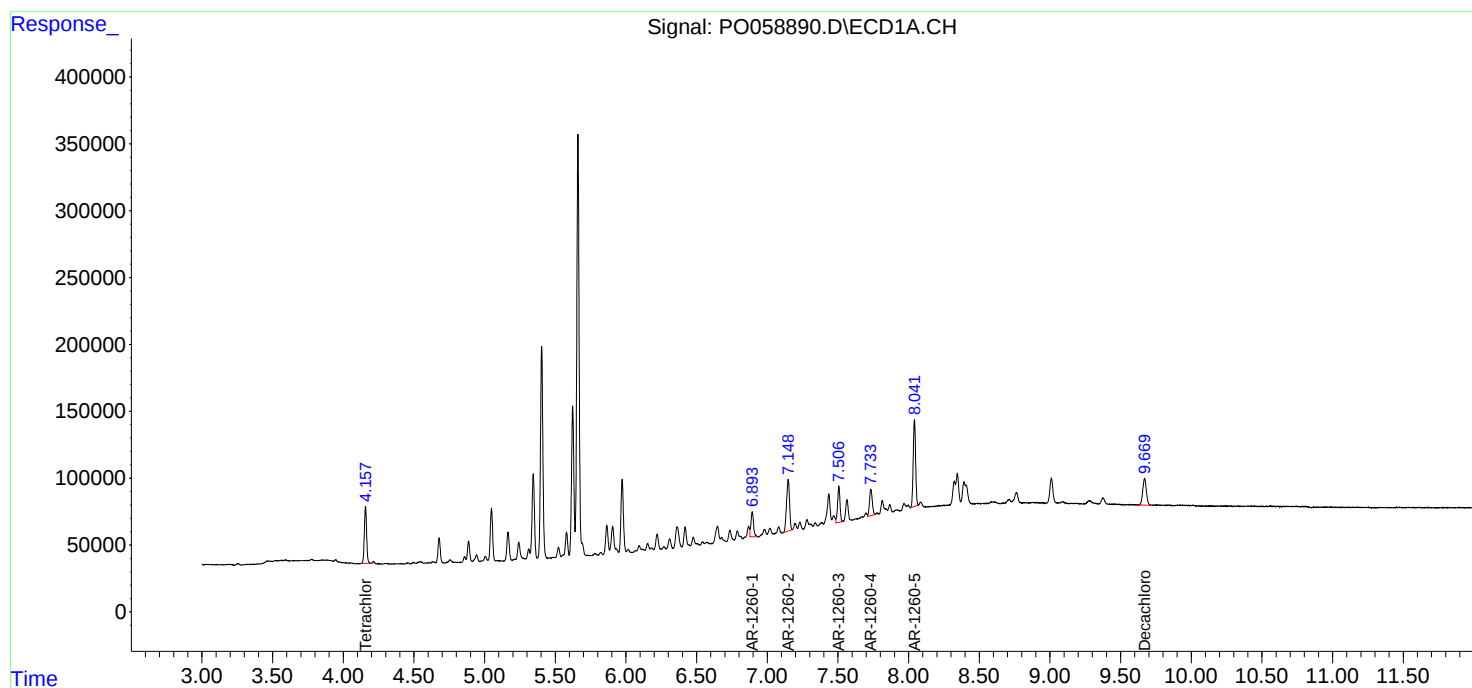

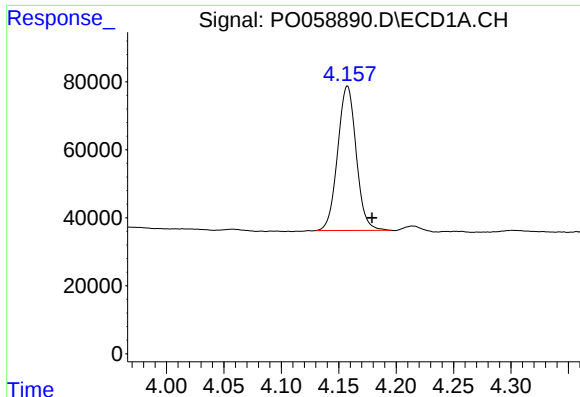


#1 Tetrachloro-m-xylene

R.T.: 4.158 min
Delta R.T.: -0.021 min
Response: 478143
Conc: 11.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PIT


Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:58 PM

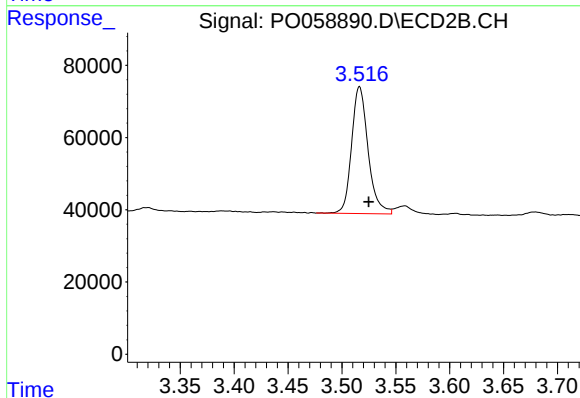


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.008 min
Response: 374653
Conc: 9.38 ng/ml

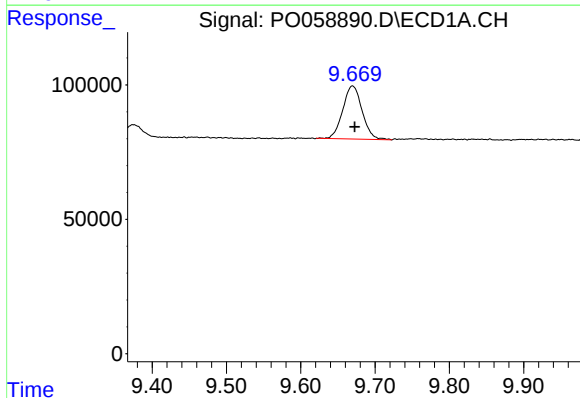


#2 Decachlorobiphenyl

R.T.: 9.670 min
Delta R.T.: -0.003 min
Response: 356999
Conc: 6.59 ng/ml

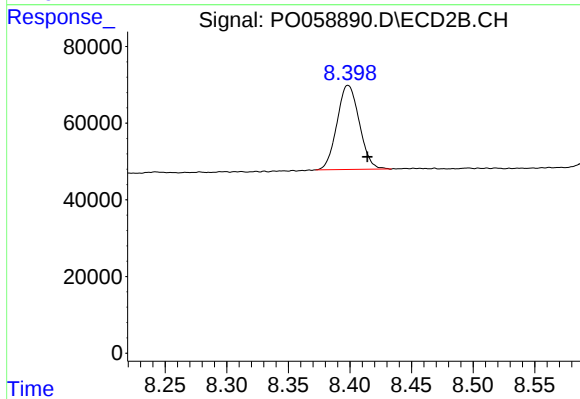

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.016 min
Response: 276789
Conc: 7.01 ng/ml

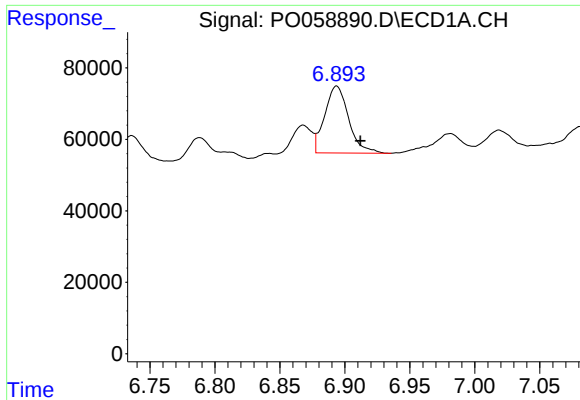


#31 AR-1260-1

R.T.: 6.894 min
Delta R.T.: -0.018 min
Response: 240757
Conc: 83.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PIT


Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:58 PM

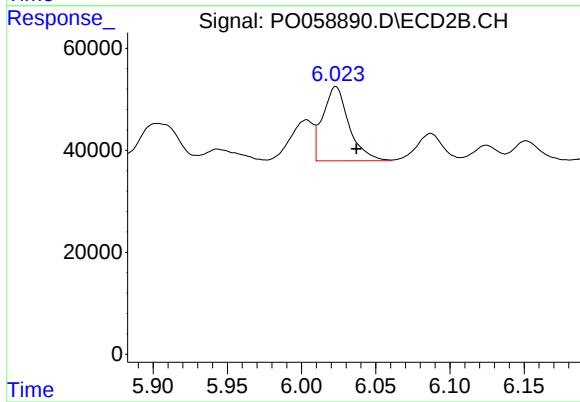


#31 AR-1260-1

R.T.: 6.023 min
Delta R.T.: -0.014 min
Response: 178611
Conc: 75.05 ng/ml

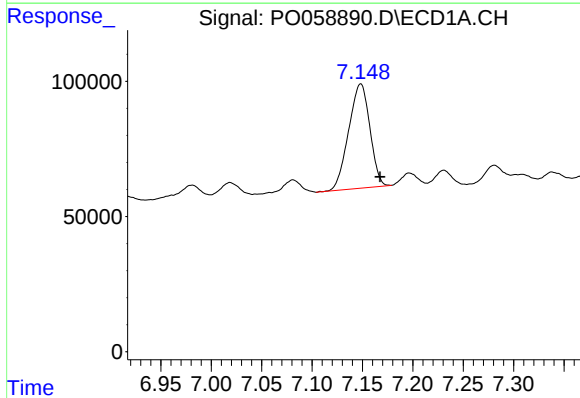


#32 AR-1260-2

R.T.: 7.148 min
Delta R.T.: -0.019 min
Response: 565183
Conc: 135.86 ng/ml

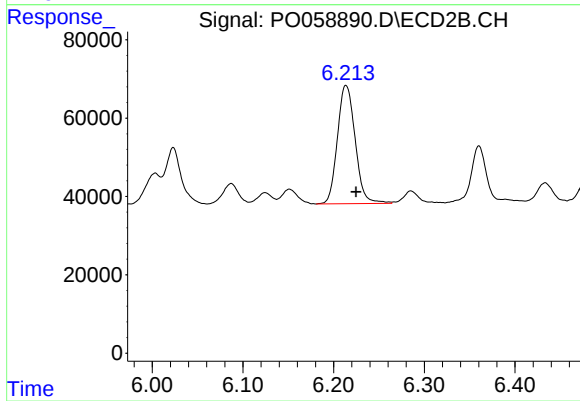

#32 AR-1260-2

R.T.: 6.214 min
Delta R.T.: -0.011 min
Response: 411358
Conc: 135.79 ng/ml

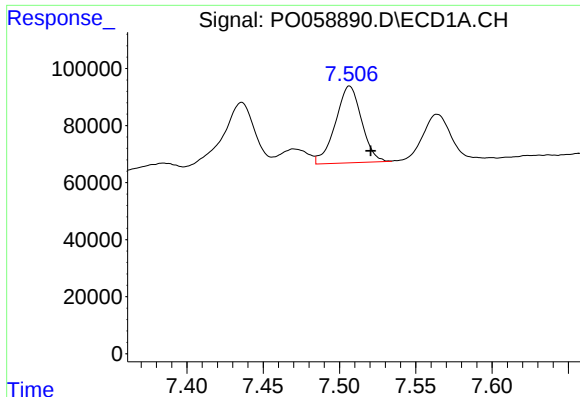


#33 AR-1260-3

R.T.: 7.507 min
Delta R.T.: -0.014 min
Response: 321088
Conc: 86.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PIT


Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:58 PM

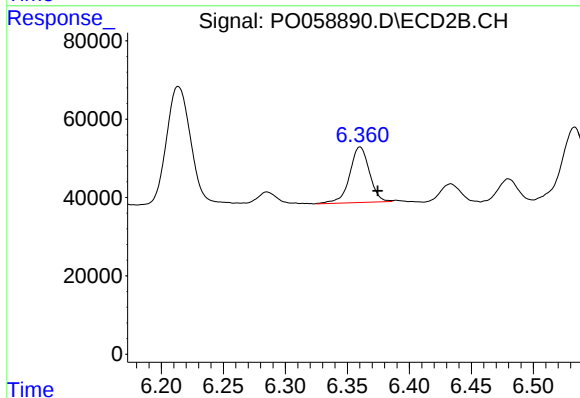


#33 AR-1260-3

R.T.: 6.360 min
Delta R.T.: -0.015 min
Response: 157300
Conc: 58.26 ng/ml m

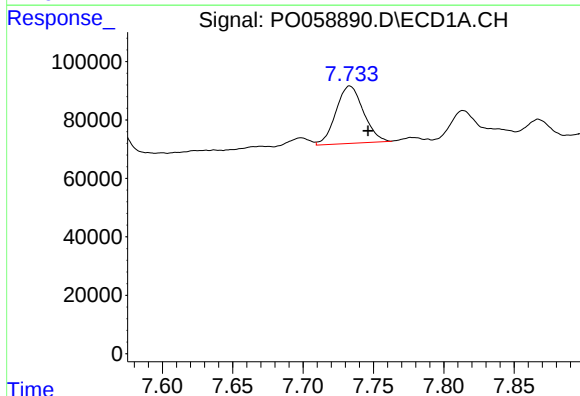


#34 AR-1260-4

R.T.: 7.733 min
Delta R.T.: -0.013 min
Response: 267056
Conc: 78.37 ng/ml

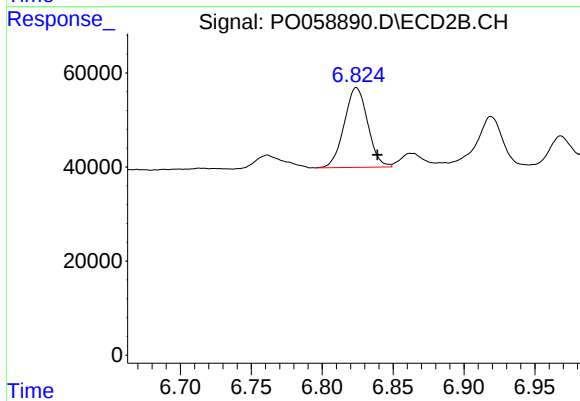

#34 AR-1260-4

R.T.: 6.824 min
Delta R.T.: -0.015 min
Response: 195695
Conc: 86.61 ng/ml

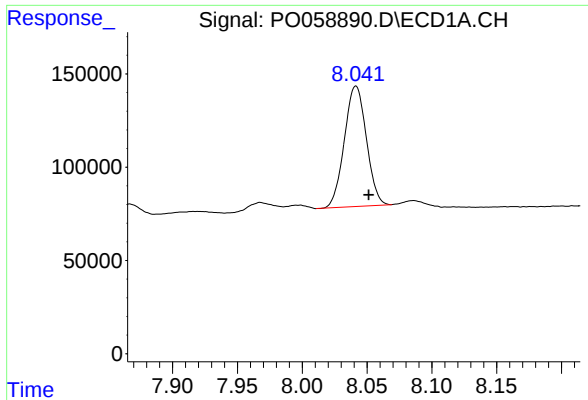


#35 AR-1260-5

R.T.: 8.041 min
Delta R.T.: -0.010 min
Response: 763234
Conc: 103.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PIT

Manual Integrations
APPROVED

Ankita
8/6/2019 2:29:58 PM

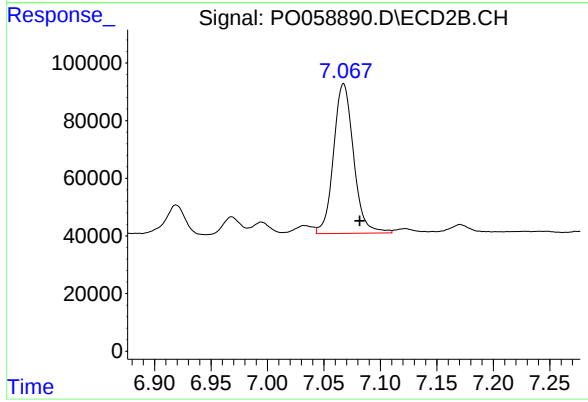

#35 AR-1260-5

R.T.: 7.067 min
Delta R.T.: -0.014 min
Response: 640960
Conc: 119.02 ng/ml