

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080519\
 Data File : P0058910.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2019 4:49
 Operator : SM/AJ
 Sample : K4170-12
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S17-03-S

Manual Integrations
 APPROVED

Ankita
 8/6/2019 2:30:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 06:54:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.152	3.514	1138299	944960	26.972m	23.654
2) SA Decachlor...	9.658	8.397	1061214	833131	19.596	21.106
Target Compounds						
26) L6 AR-1254-1	6.147	5.354	297787	269181	126.112m	103.909
27) L6 AR-1254-2	6.363	5.500	755810	447446	196.113m	195.440
28) L6 AR-1254-3	6.729	5.897	987351	844074	243.812	229.408
29) L6 AR-1254-4	7.014	6.123	1053957	640944	292.714m	275.650
30) L6 AR-1254-5	7.430	6.533	1461911	1350506	403.312m	391.501m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080519\
Data File : PO058910.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2019 4:49
Operator : SM/AJ
Sample : K4170-12
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S17-03-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 06:54:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

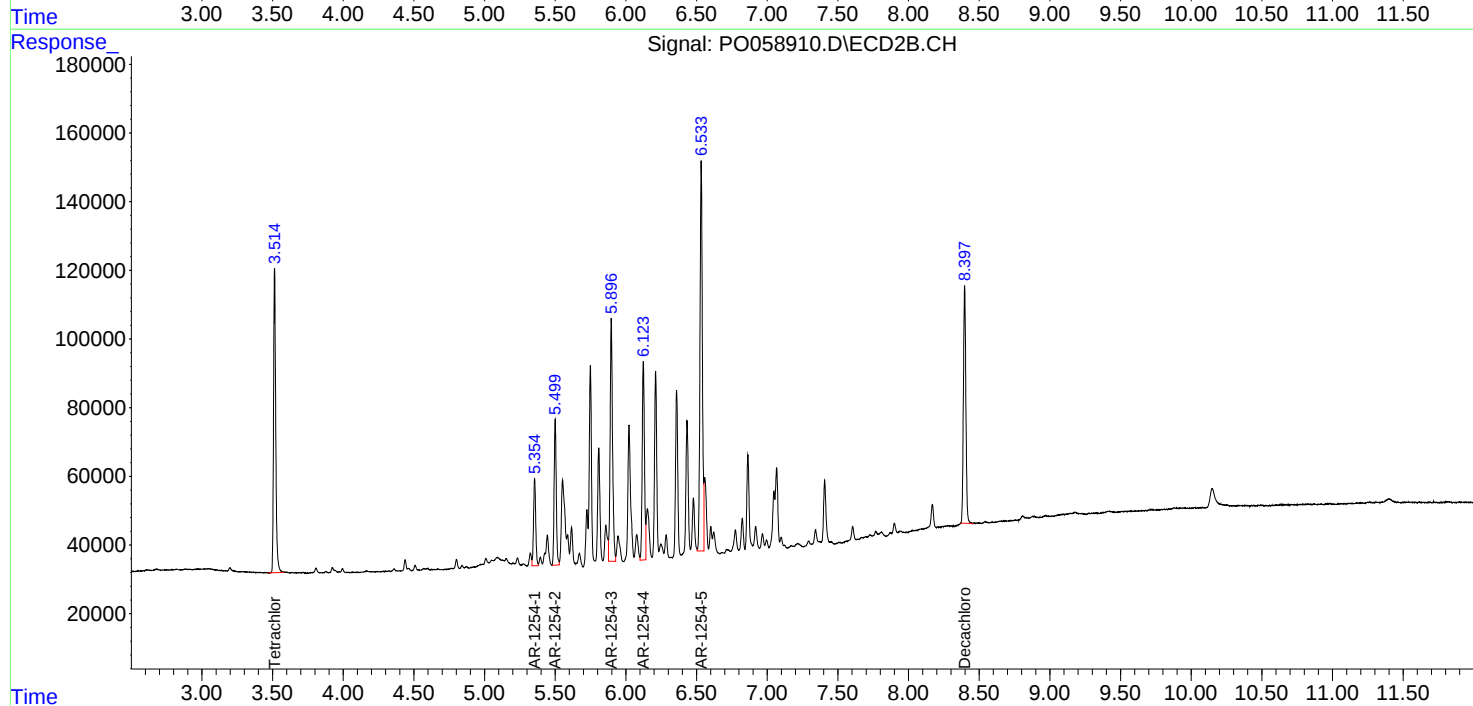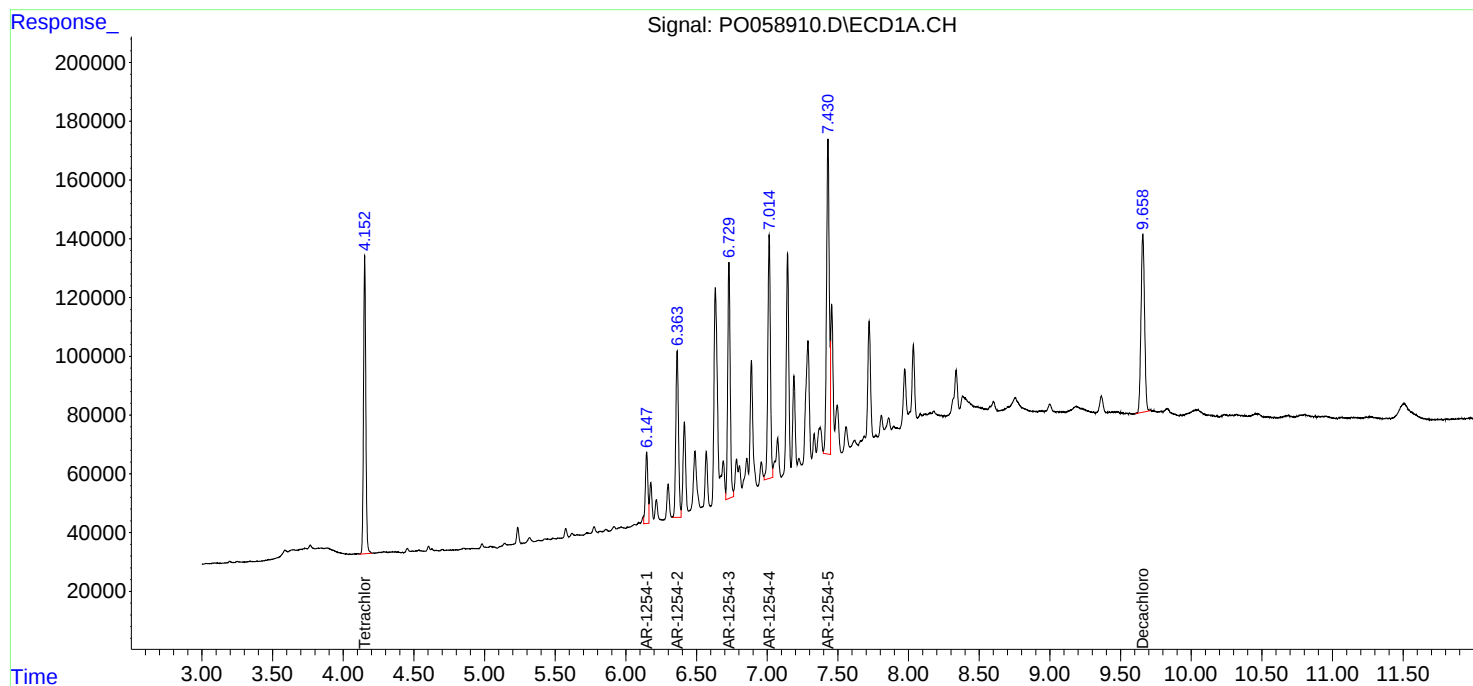

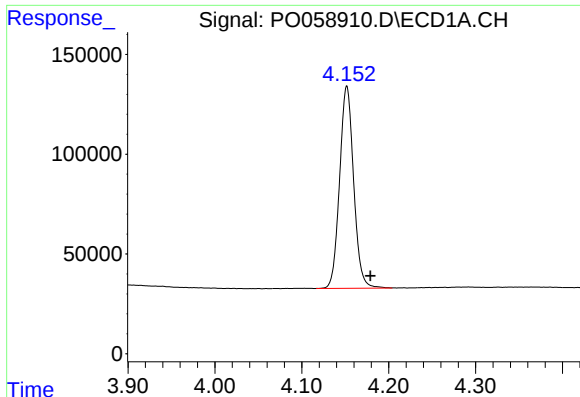


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.027 min
Response: 1138299
Conc: 26.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S17-03-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:36 PM

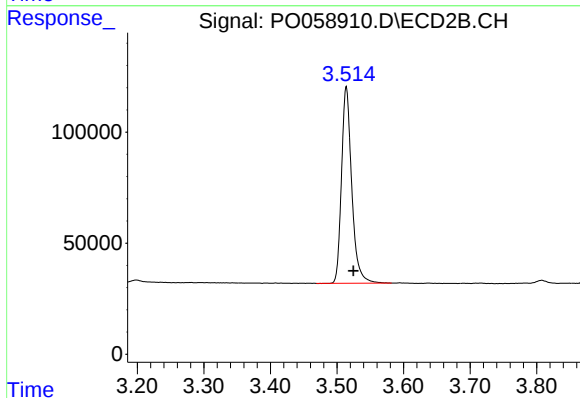


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: -0.011 min
Response: 944960
Conc: 23.65 ng/ml

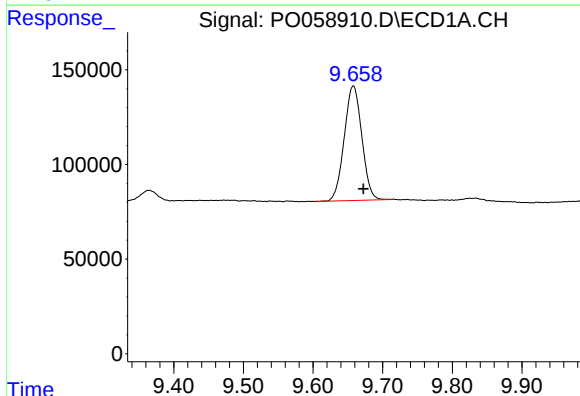


#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.015 min
Response: 1061214
Conc: 19.60 ng/ml

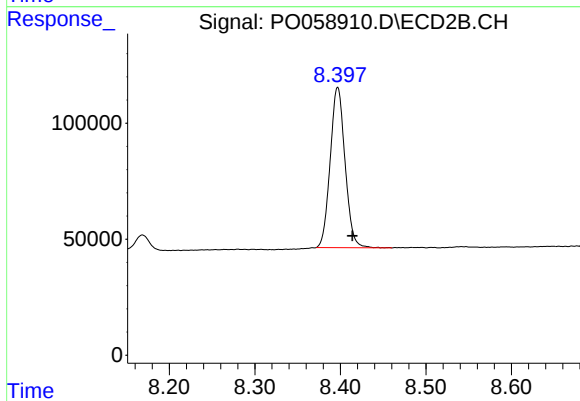

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.017 min
Response: 833131
Conc: 21.11 ng/ml

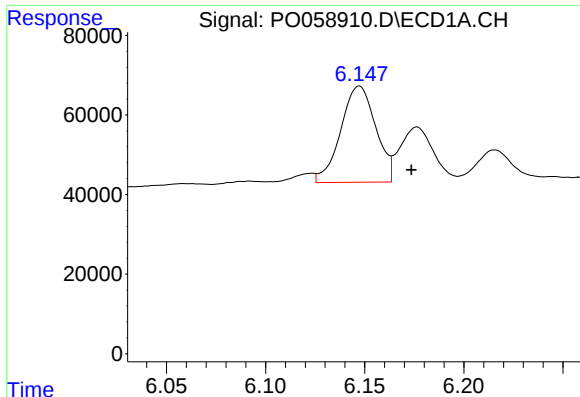


#26 AR-1254-1

R.T.: 6.147 min
Delta R.T.: -0.026 min
Response: 297787
Conc: 126.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S17-03-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:36 PM

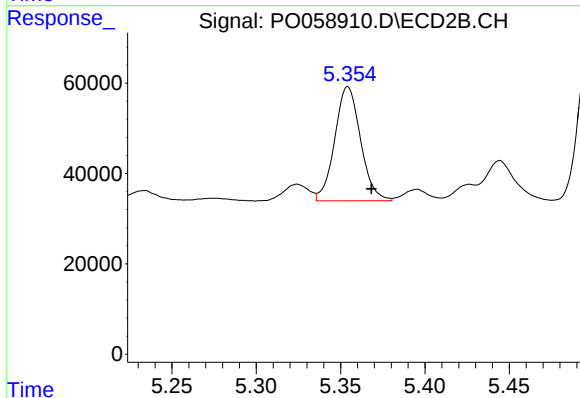


#26 AR-1254-1

R.T.: 5.354 min
Delta R.T.: -0.014 min
Response: 269181
Conc: 103.91 ng/ml

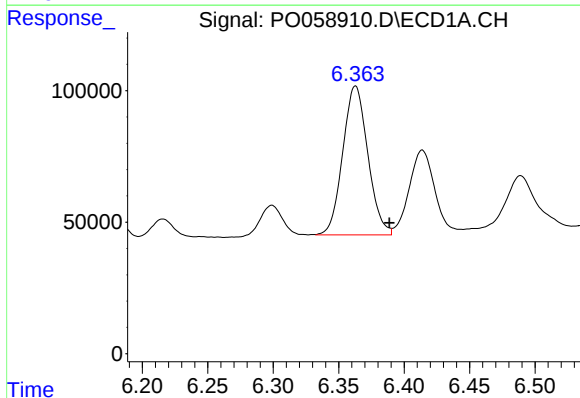


#27 AR-1254-2

R.T.: 6.363 min
Delta R.T.: -0.026 min
Response: 755810
Conc: 196.11 ng/ml m

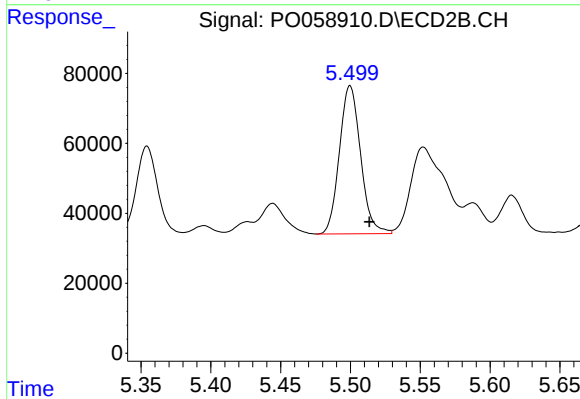

#27 AR-1254-2

R.T.: 5.500 min
Delta R.T.: -0.014 min
Response: 447446
Conc: 195.44 ng/ml

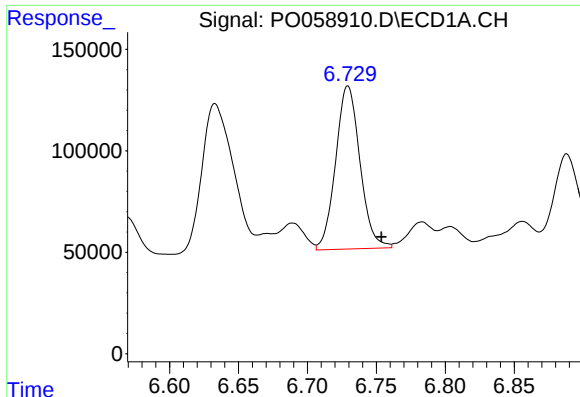


#28 AR-1254-3

R.T.: 6.729 min
Delta R.T.: -0.024 min
Response: 987351
Conc: 243.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
S17-03-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:36 PM

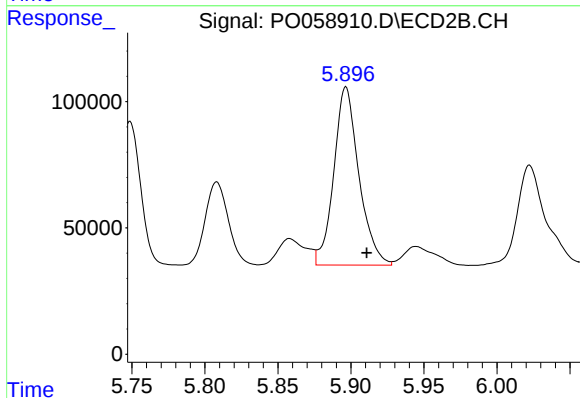


#28 AR-1254-3

R.T.: 5.897 min
Delta R.T.: -0.014 min
Response: 844074
Conc: 229.41 ng/ml

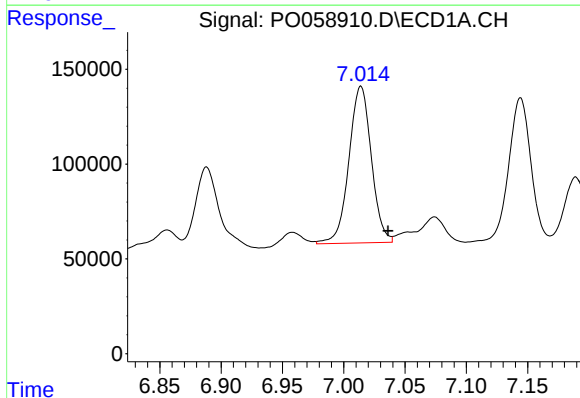


#29 AR-1254-4

R.T.: 7.014 min
Delta R.T.: -0.023 min
Response: 1053957
Conc: 292.71 ng/ml m

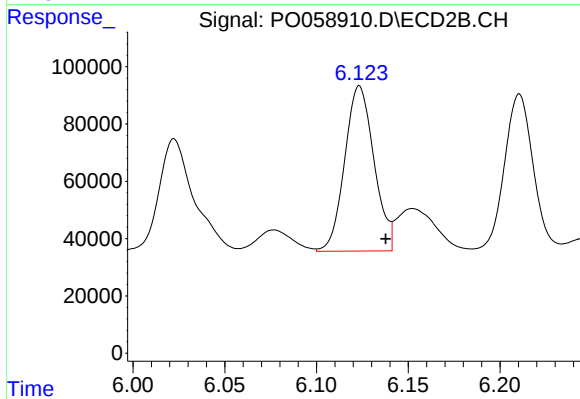

#29 AR-1254-4

R.T.: 6.123 min
Delta R.T.: -0.014 min
Response: 640944
Conc: 275.65 ng/ml

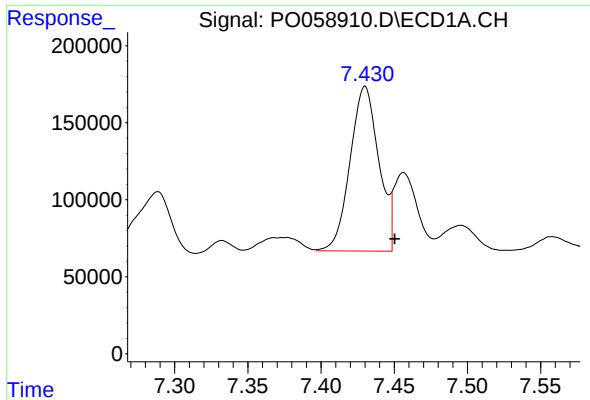


#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: -0.021 min
Response: 1461911
Conc: 403.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S17-03-S

Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:36 PM

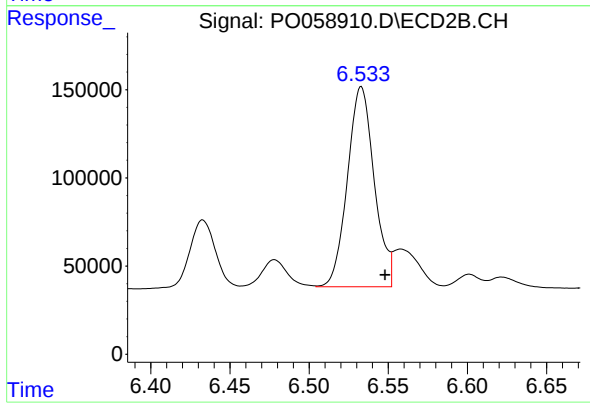

#30 AR-1254-5

R.T.: 6.533 min
Delta R.T.: -0.016 min
Response: 1350506
Conc: 391.50 ng/ml m