

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080519\
 Data File : P0058912.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2019 6:26
 Operator : SM/AJ
 Sample : K4171-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S7-01-S

Manual Integrations
 APPROVED

Ankita
 8/6/2019 2:30:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 10:38:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.151	3.515	1233214	911410	29.221m	22.814
2) SA Decachlor...	9.649	8.395	1244052	985834	22.972	24.975m
Target Compounds						
41) L9 AR-1268-1	8.303	7.340	1354826	795094	121.297m	97.617
42) L9 AR-1268-2	8.390	7.407	1064354	1171789	113.312m	154.648 #
43) L9 AR-1268-3	8.591	7.603	420383	371773	50.899m	58.163
44) L9 AR-1268-4	8.990	7.899	595221	490869	199.118m	211.520m
45) L9 AR-1268-5	9.357	8.167	1288076	1003485	59.996	58.553m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080519\
Data File : PO058912.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2019 6:26
Operator : SM/AJ
Sample : K4171-01
Misc :
ALS Vial : 61 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S7-01-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 10:38:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

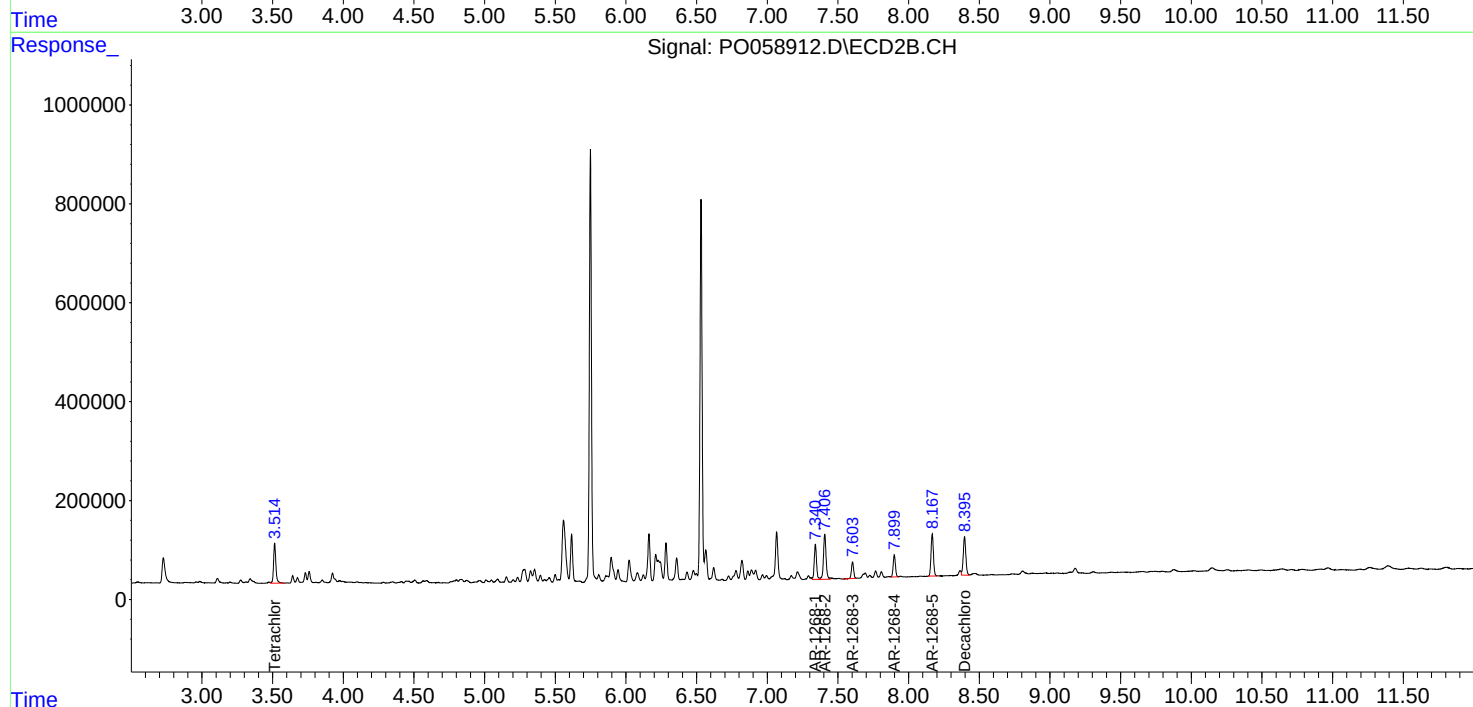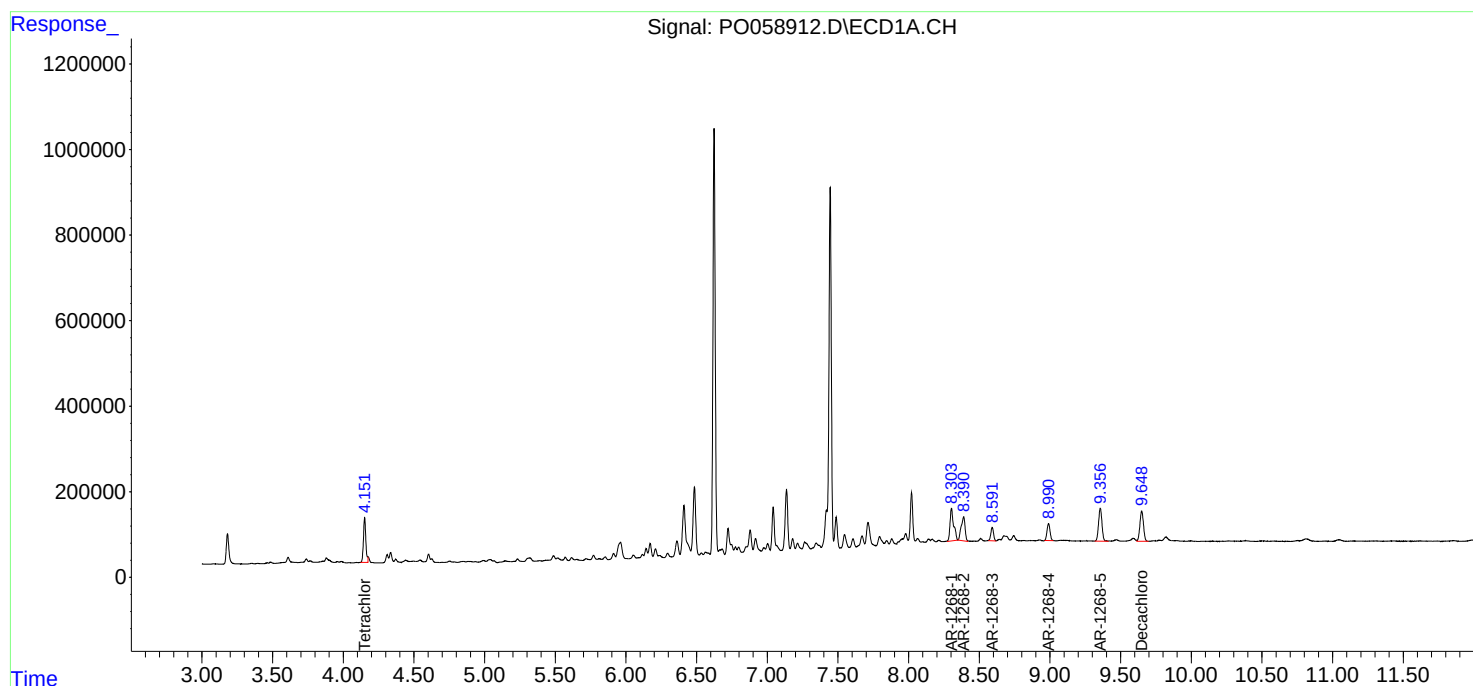

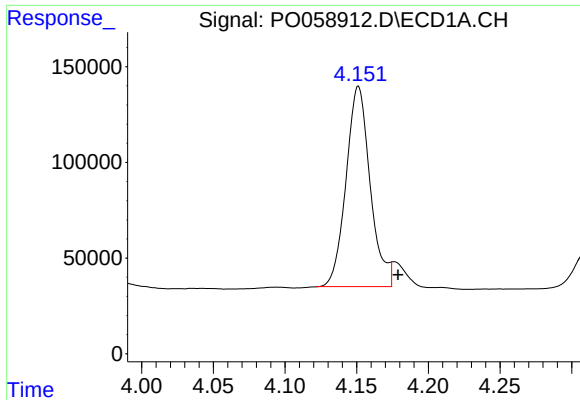


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.028 min
Response: 1233214
Conc: 29.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S7-01-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:41 PM

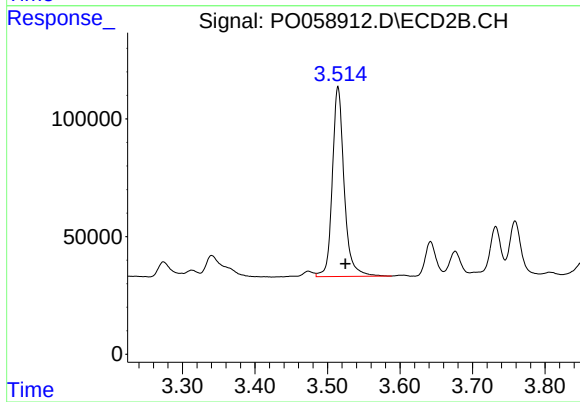


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: -0.010 min
Response: 911410
Conc: 22.81 ng/ml

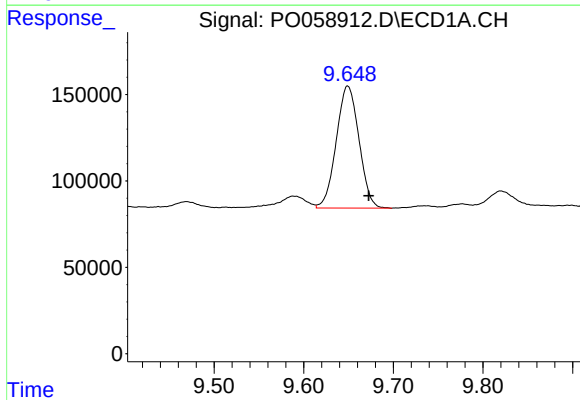


#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.024 min
Response: 1244052
Conc: 22.97 ng/ml

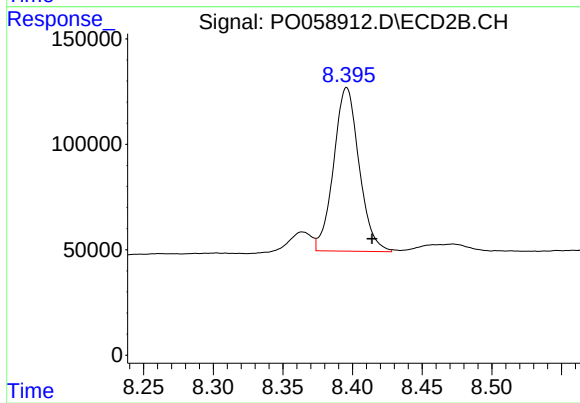

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: -0.019 min
Response: 985834
Conc: 24.97 ng/ml m

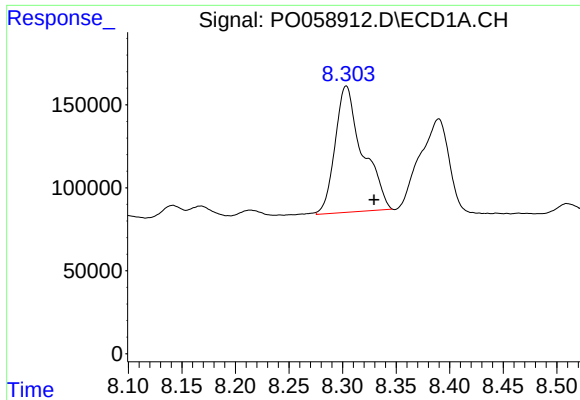


#41 AR-1268-1

R.T.: 8.303 min
Delta R.T.: -0.026 min
Response: 1354826
Conc: 121.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S7-01-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:41 PM

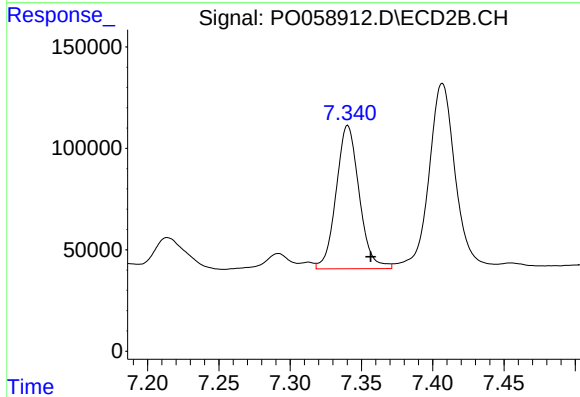


#41 AR-1268-1

R.T.: 7.340 min
Delta R.T.: -0.016 min
Response: 795094
Conc: 97.62 ng/ml

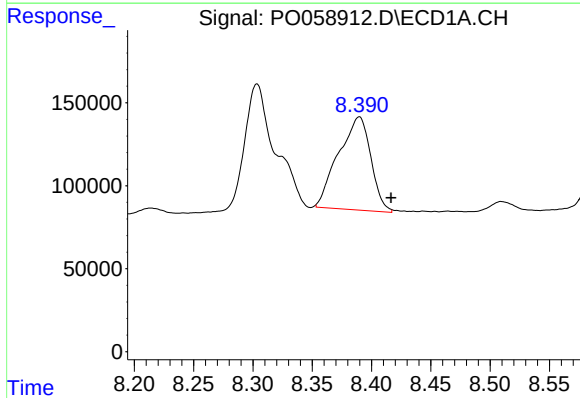


#42 AR-1268-2

R.T.: 8.390 min
Delta R.T.: -0.027 min
Response: 1064354
Conc: 113.31 ng/ml m

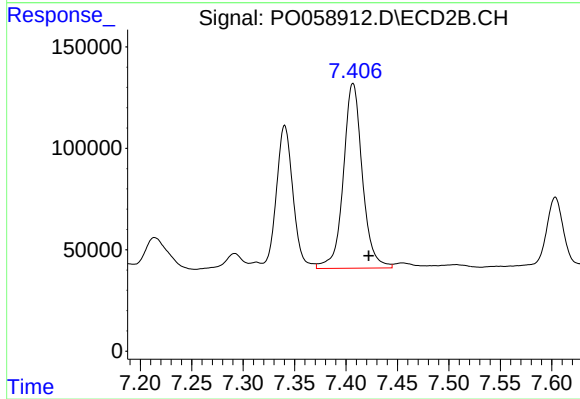

#42 AR-1268-2

R.T.: 7.407 min
Delta R.T.: -0.015 min
Response: 1171789
Conc: 154.65 ng/ml

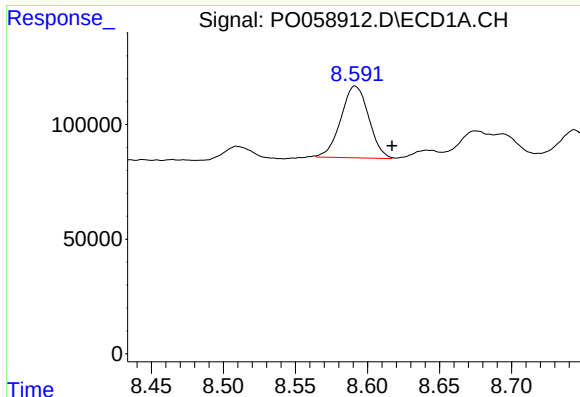


#43 AR-1268-3

R.T.: 8.591 min
Delta R.T.: -0.026 min
Response: 420383
Conc: 50.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S7-01-S


Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:41 PM

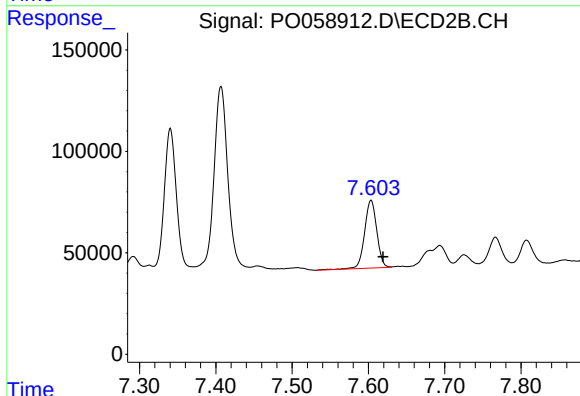


#43 AR-1268-3

R.T.: 7.603 min
Delta R.T.: -0.016 min
Response: 371773
Conc: 58.16 ng/ml

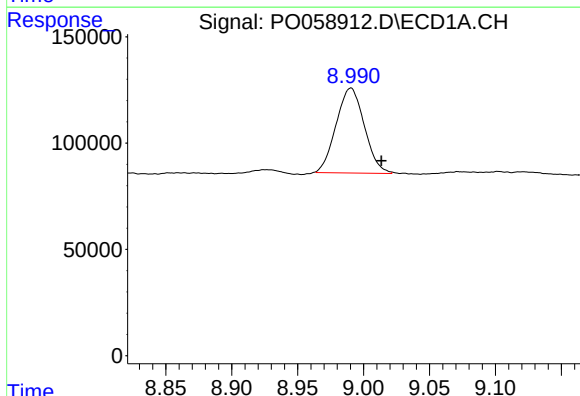


#44 AR-1268-4

R.T.: 8.990 min
Delta R.T.: -0.023 min
Response: 595221
Conc: 199.12 ng/ml m

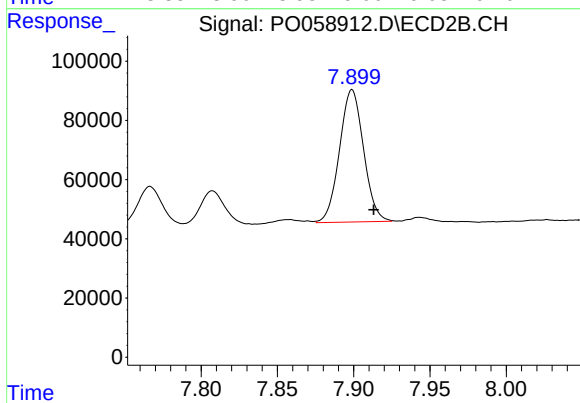

#44 AR-1268-4

R.T.: 7.899 min
Delta R.T.: -0.015 min
Response: 490869
Conc: 211.52 ng/ml m

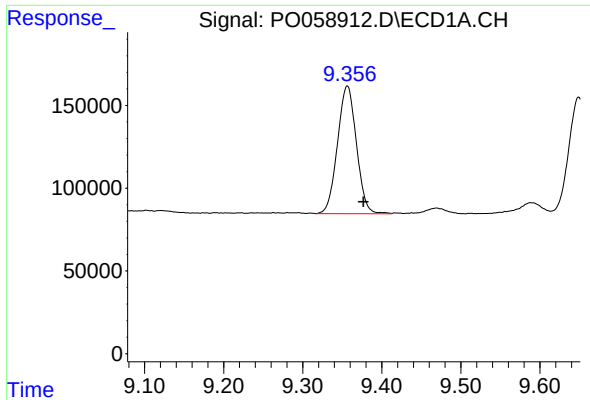


#45 AR-1268-5

R.T.: 9.357 min
Delta R.T.: -0.020 min
Response: 1288076
Conc: 60.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-01-S

Manual Integrations
APPROVED

Ankita
8/6/2019 2:30:41 PM

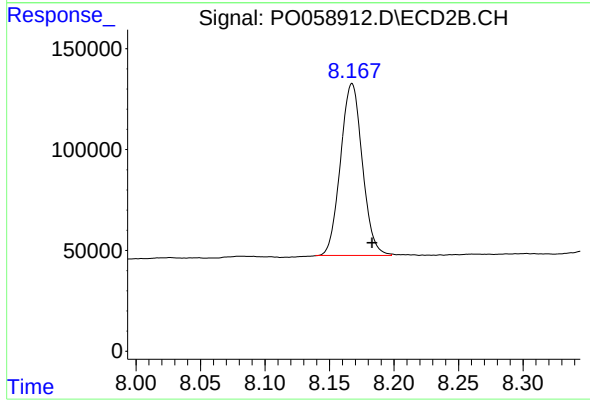

#45 AR-1268-5

R.T.: 8.167 min
Delta R.T.: -0.016 min
Response: 1003485
Conc: 58.55 ng/ml m