

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
 Data File : P0080216.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2021 18:34
 Operator : DD\AJ
 Sample : M3279-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20210572-COM-45

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 00:19:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.996	4.114	1301628	506545	21.601	22.119
2)	SA Decachlor...	11.102	9.518	877820	403323	18.713	19.408
Target Compounds							
4)	L1 AR-1016-2	0.000	5.411	0	9972	N.D.	7.838 #
5)	L1 AR-1016-3	0.000	5.610	0	79657	N.D.	112.986 #
6)	L1 AR-1016-4	0.000	5.660	0	149555	N.D.	247.499 #
7)	L1 AR-1016-5	0.000	5.898	0	126031	N.D.	171.133 #
9)	L2 AR-1221-2	0.000	4.472	0	12151	N.D.	56.657 #
10)	L2 AR-1221-3	0.000	4.573	0	4186	N.D.	6.448 #
11)	L3 AR-1232-1	0.000	4.573	0	4186	N.D.	6.942 #
12)	L3 AR-1232-2	6.041	5.411	605718	9972	867.113	17.732 #
13)	L3 AR-1232-3	0.000	5.610	0	79657	N.D.	264.587 #
14)	L3 AR-1232-4	0.000	5.700	0	141366	N.D.	496.596 #
15)	L3 AR-1232-5	0.000	5.898	0	126031	N.D.	419.666 #
17)	L4 AR-1242-2	0.000	5.411	0	9972	N.D.	10.297 #
18)	L4 AR-1242-3	0.000	5.610	0	79657	N.D.	148.459 #
19)	L4 AR-1242-4	0.000	5.700	0	141366	N.D.	251.756 #
22)	L5 AR-1248-2	0.000	5.660	0	149555	N.D.	181.524 #
23)	L5 AR-1248-3	0.000	5.700	0	141366	N.D.	170.342 #
24)	L5 AR-1248-4	0.000	5.898	0	126031	N.D.	133.377 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080521\
Data File : PO080216.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2021 18:34
Operator : DD\AJ
Sample : M3279-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 00:19:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

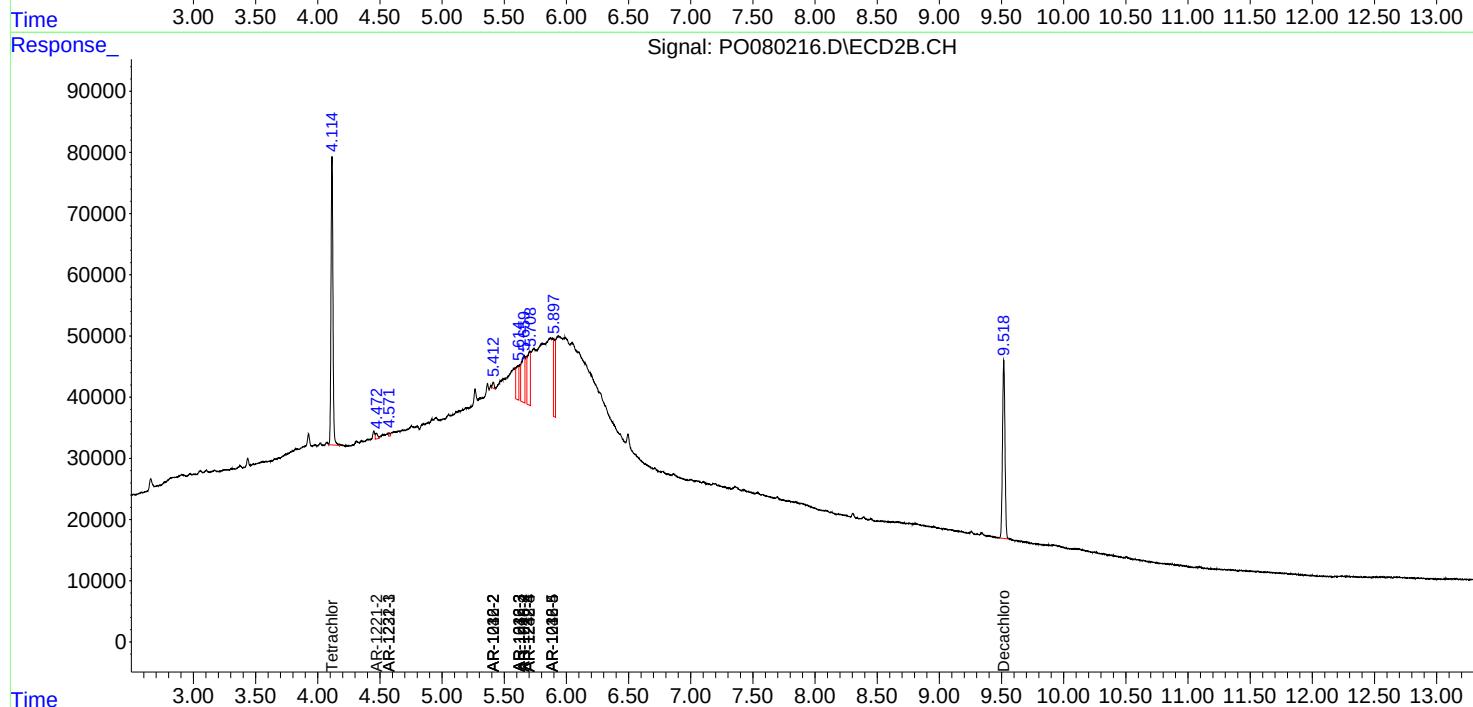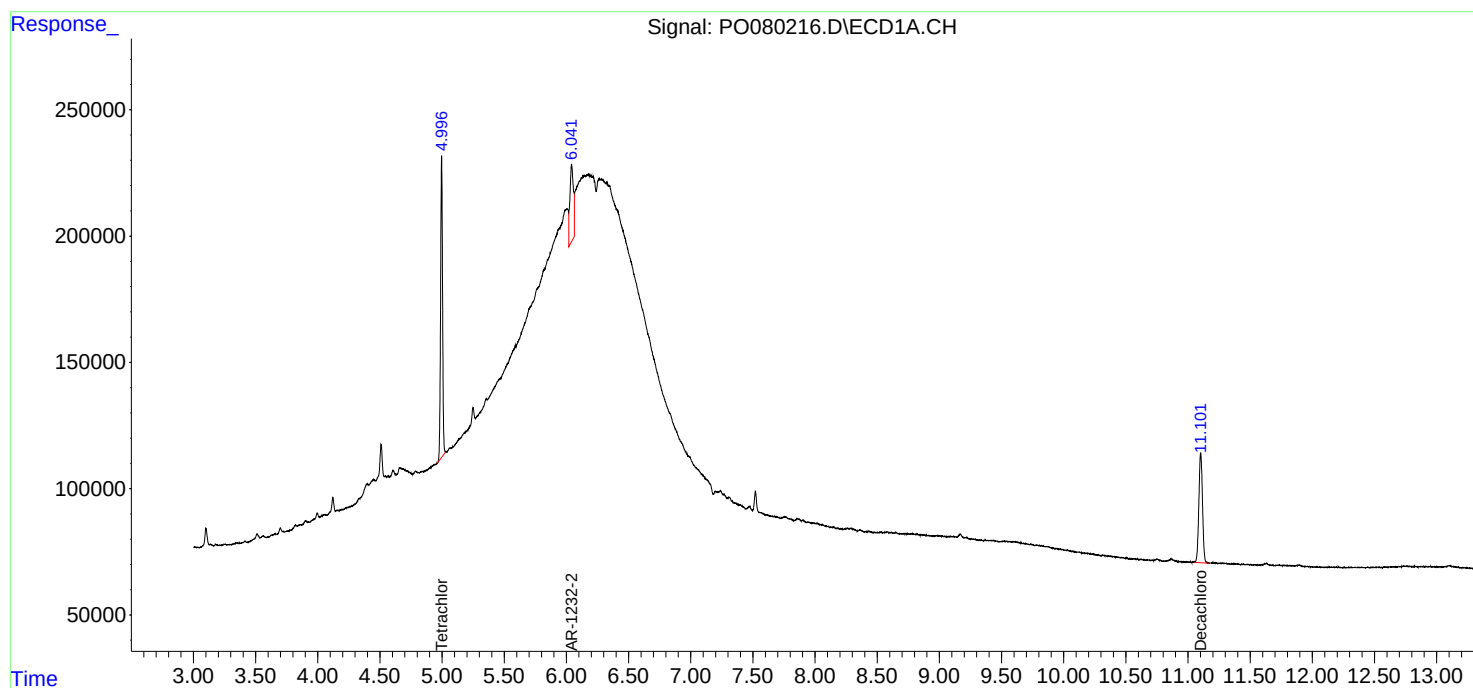


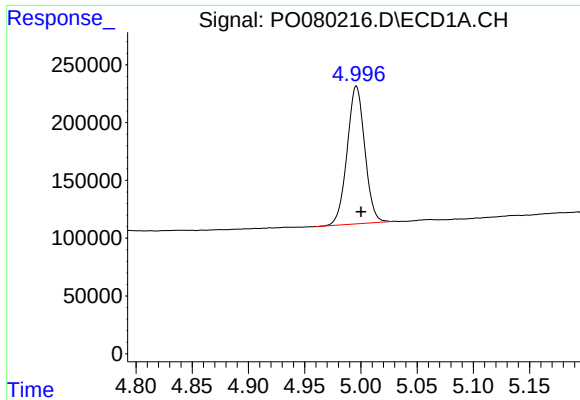

#1 Tetrachloro-m-xylene


R.T.: 4.996 min
Delta R.T.: -0.004 min
Response: 1301628
Conc: 21.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

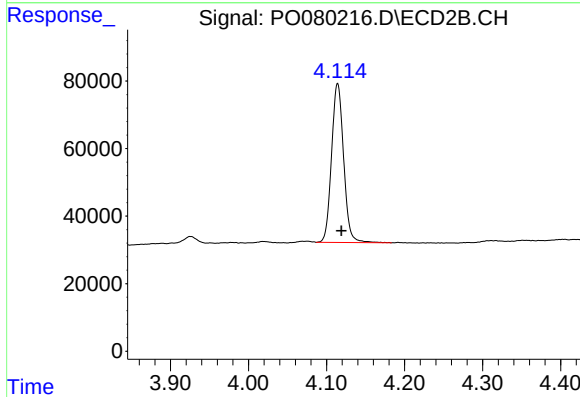


#1 Tetrachloro-m-xylene

R.T.: 4.114 min
Delta R.T.: -0.005 min
Response: 506545
Conc: 22.12 ng/ml

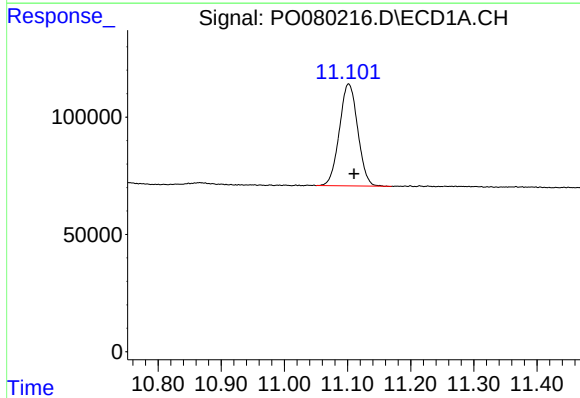


#2 Decachlorobiphenyl

R.T.: 11.102 min
Delta R.T.: -0.009 min
Response: 877820
Conc: 18.71 ng/ml

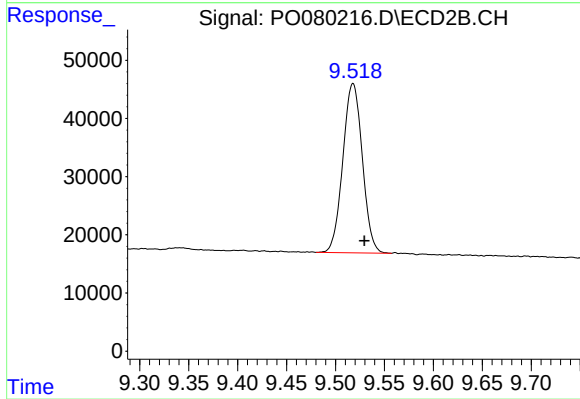

#2 Decachlorobiphenyl


R.T.: 9.518 min
Delta R.T.: -0.011 min
Response: 403323
Conc: 19.41 ng/ml

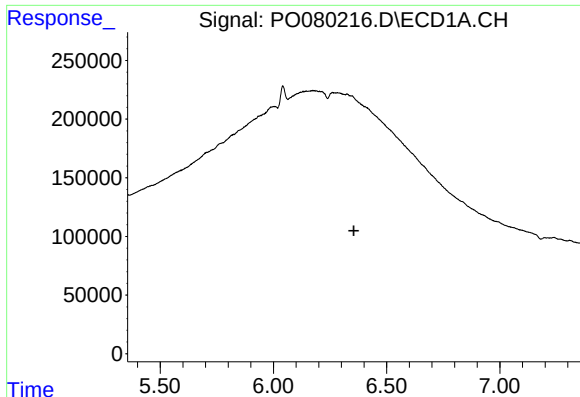

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T.: 6.356 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

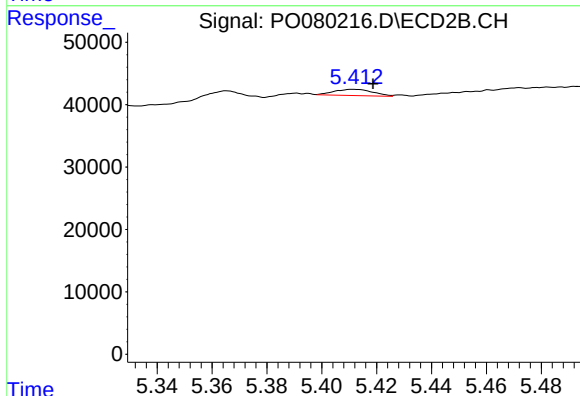


#4 AR-1016-2

R.T.: 5.411 min
Delta R.T.: -0.007 min
Response: 9972
Conc: 7.84 ng/ml

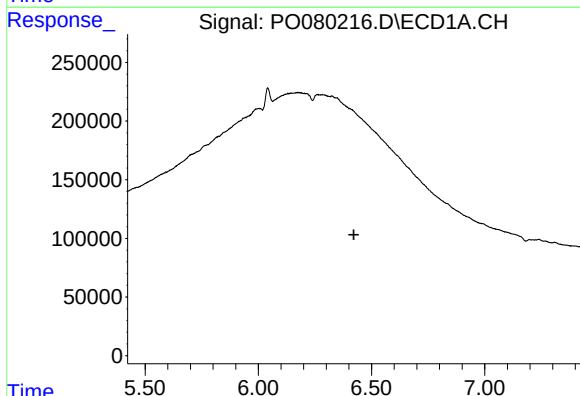


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T.: 6.422 min
Response: 0
Conc: N.D.

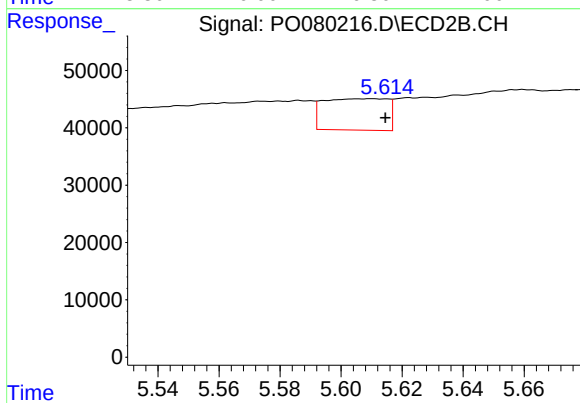

#5 AR-1016-3


R.T.: 5.610 min
Delta R.T.: -0.004 min
Response: 79657
Conc: 112.99 ng/ml

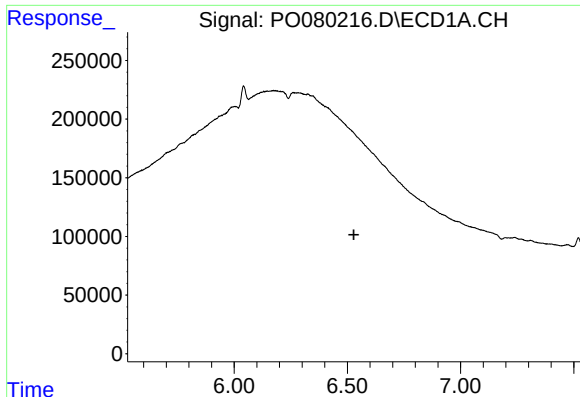

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 6.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

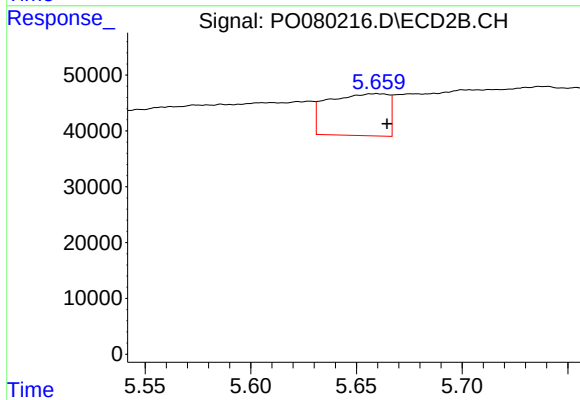


#6 AR-1016-4

R.T.: 5.660 min
Delta R.T.: -0.005 min
Response: 149555
Conc: 247.50 ng/ml

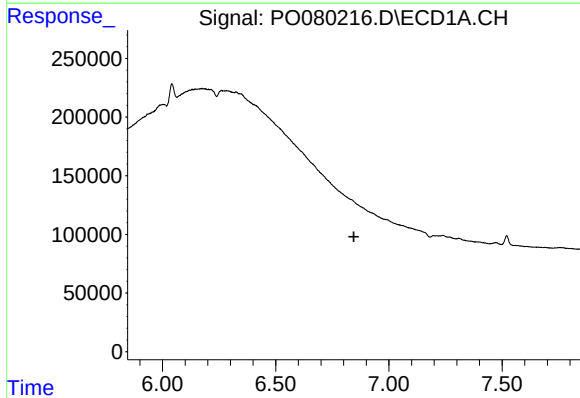


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T.: 6.845 min
Response: 0
Conc: N.D.

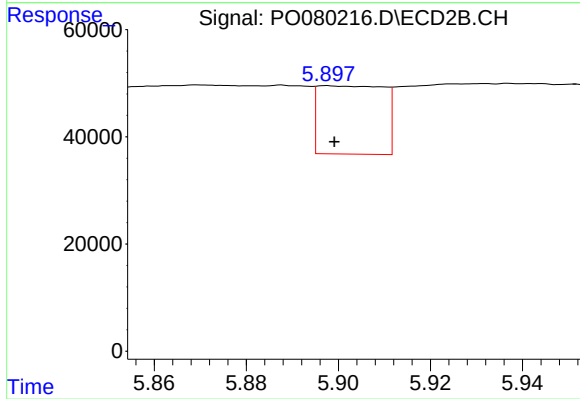

#7 AR-1016-5


R.T.: 5.898 min
Delta R.T.: -0.002 min
Response: 126031
Conc: 171.13 ng/ml

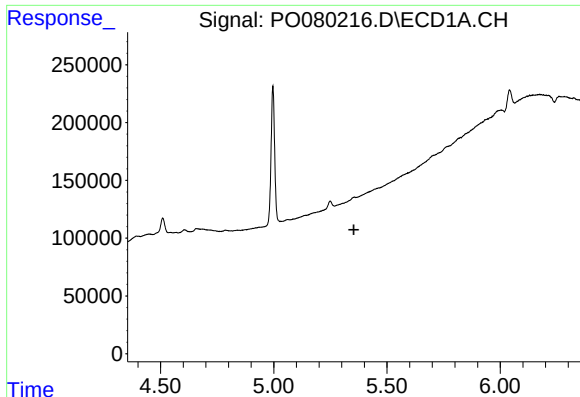

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

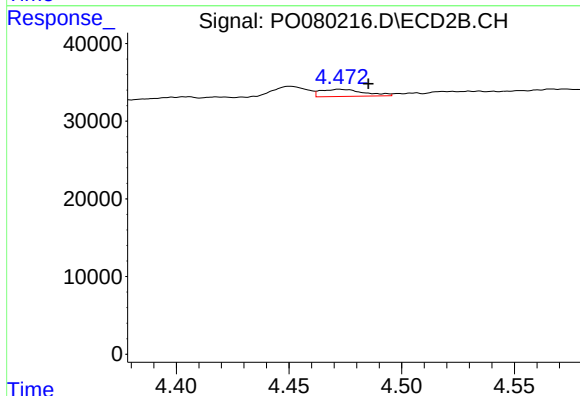


#9 AR-1221-2

R.T.: 4.472 min
Delta R.T.: -0.013 min
Response: 12151
Conc: 56.66 ng/ml

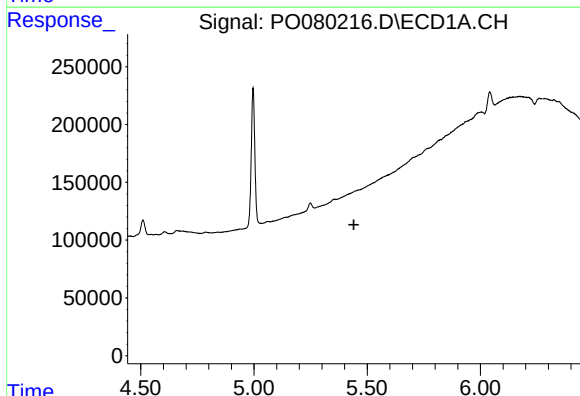


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 5.442 min
Response: 0
Conc: N.D.

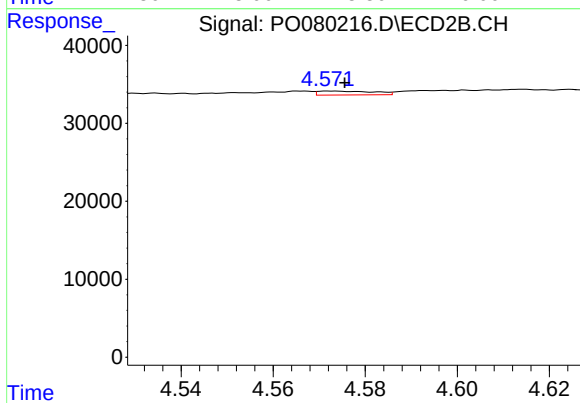

#10 AR-1221-3


R.T.: 4.573 min
Delta R.T.: -0.003 min
Response: 4186
Conc: 6.45 ng/ml

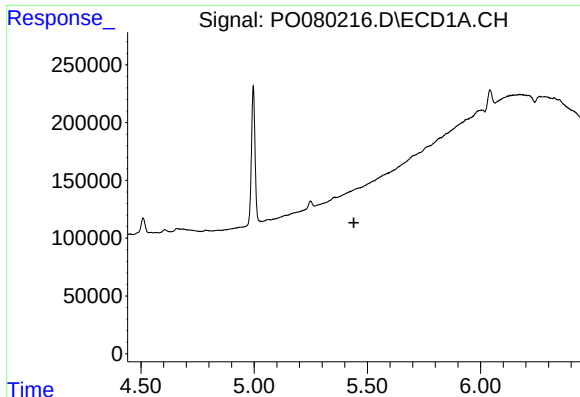

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

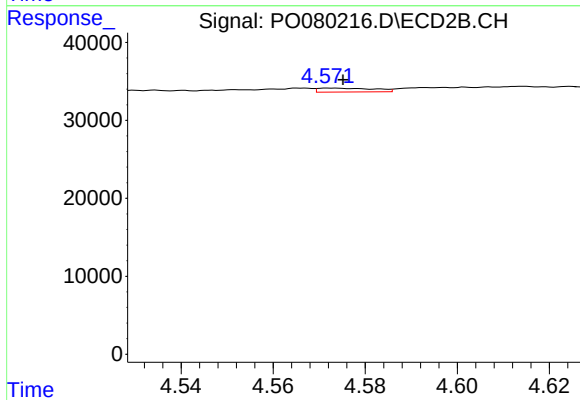


#11 AR-1232-1

R.T.: 4.573 min
Delta R.T.: -0.003 min
Response: 4186
Conc: 6.94 ng/ml

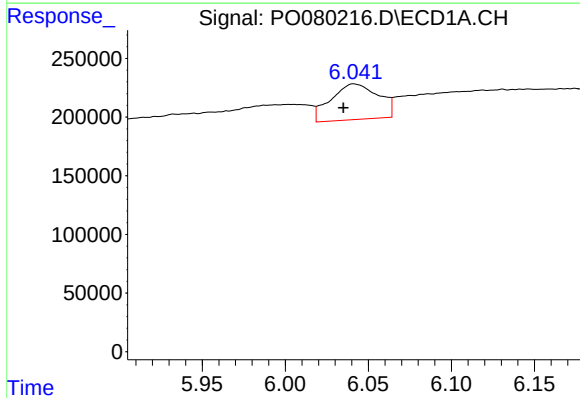


#12 AR-1232-2

R.T.: 6.041 min
Delta R.T.: 0.006 min
Response: 605718
Conc: 867.11 ng/ml

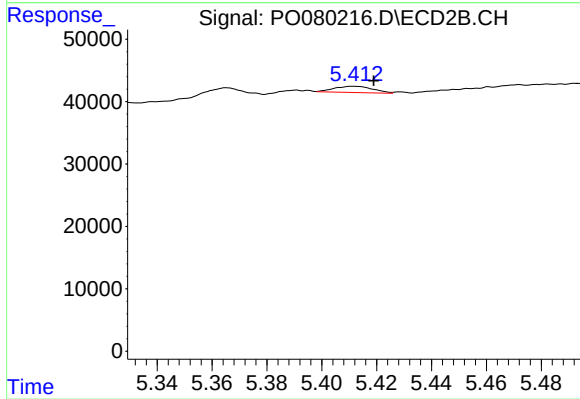

#12 AR-1232-2


R.T.: 5.411 min
Delta R.T.: -0.008 min
Response: 9972
Conc: 17.73 ng/ml

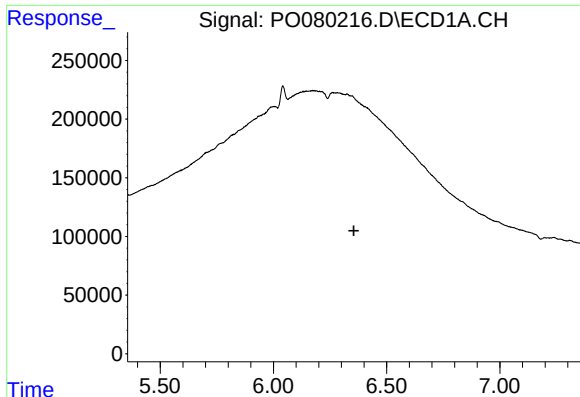

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

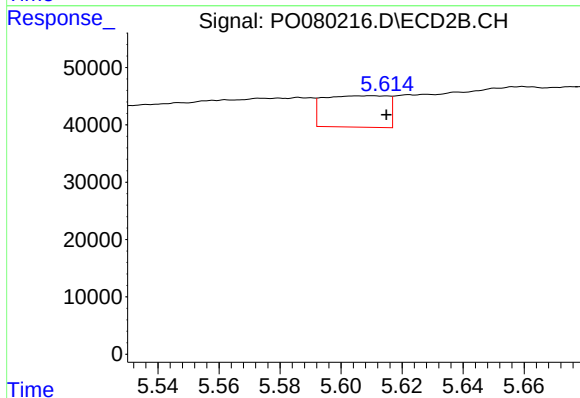


#13 AR-1232-3

R.T.: 5.610 min
Delta R.T.: -0.005 min
Response: 79657
Conc: 264.59 ng/ml

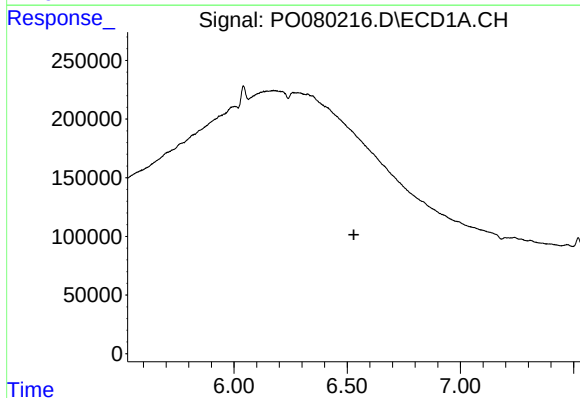


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 6.530 min
Response: 0
Conc: N.D.

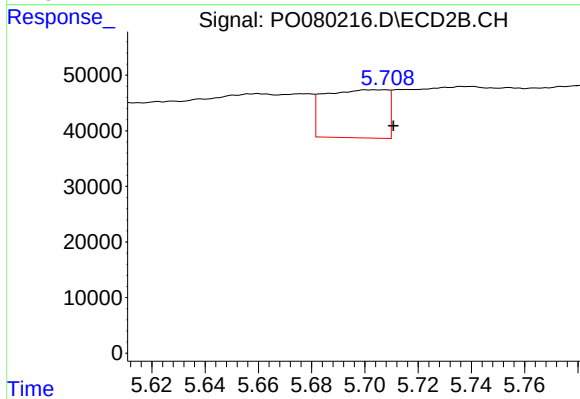

#14 AR-1232-4


R.T.: 5.700 min
Delta R.T.: -0.011 min
Response: 141366
Conc: 496.60 ng/ml

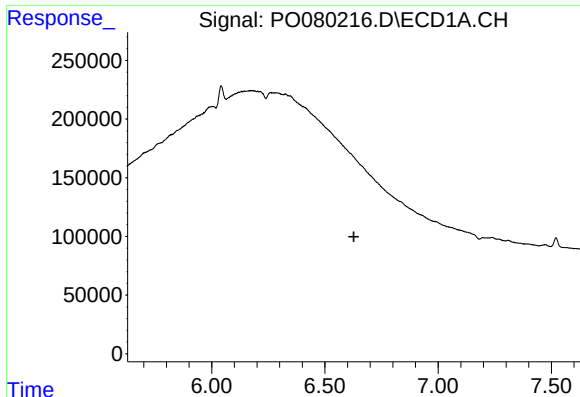

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

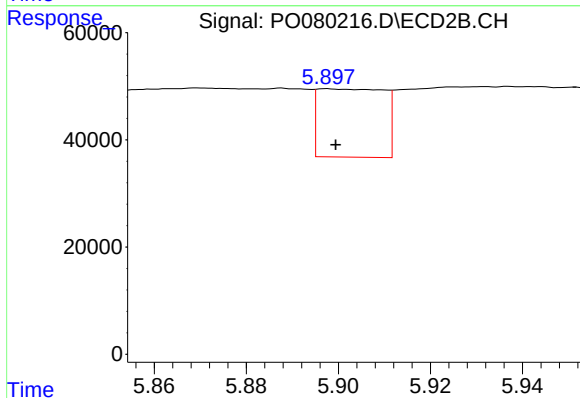


#15 AR-1232-5

R.T.: 5.898 min
Delta R.T.: -0.002 min
Response: 126031
Conc: 419.67 ng/ml

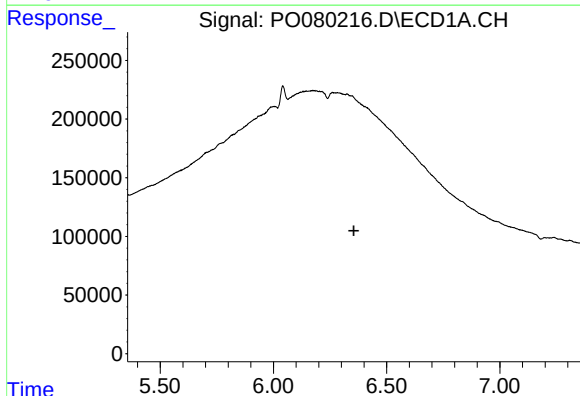


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 6.356 min
Response: 0
Conc: N.D.

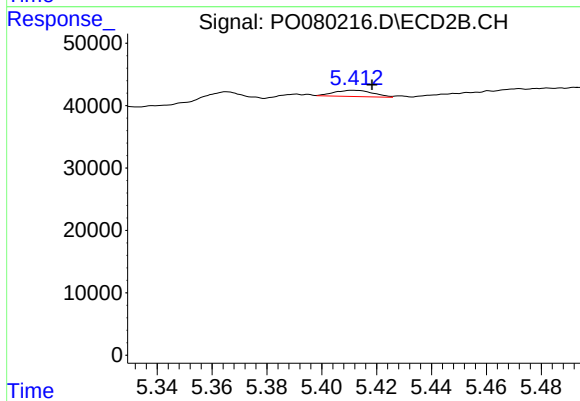

#17 AR-1242-2


R.T.: 5.411 min
Delta R.T.: -0.007 min
Response: 9972
Conc: 10.30 ng/ml

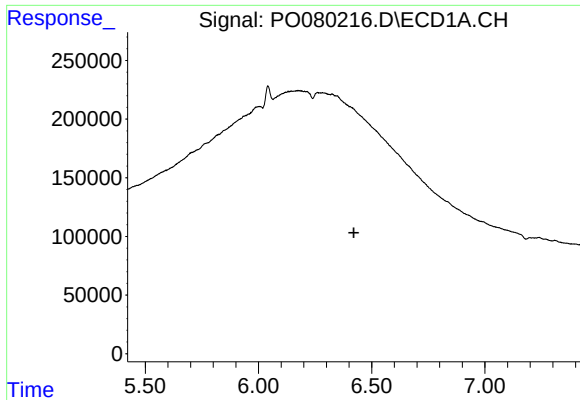

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 6.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

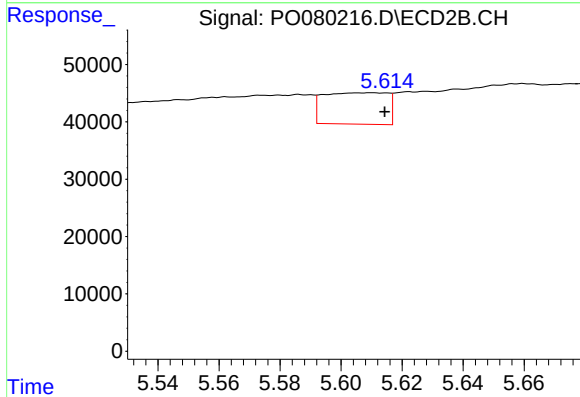


#18 AR-1242-3

R.T.: 5.610 min
Delta R.T.: -0.004 min
Response: 79657
Conc: 148.46 ng/ml

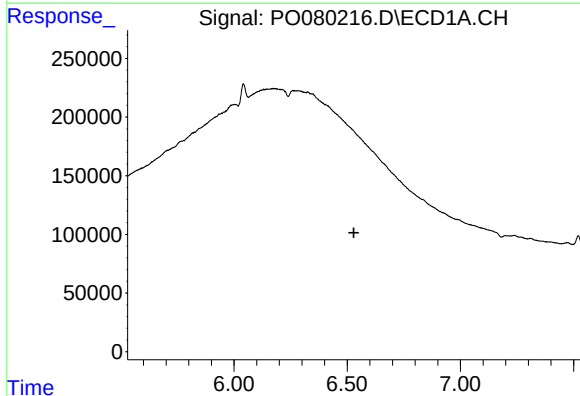


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 6.529 min
Response: 0
Conc: N.D.

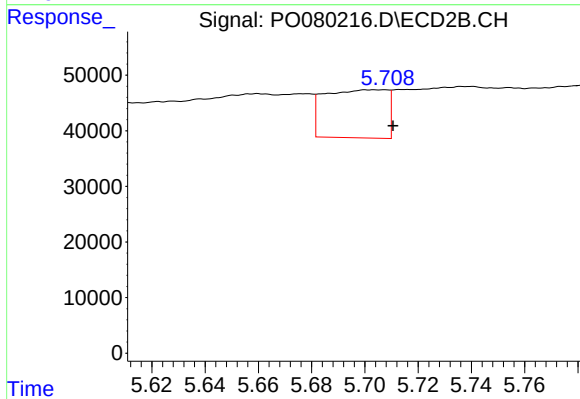

#19 AR-1242-4


R.T.: 5.700 min
Delta R.T.: -0.010 min
Response: 141366
Conc: 251.76 ng/ml

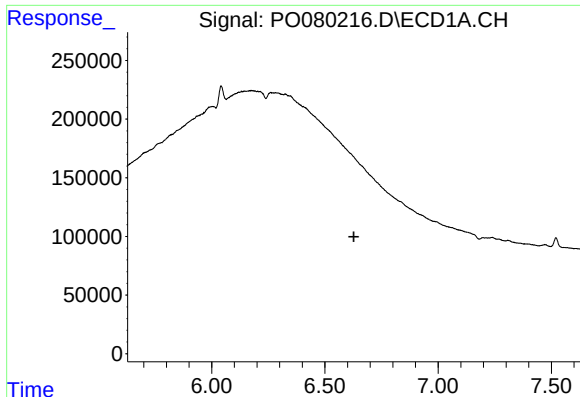

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

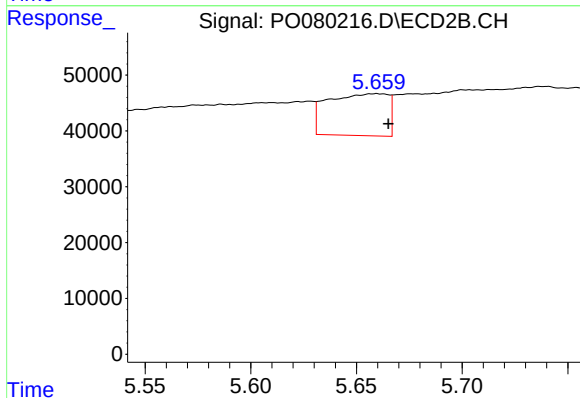


#22 AR-1248-2

R.T.: 5.660 min
Delta R.T.: -0.005 min
Response: 149555
Conc: 181.52 ng/ml

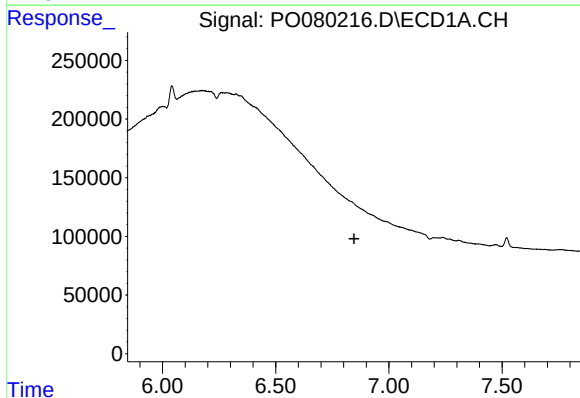


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.846 min
Response: 0
Conc: N.D.

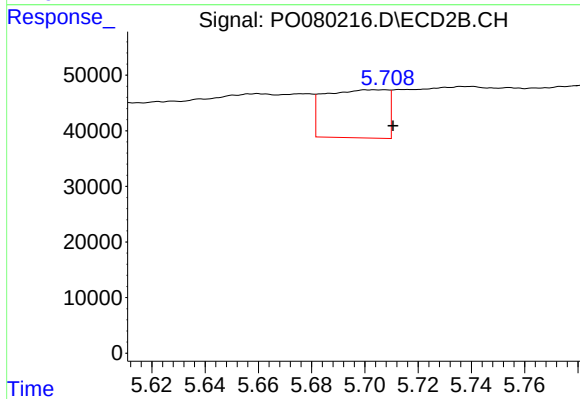

#23 AR-1248-3


R.T.: 5.700 min
Delta R.T.: -0.010 min
Response: 141366
Conc: 170.34 ng/ml

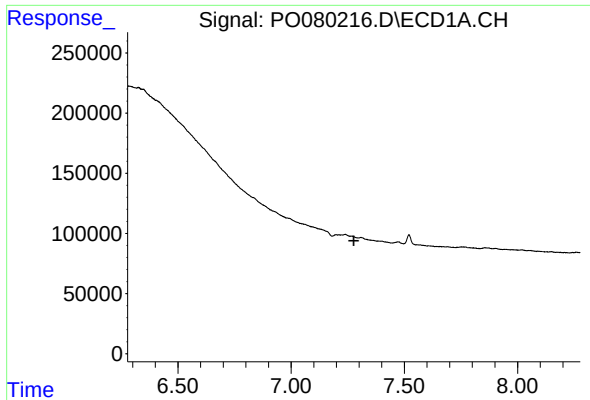

#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 7.277 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
20210572-COM-45

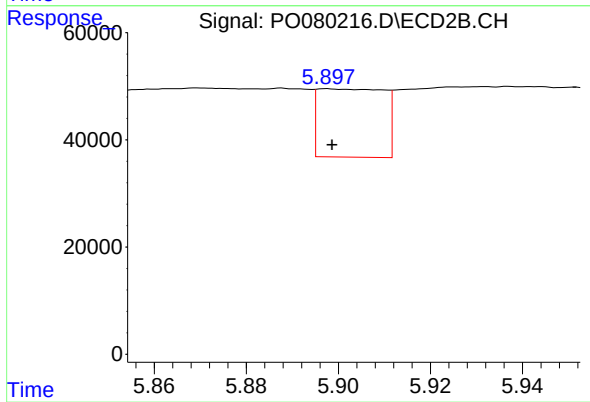

#24 AR-1248-4

R.T.: 5.898 min
Delta R.T.: -0.001 min
Response: 126031
Conc: 133.38 ng/ml