

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
 Data File : P0080189.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2021 10:36
 Operator : DD\AJ
 Sample : M3268-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20210576-COM-49

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 15:29:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.995	4.114	1085177	407523	18.009	17.795
2)	SA Decachlor...	11.100	9.519	460991	220302	9.827	10.601

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
Data File : P0080189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2021 10:36
Operator : DD\AJ
Sample : M3268-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20210576-COM-49

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 15:29:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

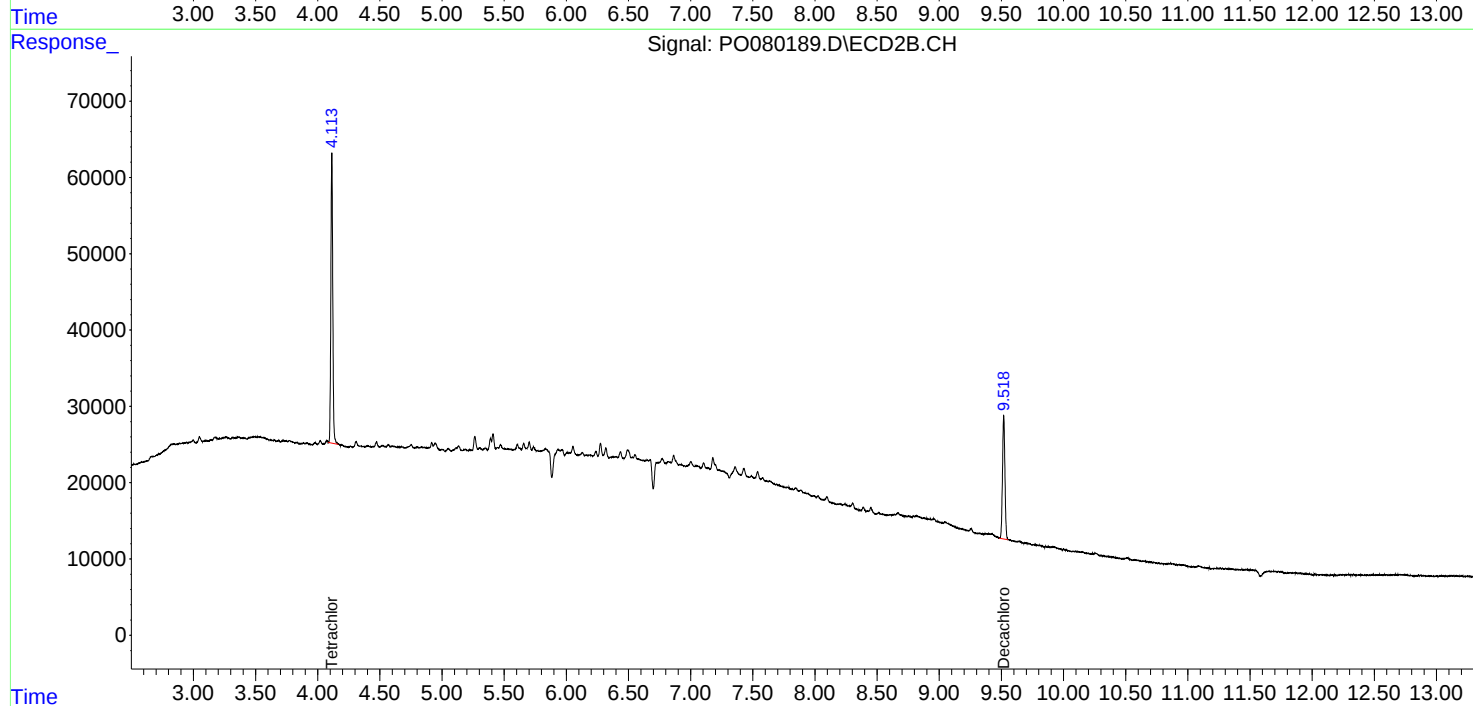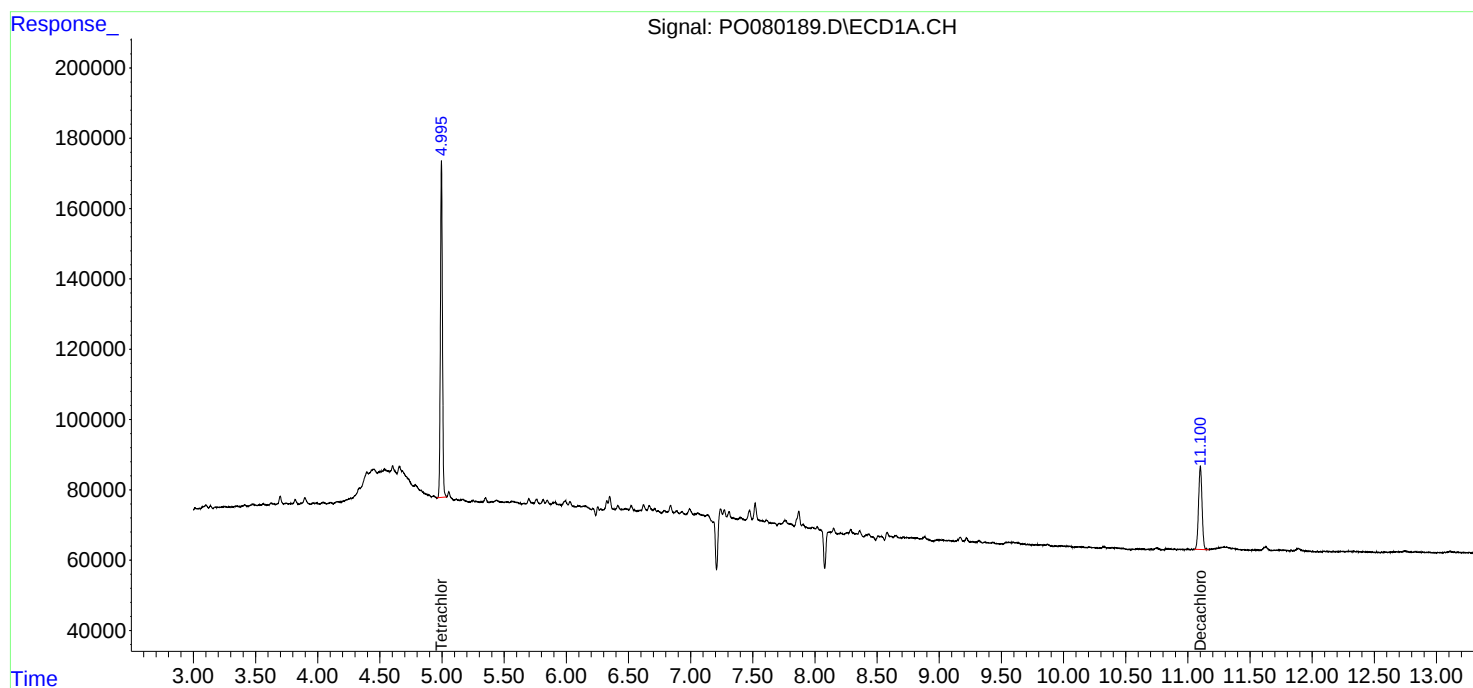


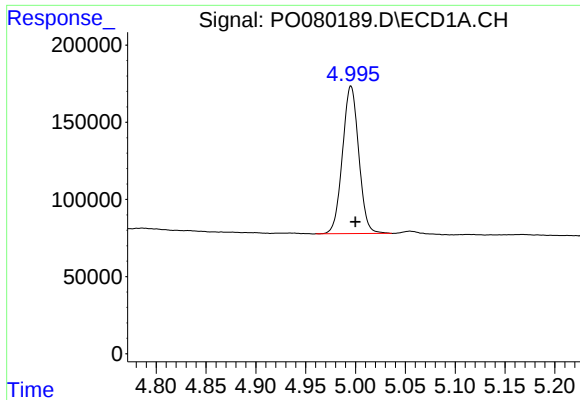

#1 Tetrachloro-m-xylene


R.T.: 4.995 min
Delta R.T.: -0.005 min
Response: 1085177
Conc: 18.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
20210576-COM-49

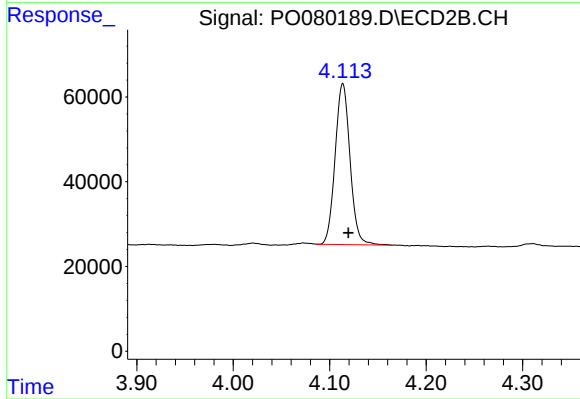


#1 Tetrachloro-m-xylene

R.T.: 4.114 min
Delta R.T.: -0.006 min
Response: 407523
Conc: 17.79 ng/ml

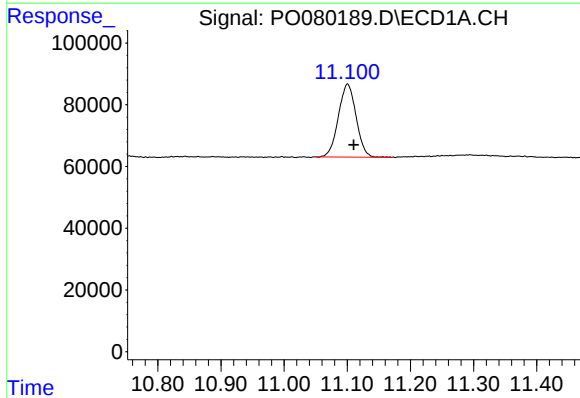

#2 Decachlorobiphenyl

R.T.: 11.100 min
Delta R.T.: -0.010 min
Response: 460991
Conc: 9.83 ng/ml

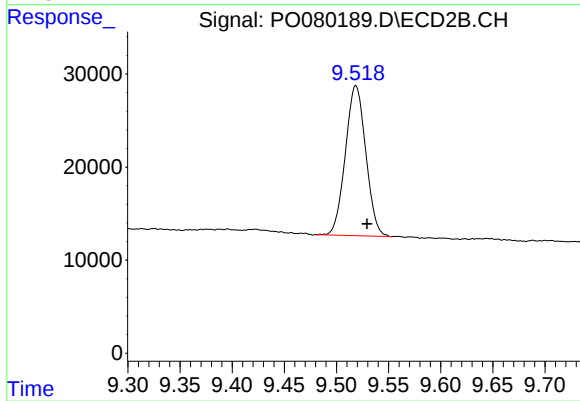

#2 Decachlorobiphenyl

R.T.: 9.519 min
Delta R.T.: -0.011 min
Response: 220302
Conc: 10.60 ng/ml