

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
 Data File : P0080191.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2021 11:10
 Operator : DD\AJ
 Sample : M3283-02RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-031-IDWGW-20210803RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 15:30:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.996	4.115	1114592	413954	18.497	18.076
2) SA Decachlor...	11.101	9.517	189809	87181	4.046	4.195

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080191\
Data File : P0080191.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2021 11:10
Operator : DD\AJ
Sample : M3283-02RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-031-IDWGW-20210803RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 15:30:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

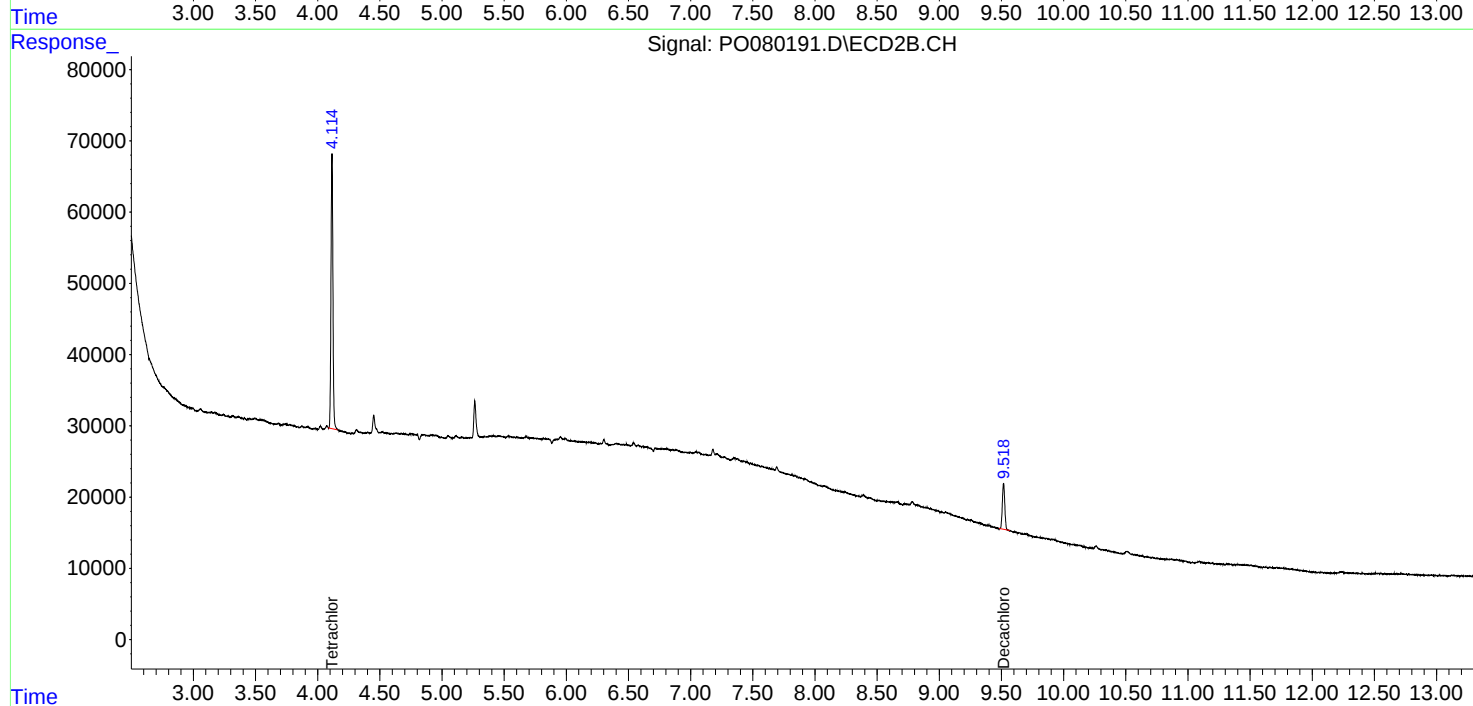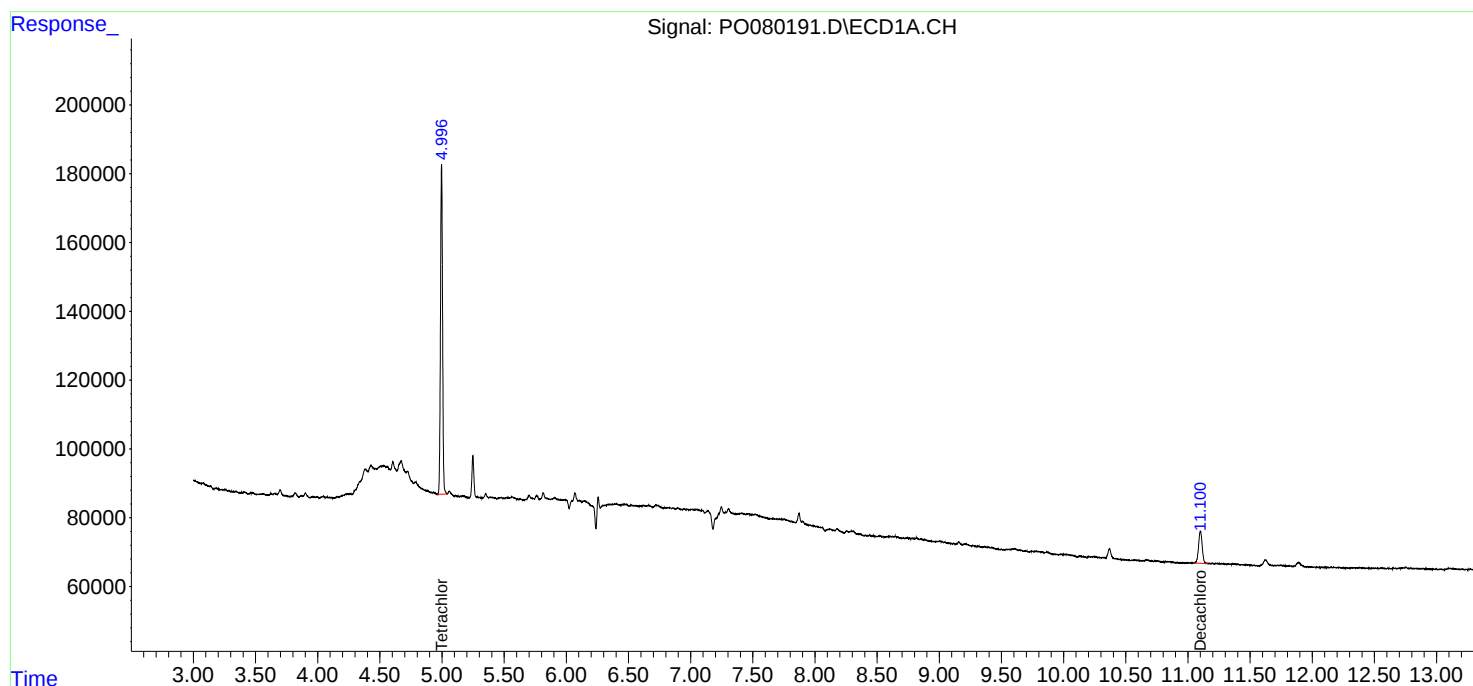


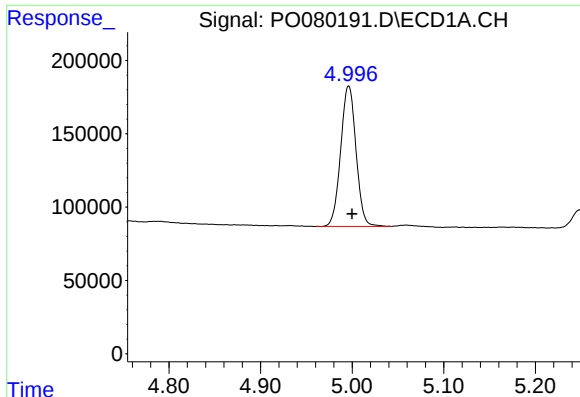

#1 Tetrachloro-m-xylene


R.T.: 4.996 min
Delta R.T.: -0.004 min
Response: 1114592
Conc: 18.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-031-IDWGW-20210803RE

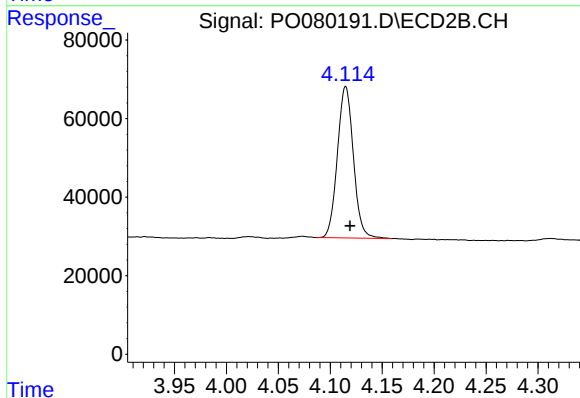


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.004 min
Response: 413954
Conc: 18.08 ng/ml

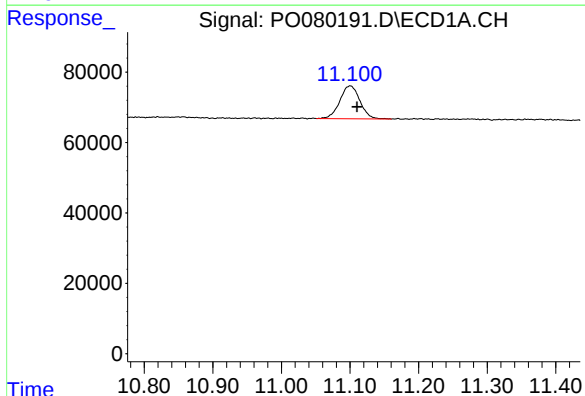

#2 Decachlorobiphenyl

R.T.: 11.101 min
Delta R.T.: -0.010 min
Response: 189809
Conc: 4.05 ng/ml

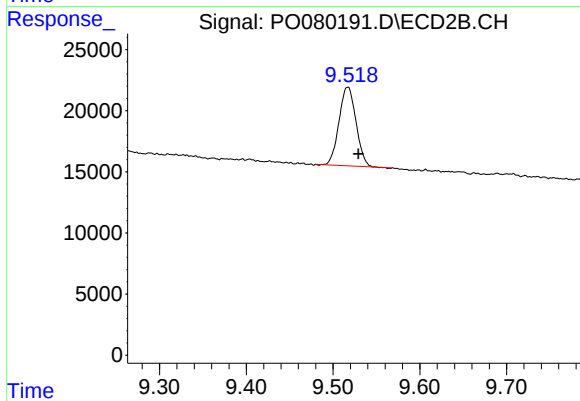

#2 Decachlorobiphenyl

R.T.: 9.517 min
Delta R.T.: -0.012 min
Response: 87181
Conc: 4.20 ng/ml