

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
 Data File : P0080199.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2021 13:41
 Operator : DD\AJ
 Sample : M3292-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 25546

Manual Integrations
 APPROVED

mohammad
 8/6/2021 3:08:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 15:32:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.996	4.114	1116543	427693	18.529	18.676
2) SA Decachlor...	11.102	9.518	920126	415696	19.615	20.003m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
Data File : P0080199.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2021 13:41
Operator : DD\AJ
Sample : M3292-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
25546


Manual Integrations
APPROVED

mohammad
8/6/2021 3:08:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 15:32:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

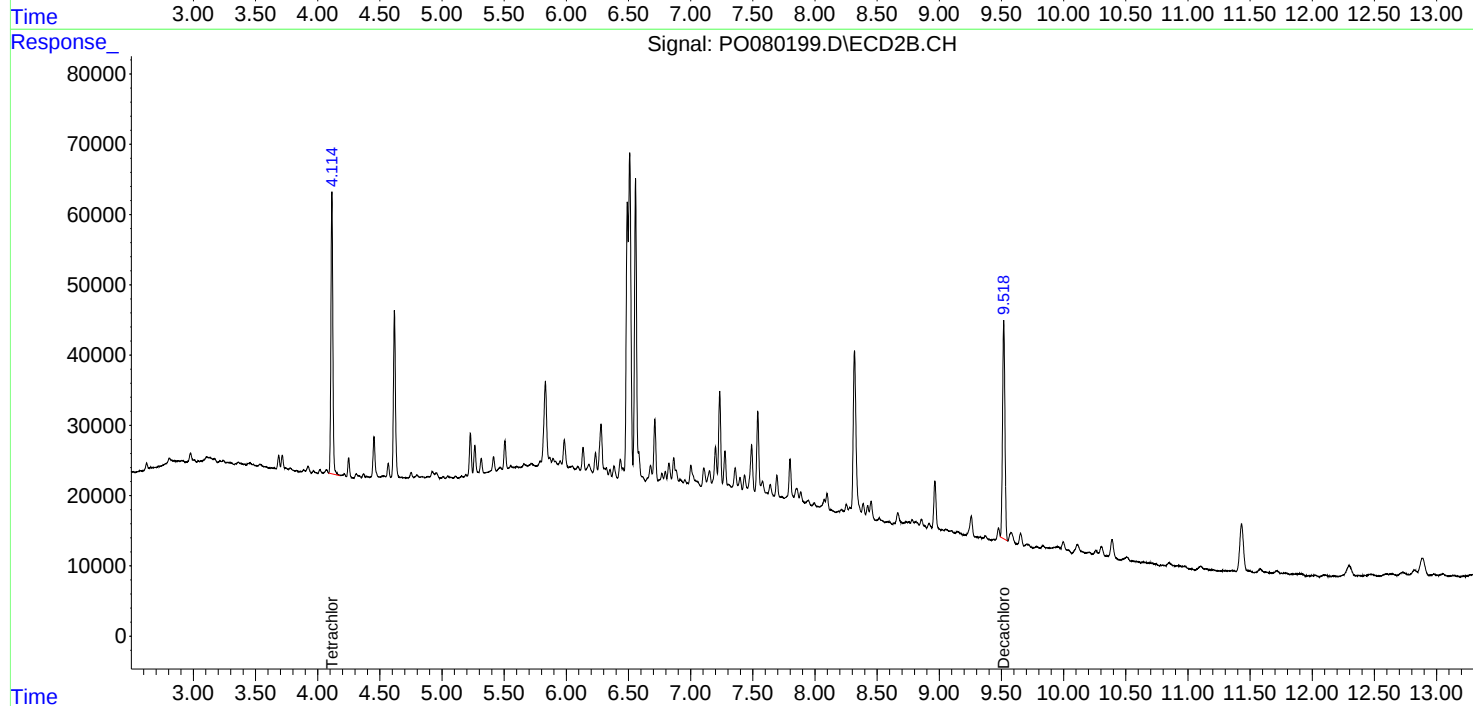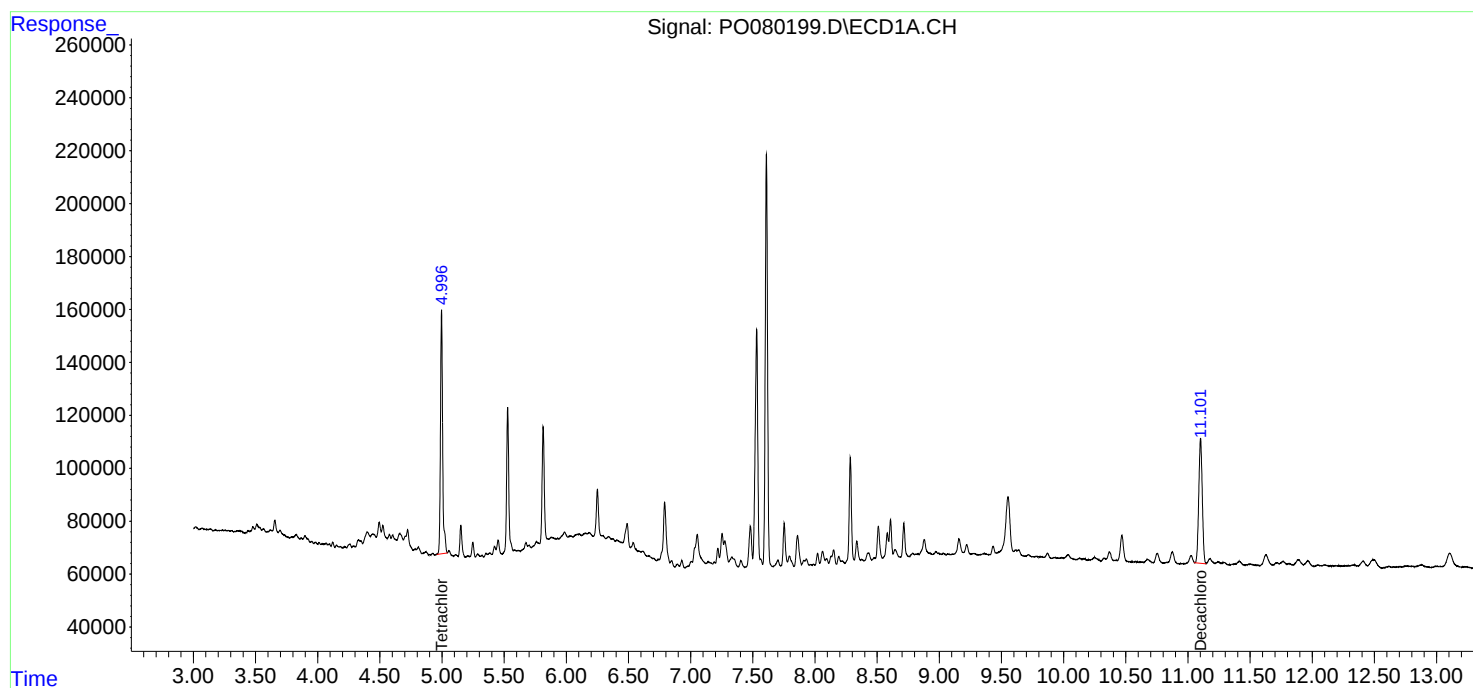

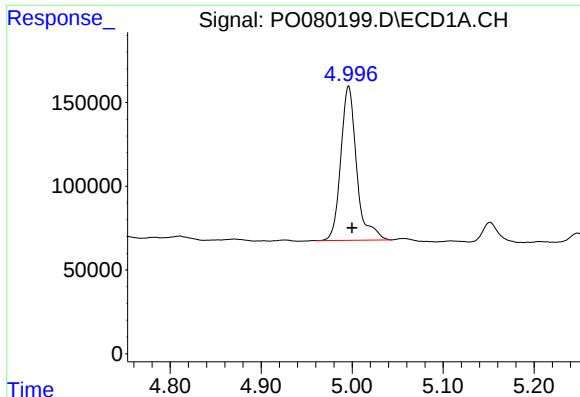


#1 Tetrachloro-m-xylene

R.T.: 4.996 min
Delta R.T.: -0.004 min
Response: 1116543
Conc: 18.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
25546


Manual Integrations
APPROVED

mohammad
8/6/2021 3:08:56 PM

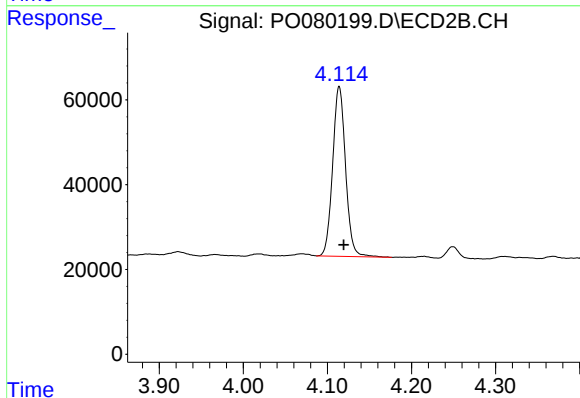


#1 Tetrachloro-m-xylene

R.T.: 4.114 min
Delta R.T.: -0.005 min
Response: 427693
Conc: 18.68 ng/ml

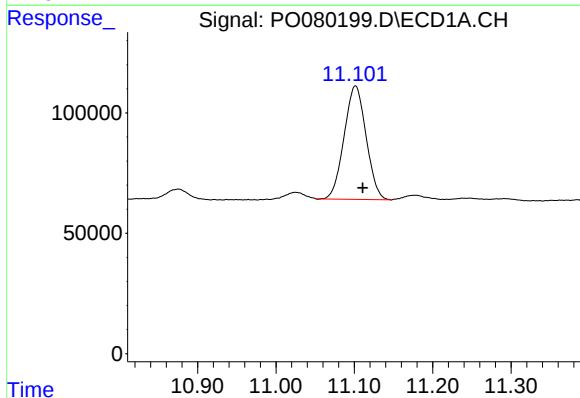

#2 Decachlorobiphenyl

R.T.: 11.102 min
Delta R.T.: -0.009 min
Response: 920126
Conc: 19.61 ng/ml

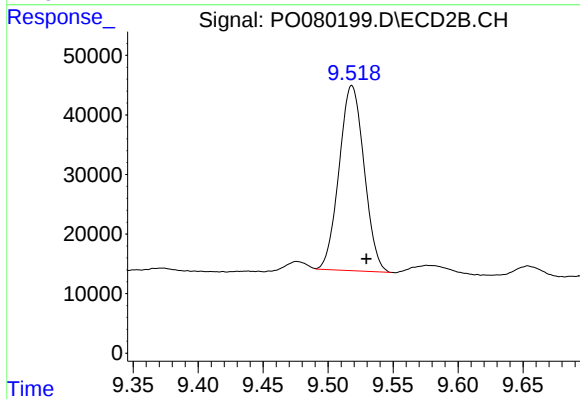

#2 Decachlorobiphenyl

R.T.: 9.518 min
Delta R.T.: -0.011 min
Response: 415696
Conc: 20.00 ng/ml m