

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
 Data File : P0080230.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Aug 2021 22:54
 Operator : DD\AJ
 Sample : M3281-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TWP01

Manual Integrations
 APPROVED

mohammad
 8/6/2021 3:09:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 00:27:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.995	4.113	1267430	517774	21.033m	22.609
2) SA Decachlor...	11.099	9.516	857700	384305	18.284	18.493

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080521\
Data File : P0080230.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Aug 2021 22:54
Operator : DD\AJ
Sample : M3281-03
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TWP01


Manual Integrations
APPROVED

mohammad
8/6/2021 3:09:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 00:27:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

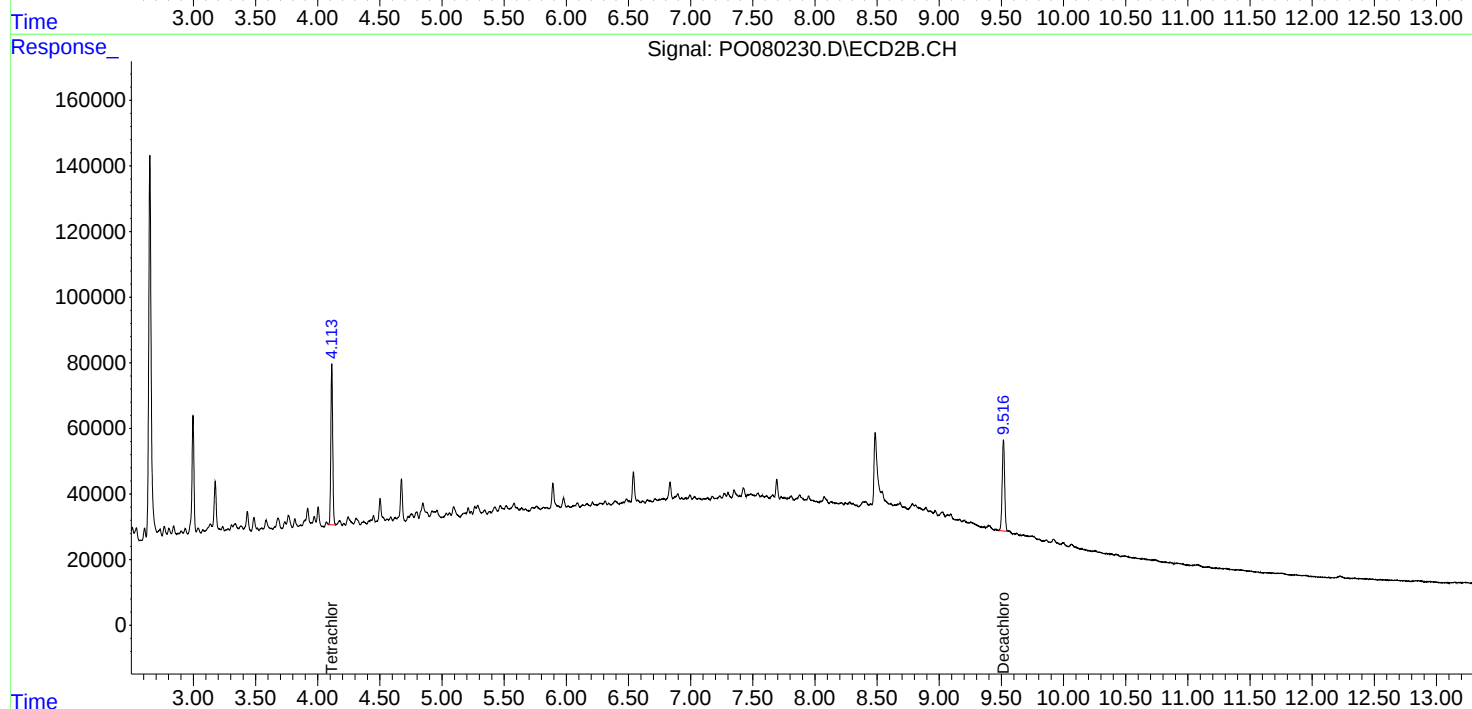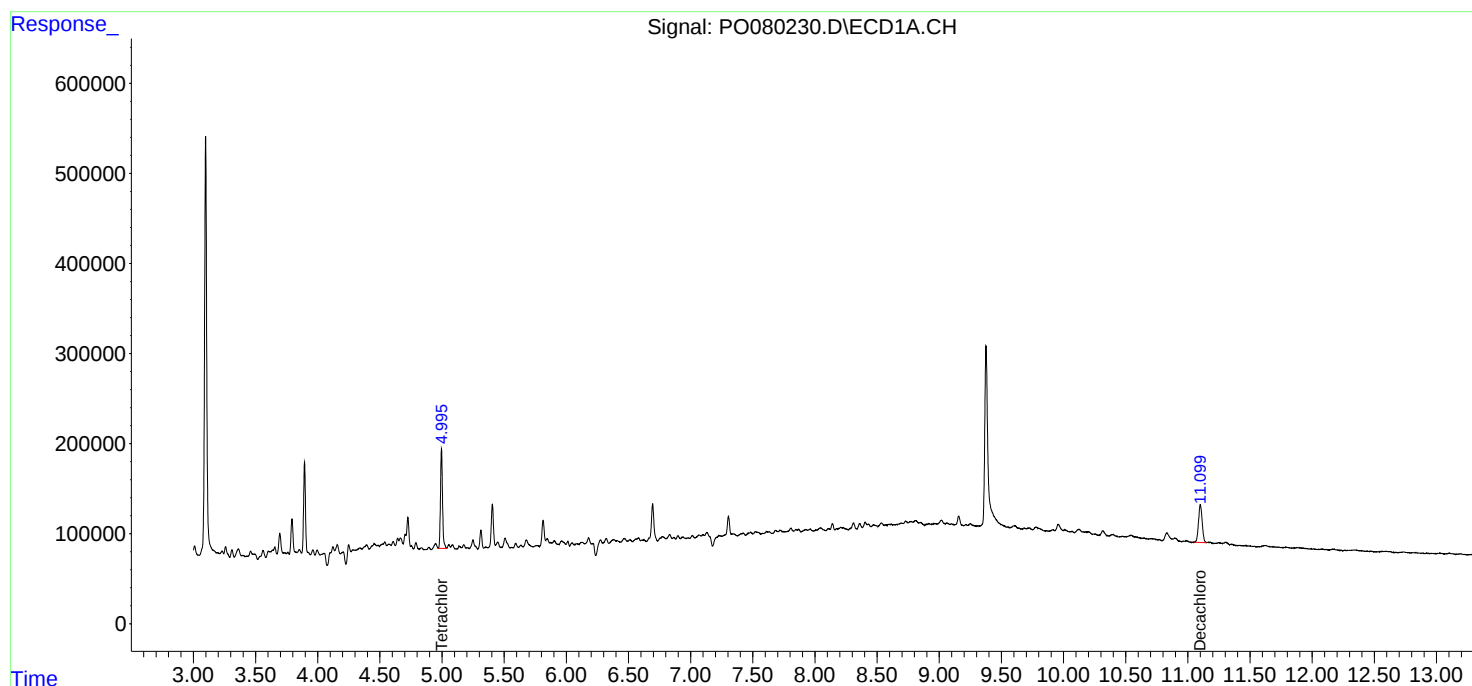

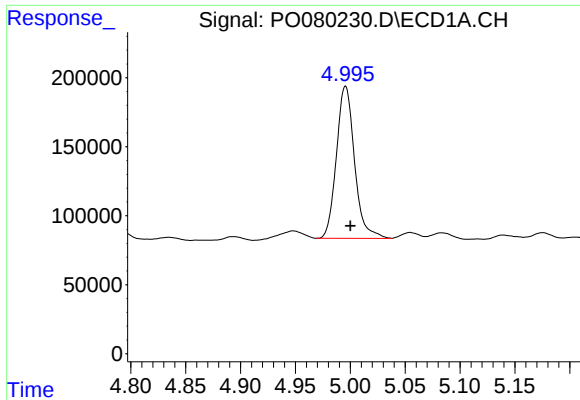


#1 Tetrachloro-m-xylene

R.T.: 4.995 min
Delta R.T.: -0.005 min
Response: 1267430
Conc: 21.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TWP01


Manual Integrations
APPROVED

mohammad
8/6/2021 3:09:13 PM

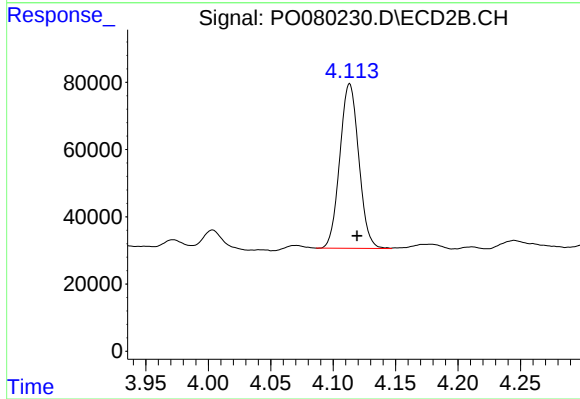


#1 Tetrachloro-m-xylene

R.T.: 4.113 min
Delta R.T.: -0.006 min
Response: 517774
Conc: 22.61 ng/ml

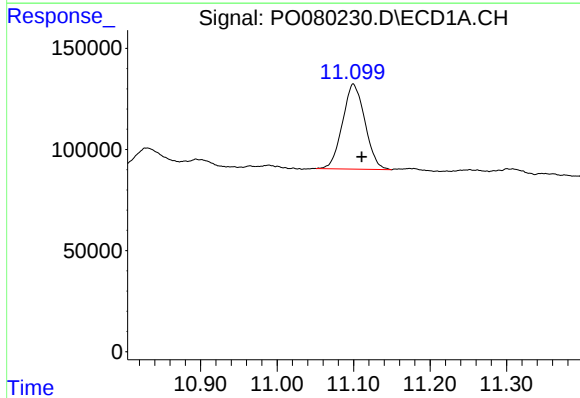

#2 Decachlorobiphenyl

R.T.: 11.099 min
Delta R.T.: -0.011 min
Response: 857700
Conc: 18.28 ng/ml

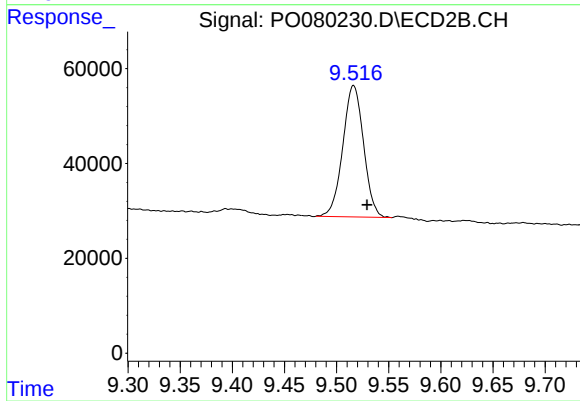

#2 Decachlorobiphenyl

R.T.: 9.516 min
Delta R.T.: -0.013 min
Response: 384305
Conc: 18.49 ng/ml