

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080522\
 Data File : P0088626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 22:43
 Operator : YP/AJ
 Sample : N4046-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BEACONPOINT-BACKFILL-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 02:41:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.438	3.595	59706930	23110792	22.135	21.353
2) SA Decachlor...	10.271	8.587	43200613	26212814	22.387	21.629

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080522\
Data File : PO088626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 22:43
Operator : YP/AJ
Sample : N4046-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BEACONPOINT-BACKFILL-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 02:41:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

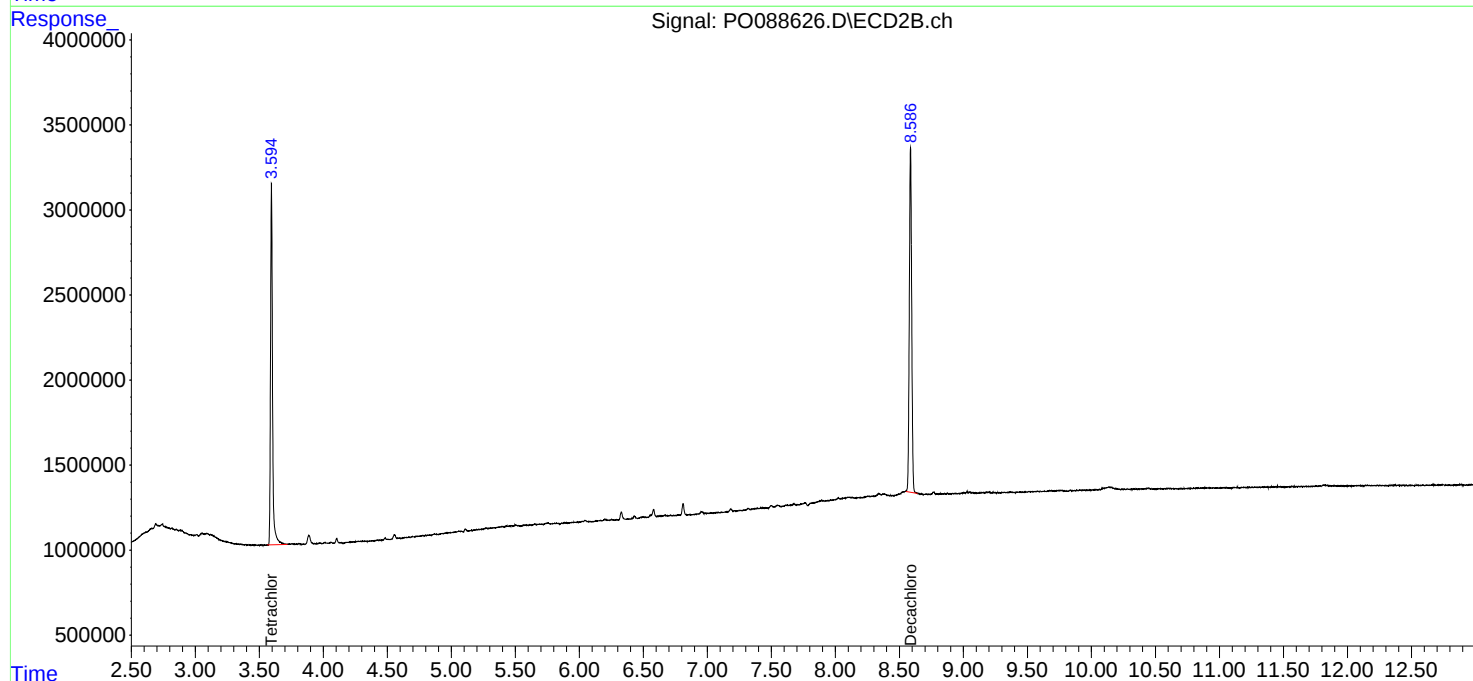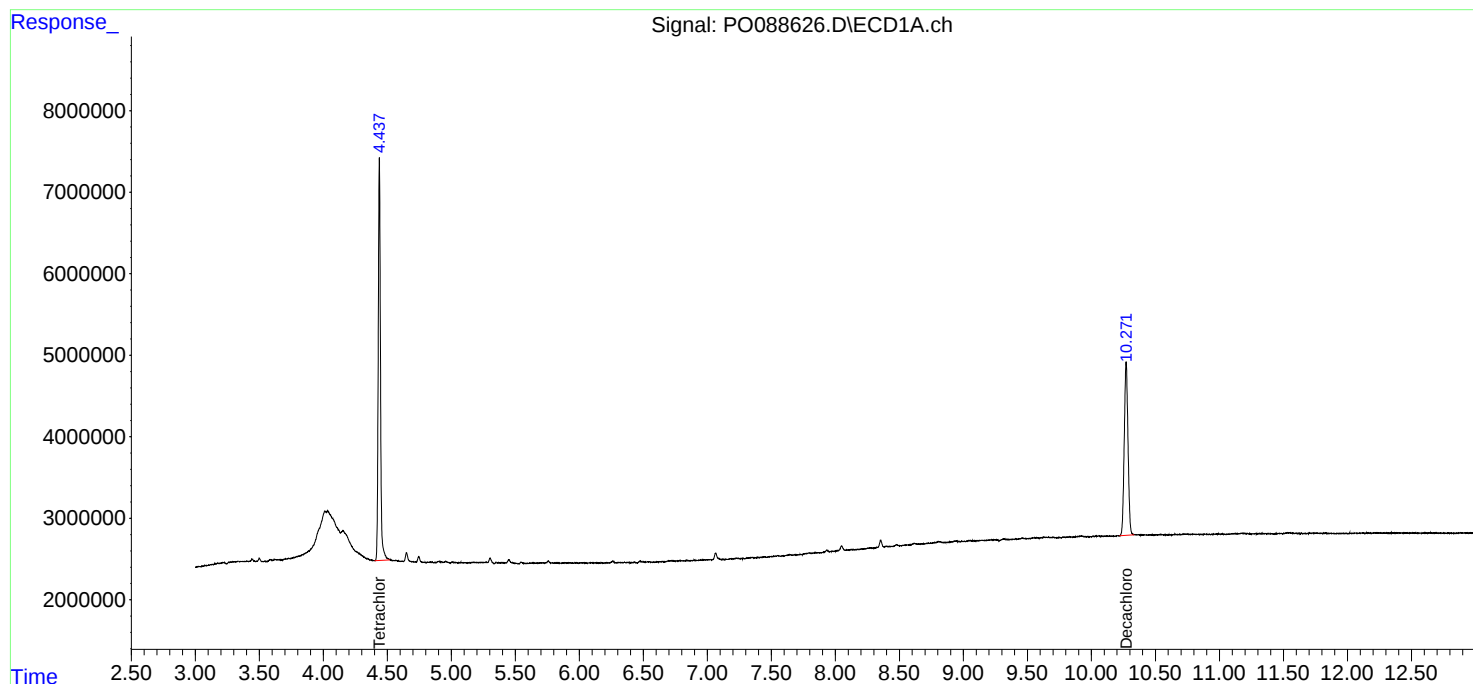


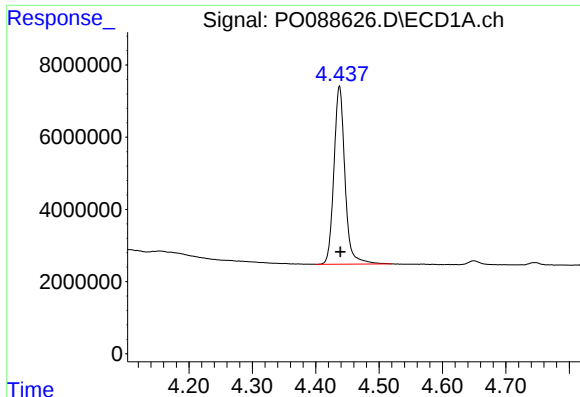

#1 Tetrachloro-m-xylene


R.T.: 4.438 min
Delta R.T.: -0.002 min
Response: 59706930
Conc: 22.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
BEACONPOINT-BACKFILL-06

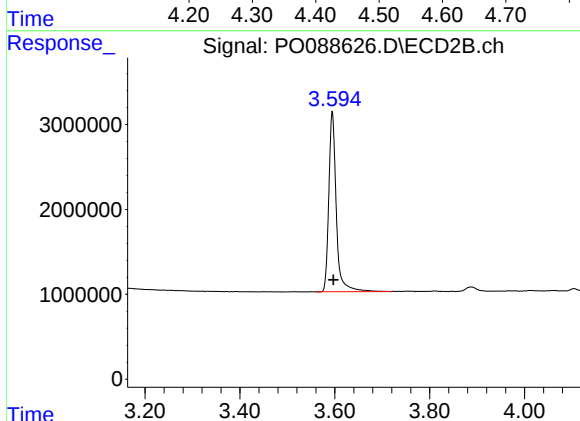


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: -0.002 min
Response: 23110792
Conc: 21.35 ng/ml

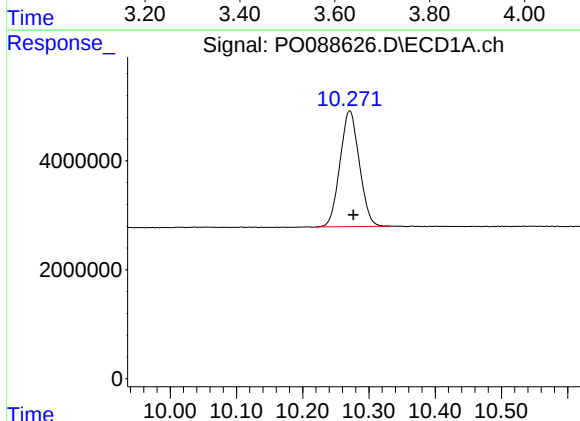

#2 Decachlorobiphenyl

R.T.: 10.271 min
Delta R.T.: -0.006 min
Response: 43200613
Conc: 22.39 ng/ml

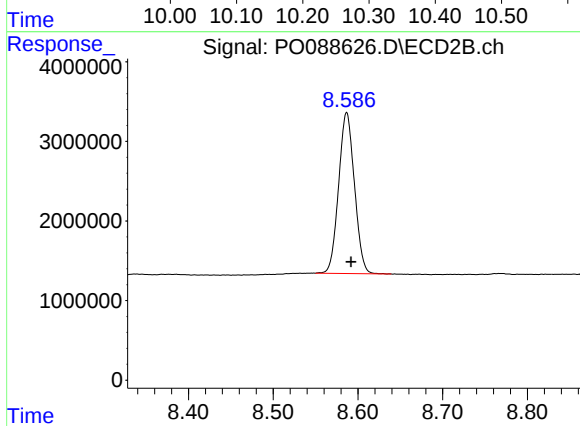

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.005 min
Response: 26212814
Conc: 21.63 ng/ml