

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080522\
 Data File : P0088640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 03:32
 Operator : YP/AJ
 Sample : N4061-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-328

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/08/2022
 Supervised By :Ankita Jodhani 08/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 07:36:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.436	3.594	60528598	22854840	22.440	21.117
2) SA Decachlor...	10.270	8.585	39687165	23311114	20.567	19.235m
Target Compounds						
26) L6 AR-1254-1	6.474	5.473	5350902	3155273	58.578	45.812
27) L6 AR-1254-2	6.693	5.620	8713054	2866137	63.714	48.398
28) L6 AR-1254-3	7.061	6.022	8645395	4092012	61.434	44.006 #
29) L6 AR-1254-4	7.346	6.251	5108372	2074139	50.555	36.613 #
30) L6 AR-1254-5	7.768	6.667	6633677	5475811	62.294m	67.083

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080522\
Data File : PO088640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 03:32
Operator : YP/AJ
Sample : N4061-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 07:36:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

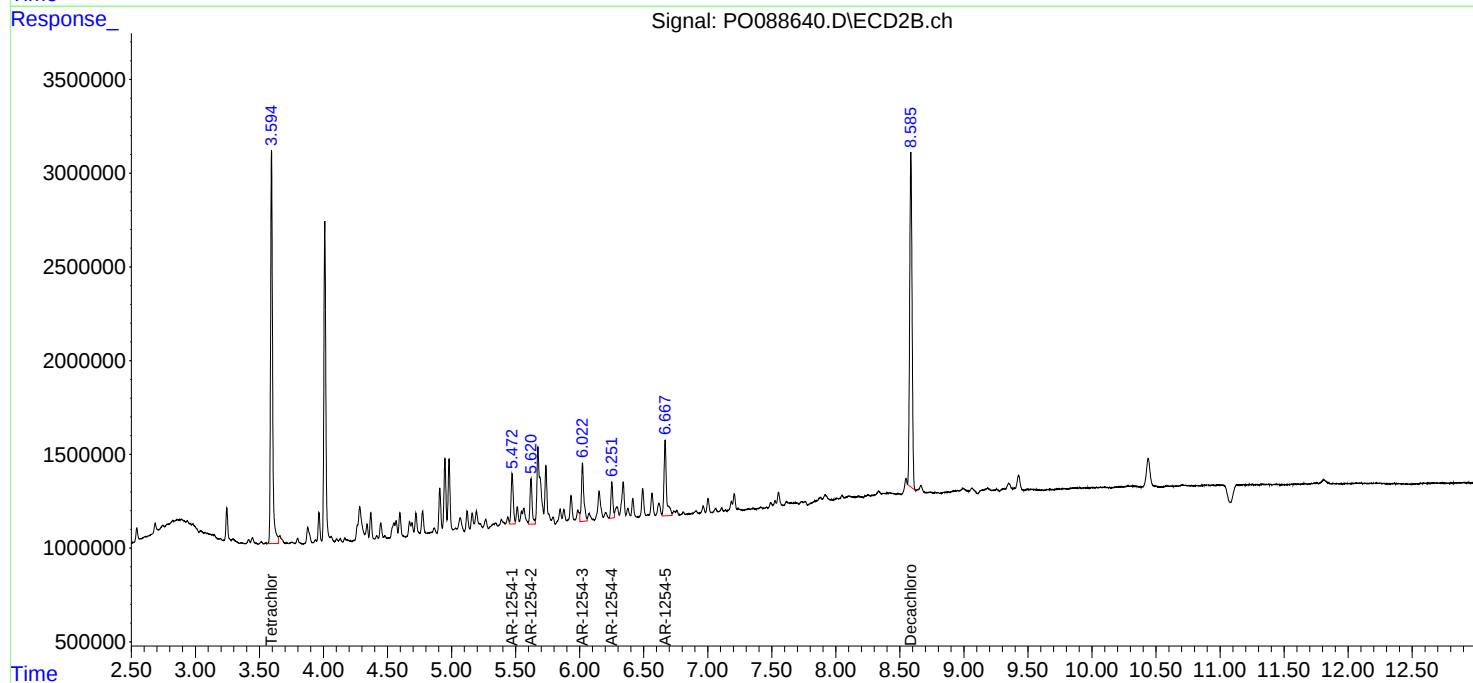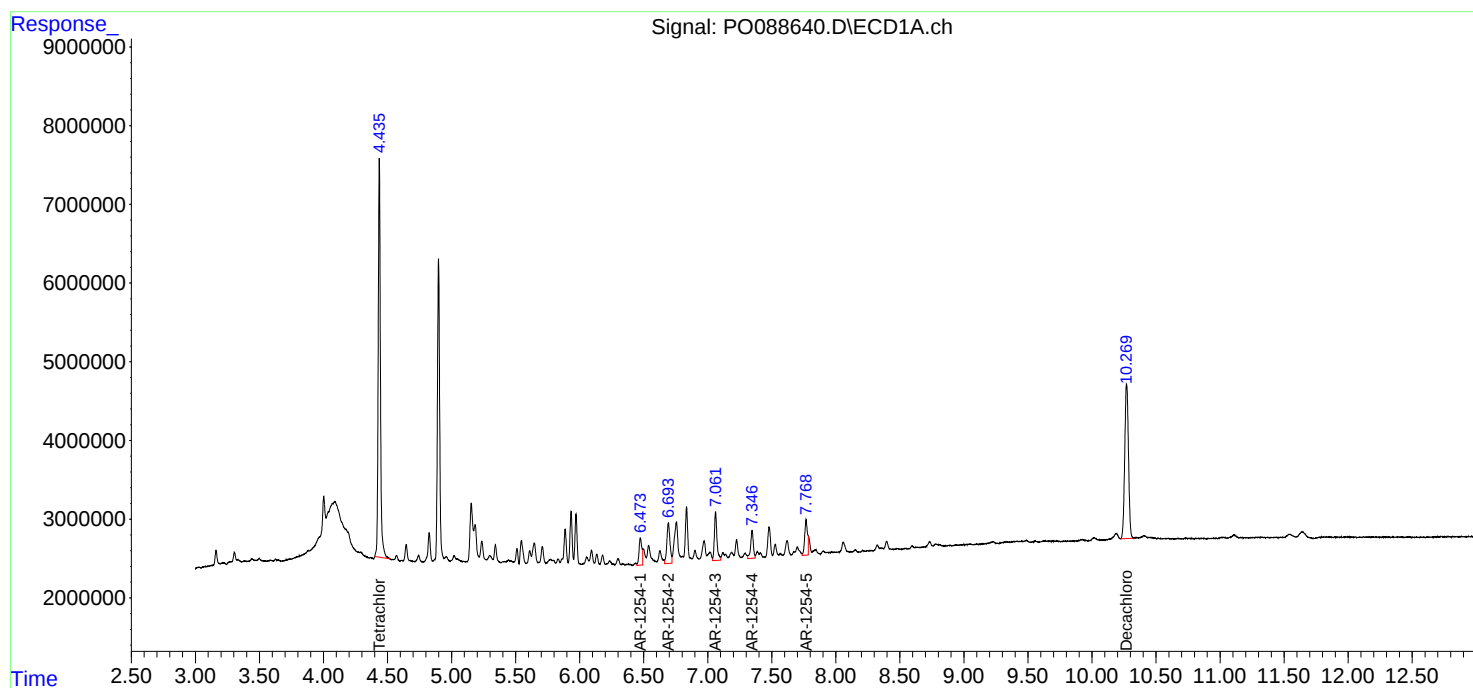

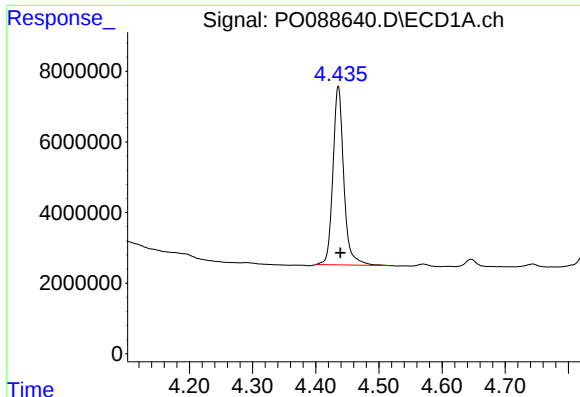


#1 Tetrachloro-m-xylene

R.T.: 4.436 min
Delta R.T.: -0.003 min
Response: 60528598
Conc: 22.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

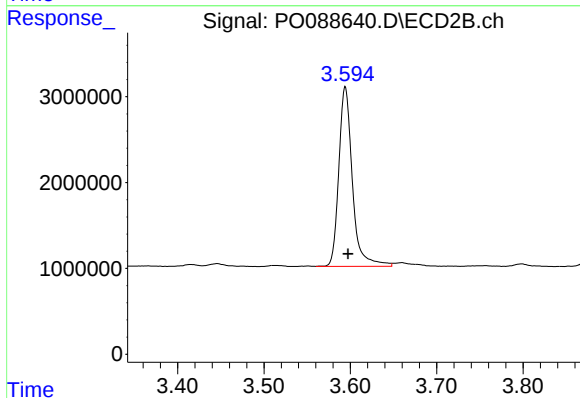


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: -0.003 min
Response: 22854840
Conc: 21.12 ng/ml

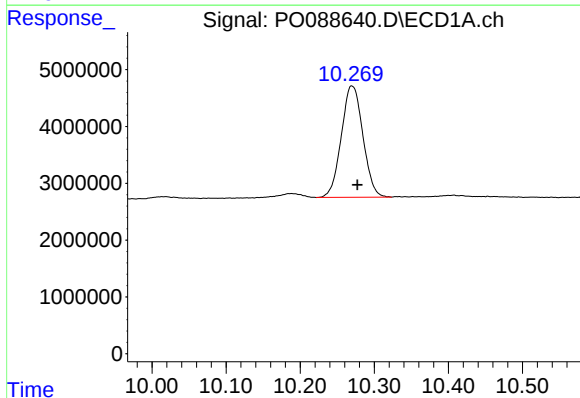


#2 Decachlorobiphenyl

R.T.: 10.270 min
Delta R.T.: -0.007 min
Response: 39687165
Conc: 20.57 ng/ml

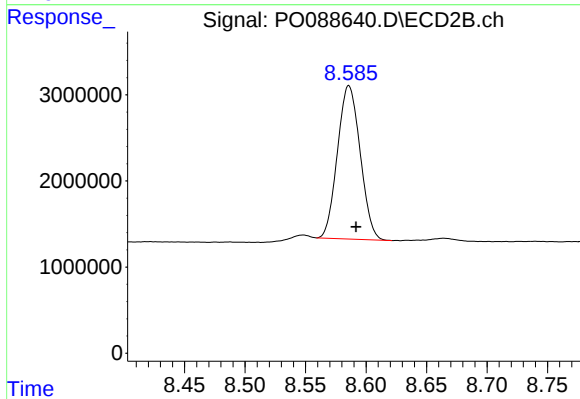

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: -0.006 min
Response: 23311114
Conc: 19.24 ng/ml m

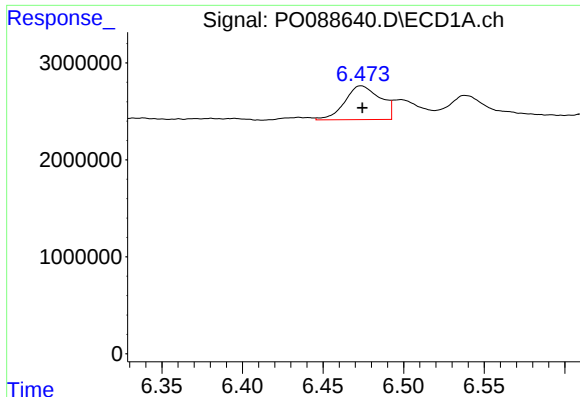


#26 AR-1254-1

R.T.: 6.474 min
Delta R.T.: 0.000 min
Response: 5350902
Conc: 58.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

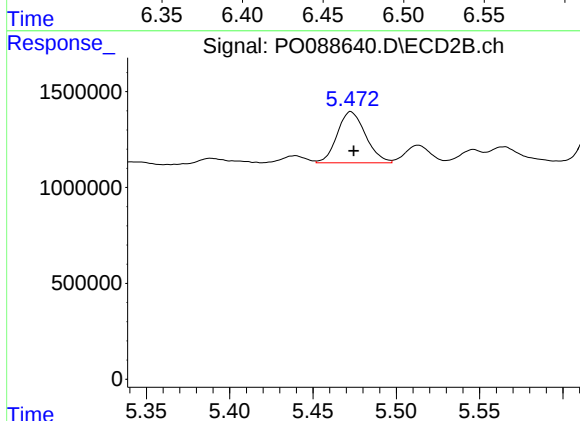


#26 AR-1254-1

R.T.: 5.473 min
Delta R.T.: -0.002 min
Response: 3155273
Conc: 45.81 ng/ml

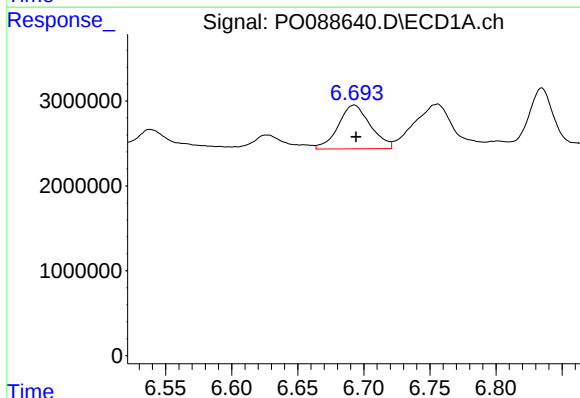


#27 AR-1254-2

R.T.: 6.693 min
Delta R.T.: -0.001 min
Response: 8713054
Conc: 63.71 ng/ml

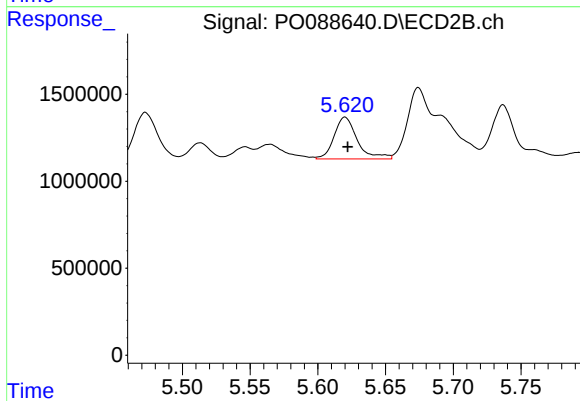

#27 AR-1254-2

R.T.: 5.620 min
Delta R.T.: -0.002 min
Response: 2866137
Conc: 48.40 ng/ml

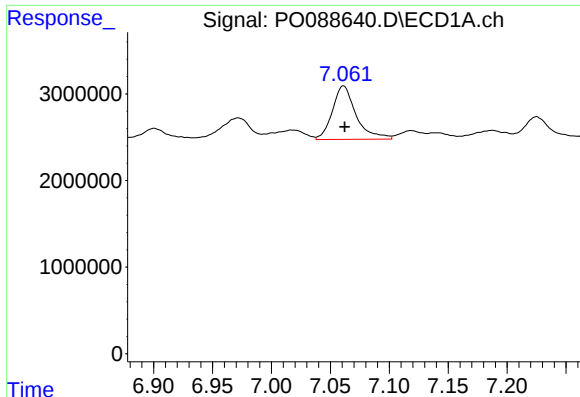


#28 AR-1254-3

R.T.: 7.061 min
Delta R.T.: -0.001 min
Response: 8645395
Conc: 61.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

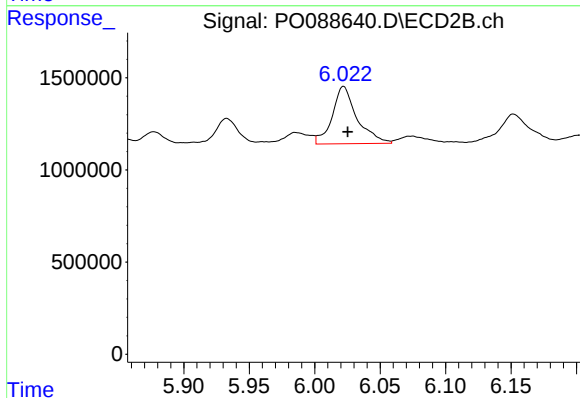


#28 AR-1254-3

R.T.: 6.022 min
Delta R.T.: -0.003 min
Response: 4092012
Conc: 44.01 ng/ml

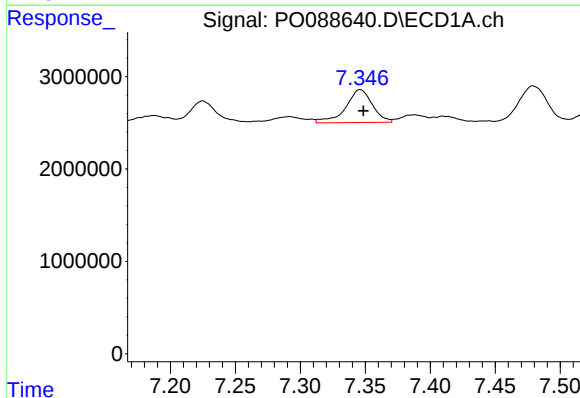


#29 AR-1254-4

R.T.: 7.346 min
Delta R.T.: -0.002 min
Response: 5108372
Conc: 50.56 ng/ml

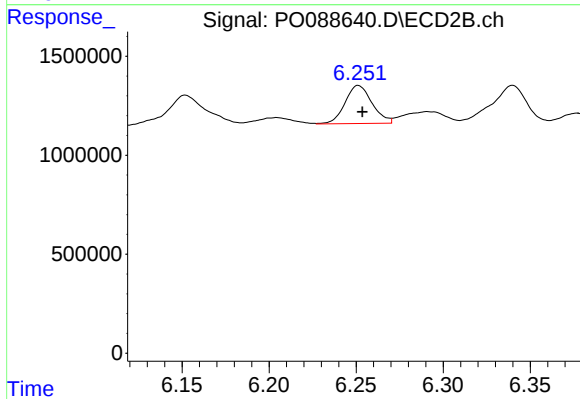

#29 AR-1254-4

R.T.: 6.251 min
Delta R.T.: -0.002 min
Response: 2074139
Conc: 36.61 ng/ml

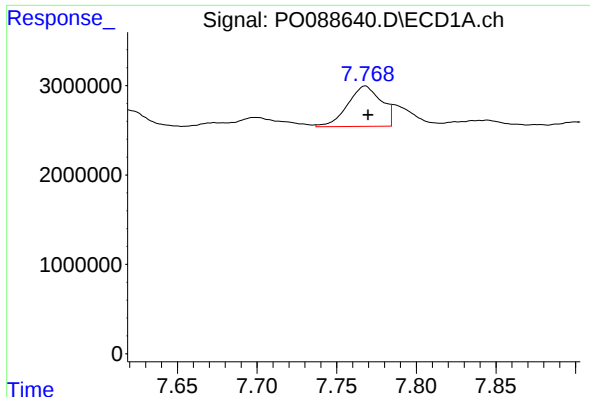


#30 AR-1254-5

R.T.: 7.768 min
Delta R.T.: -0.002 min
Response: 6633677
Conc: 62.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

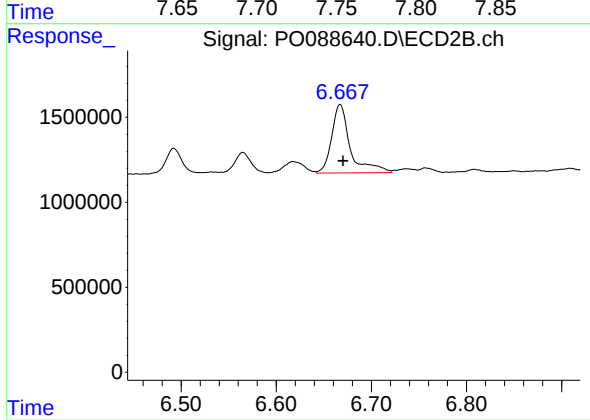

#30 AR-1254-5

R.T.: 6.667 min
Delta R.T.: -0.003 min
Response: 5475811
Conc: 67.08 ng/ml