

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080522\
 Data File : P0088678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 15:46
 Operator : YP/AJ
 Sample : N4018-03
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33773-74

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/08/2022
 Supervised By :Ankita Jodhani 08/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 21:50:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 05 23:24:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.436	3.595	37776885	15890620	14.005m	14.682m
2) SA Decachlor...	10.272	8.587	19429458	9756339	10.069	8.050

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080522\
Data File : PO088678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 15:46
Operator : YP/AJ
Sample : N4018-03
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33773-74


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 21:50:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 05 23:24:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

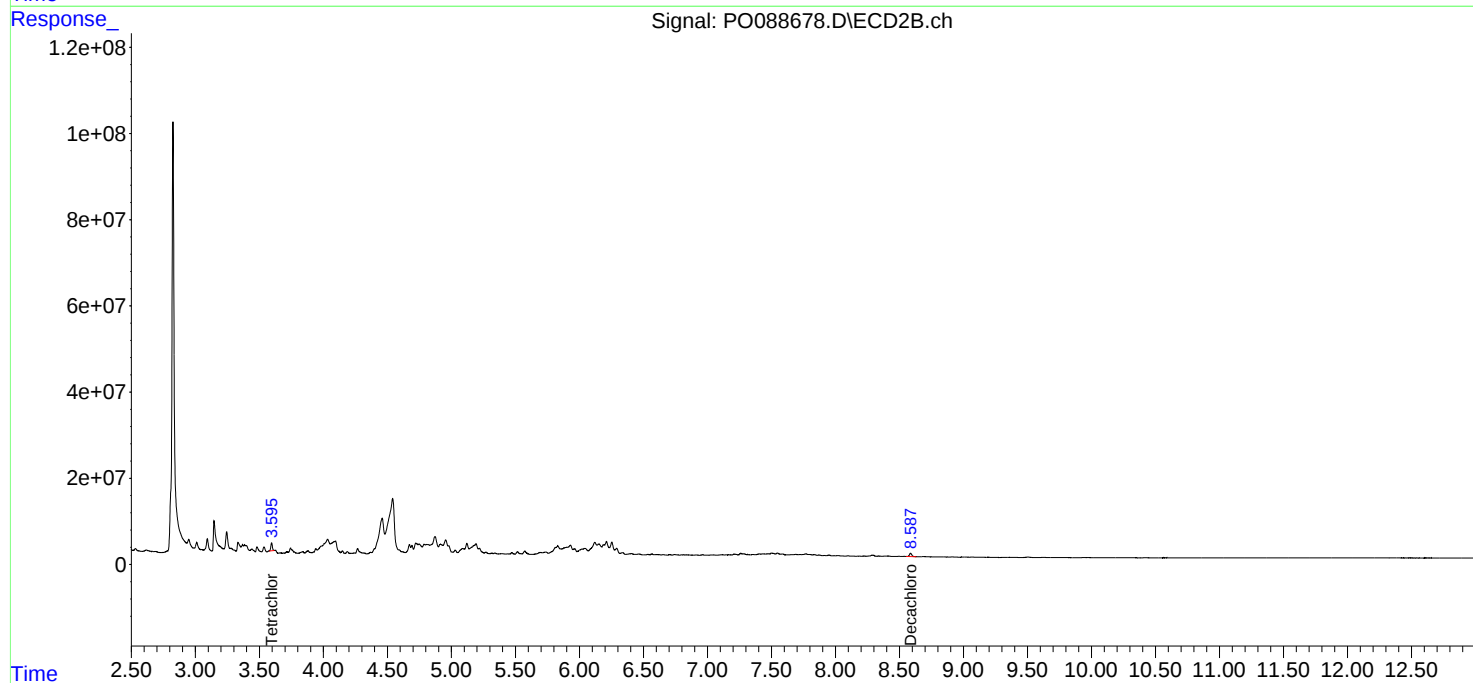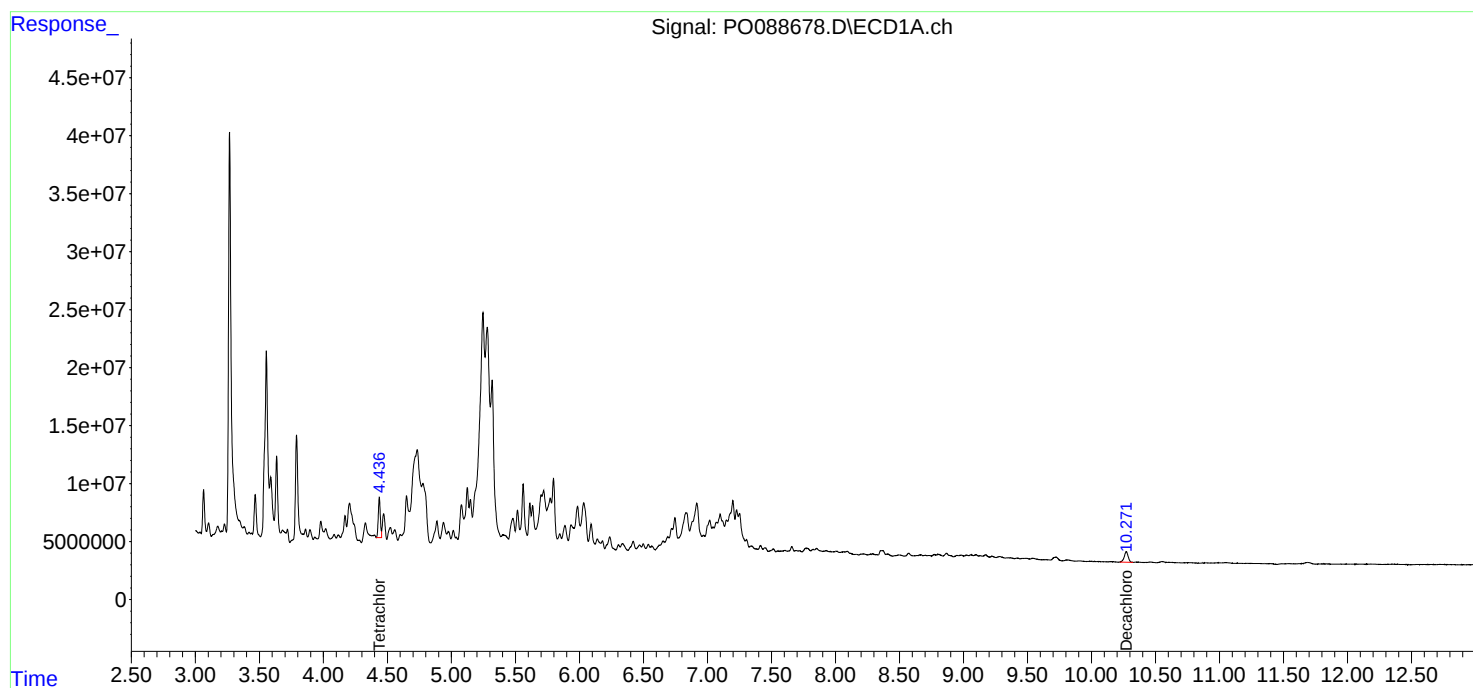

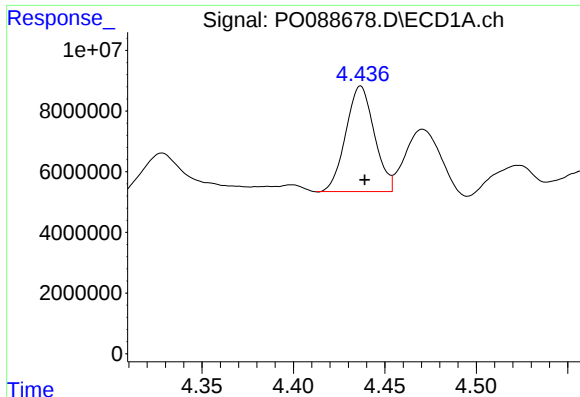


#1 Tetrachloro-m-xylene

R.T.: 4.436 min
Delta R.T.: -0.003 min
Response: 37776885
Conc: 14.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
33773-74


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2022
Supervised By :Ankita Jodhani 08/08/2022

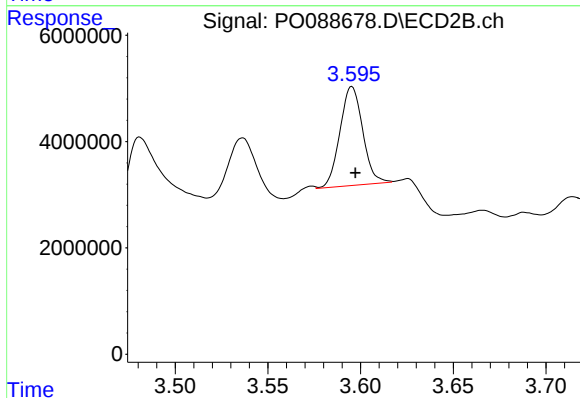


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: -0.002 min
Response: 15890620
Conc: 14.68 ng/ml m

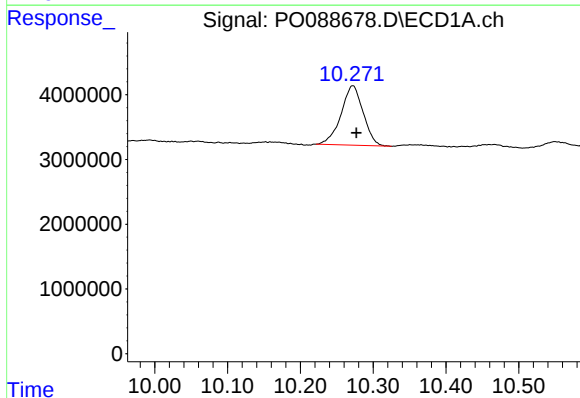

#2 Decachlorobiphenyl

R.T.: 10.272 min
Delta R.T.: -0.005 min
Response: 19429458
Conc: 10.07 ng/ml

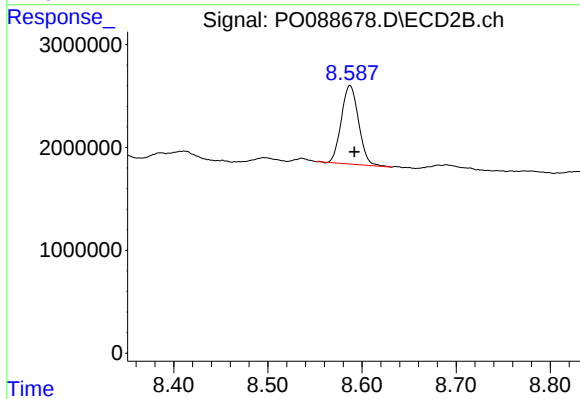

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.004 min
Response: 9756339
Conc: 8.05 ng/ml