

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080618\
Data File : P0047755.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2018 23:33
Operator : SM/SJ
Sample : J4331-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
073118-TIPC-E-U-M

Manual Integrations
APPROVED

Sohil
8/7/2018 3:55:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 08:52:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.398	3.642	3892401	3953505	19.279	16.090m
2)	SA Decachlor...	10.088	8.628	2893999	3081051	17.744	19.601m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080618\
Data File : P0047755.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2018 23:33
Operator : SM/SJ
Sample : J4331-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
073118-TIPC-E-U-M


Manual Integrations
APPROVED

Sohil
8/7/2018 3:55:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 08:52:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

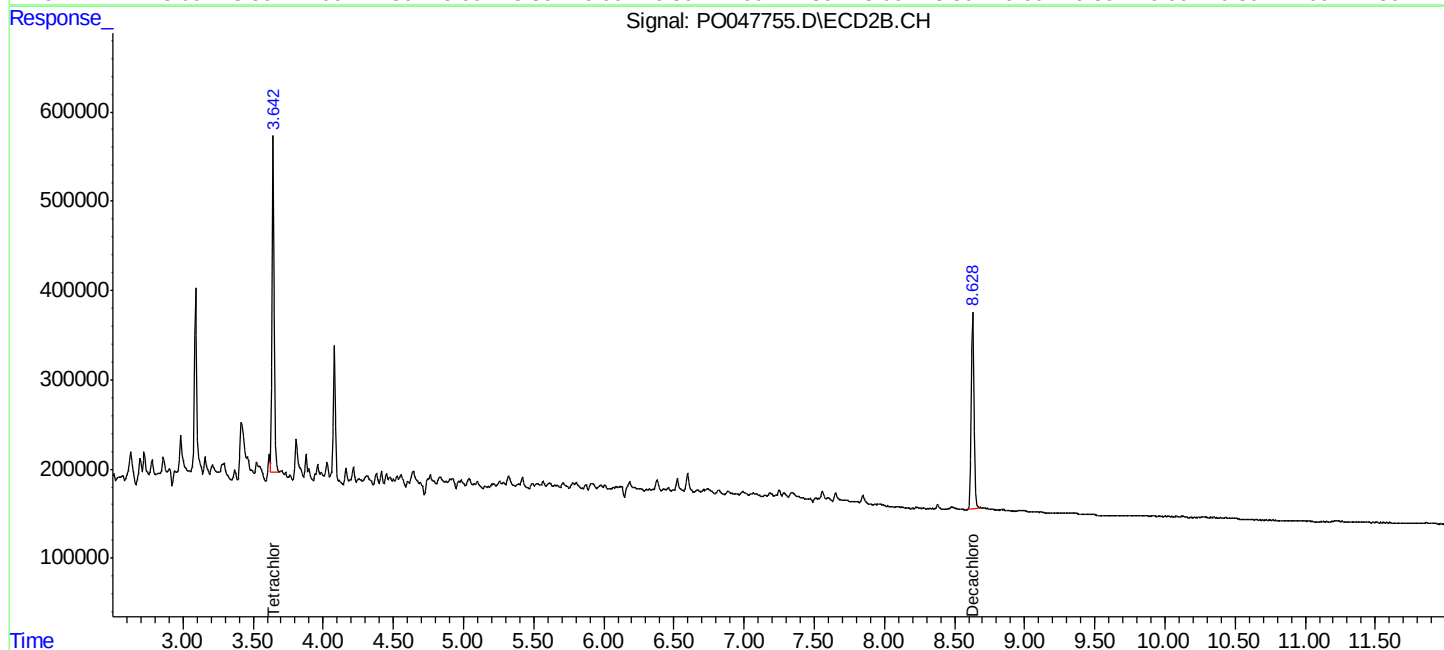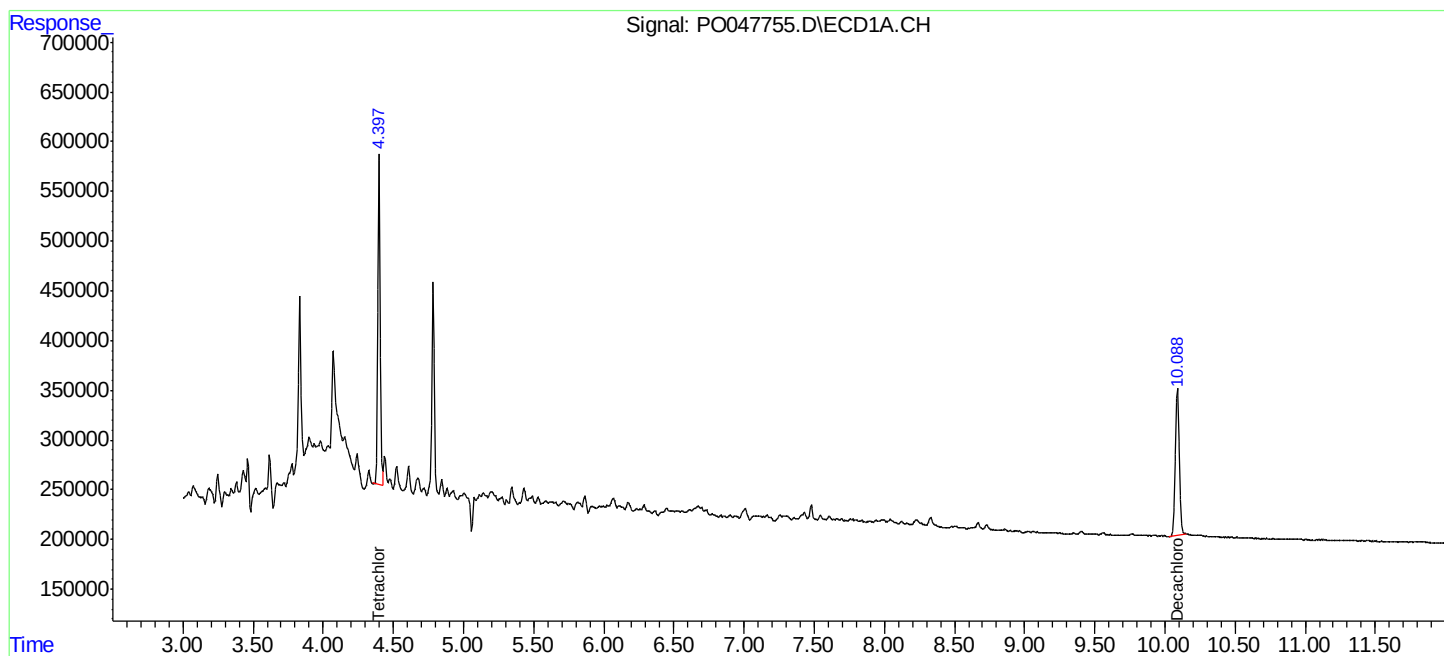

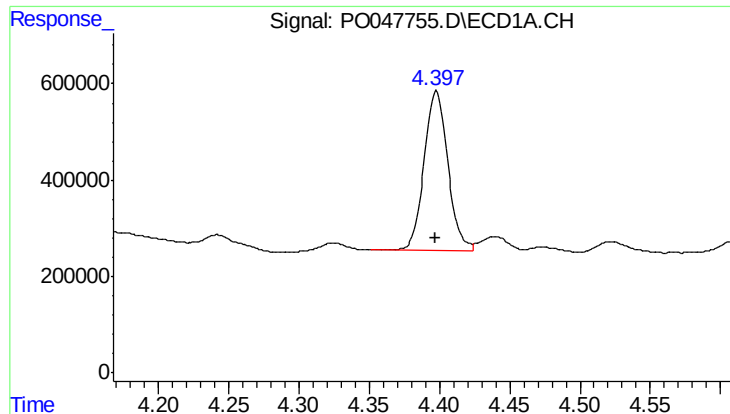


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3892401
Conc: 19.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
073118-TIPC-E-U-M


Manual Integrations
APPROVED

Sohil
8/7/2018 3:55:27 PM

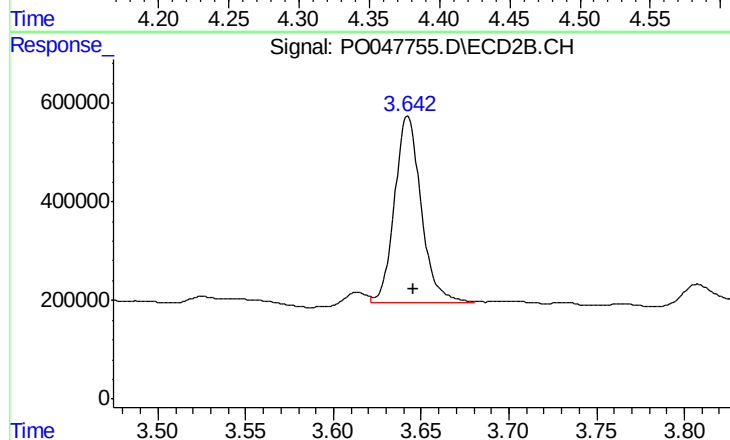


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 3953505
Conc: 16.09 ng/ml m

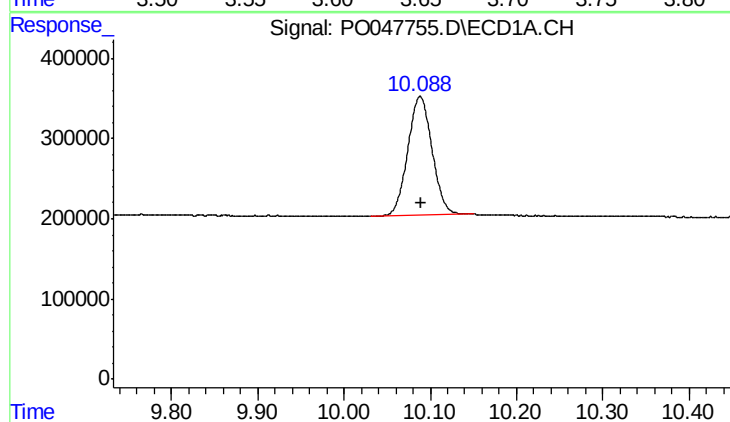

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.002 min
Response: 2893999
Conc: 17.74 ng/ml

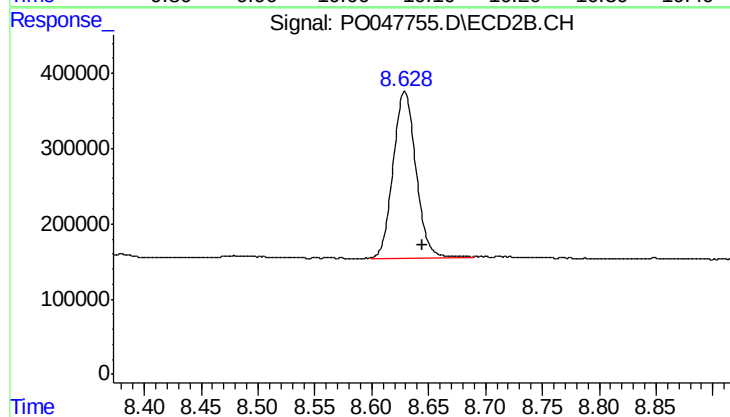

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.016 min
Response: 3081051
Conc: 19.60 ng/ml m