

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0080618\
 Data File : P0047769.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2018 6:40
 Operator : SM/SJ
 Sample : J4327-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-02-007-ABCD

Manual Integrations
 APPROVED

Sohil
 8/7/2018 3:55:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 09:26:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.643	4525741	5285475	22.416	21.511
2) SA Decachlor...	10.089	8.628	2769952	2824964	16.983	17.971m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0080618\
Data File : P0047769.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2018 6:40
Operator : SM/SJ
Sample : J4327-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-02-007-ABCD


Manual Integrations
APPROVED

Sohil
8/7/2018 3:55:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 09:26:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

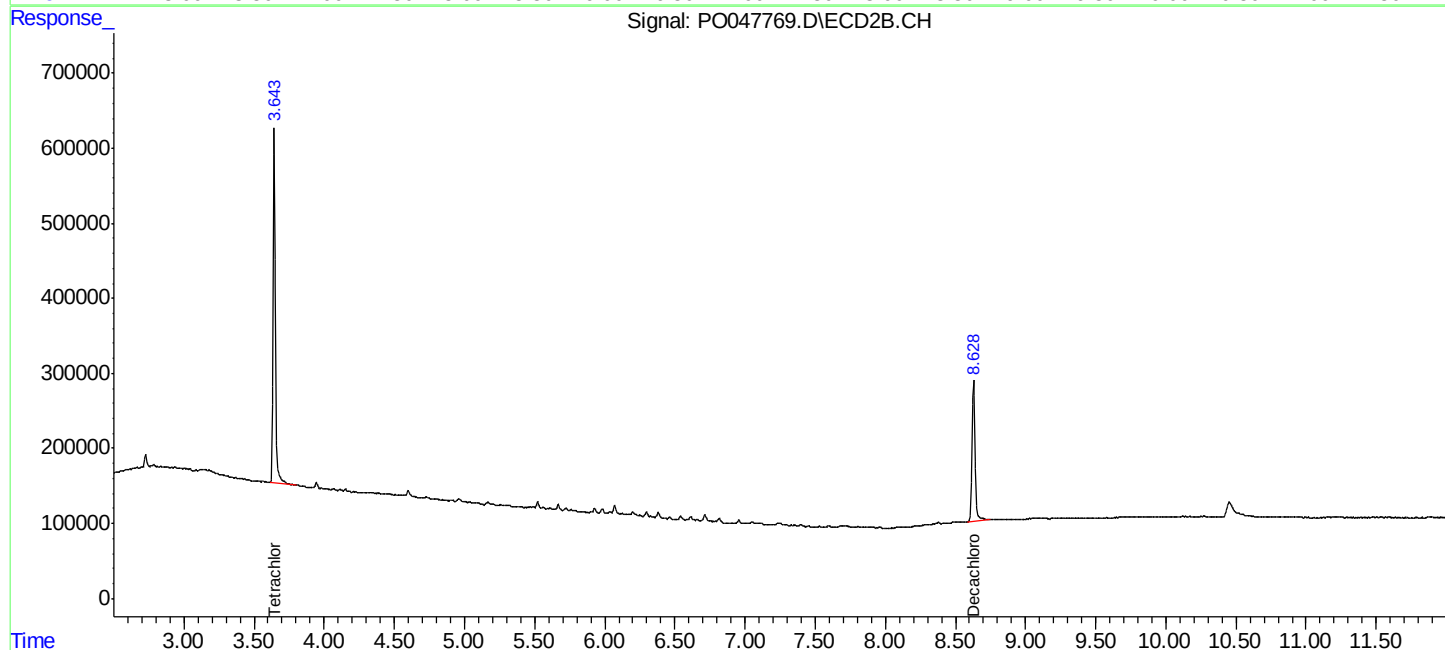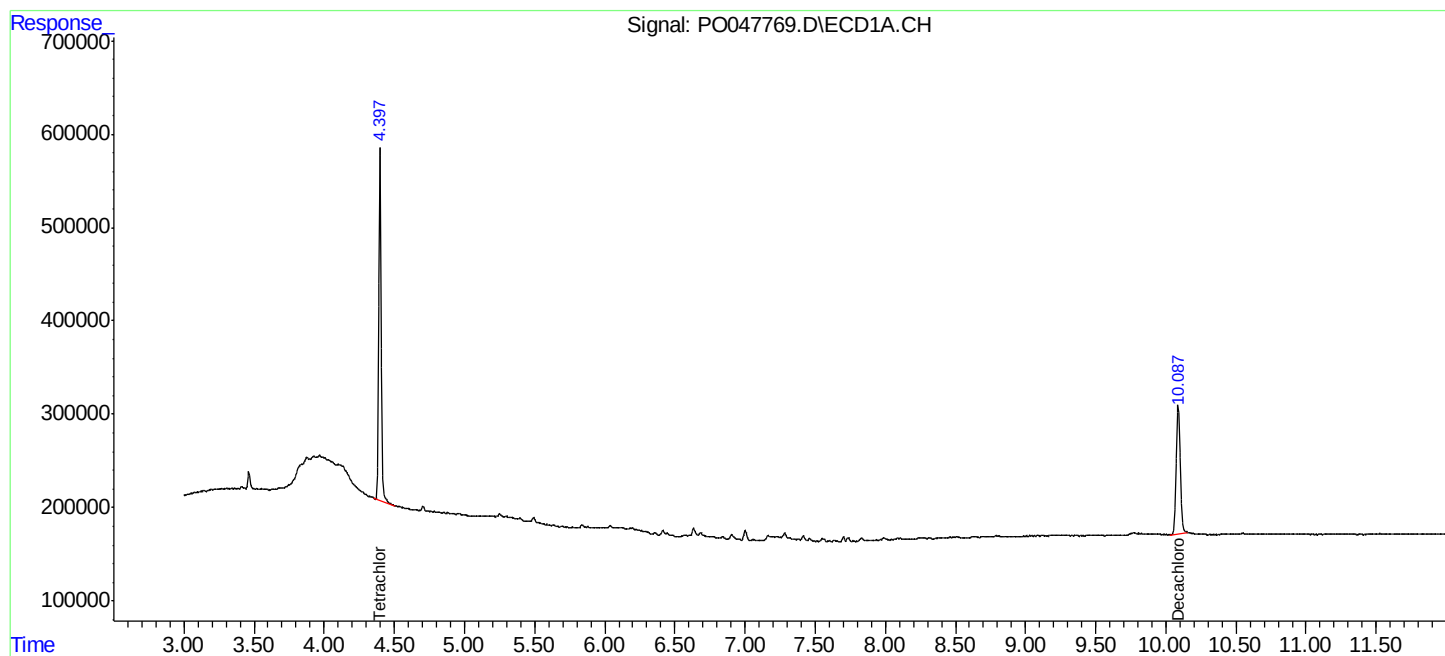

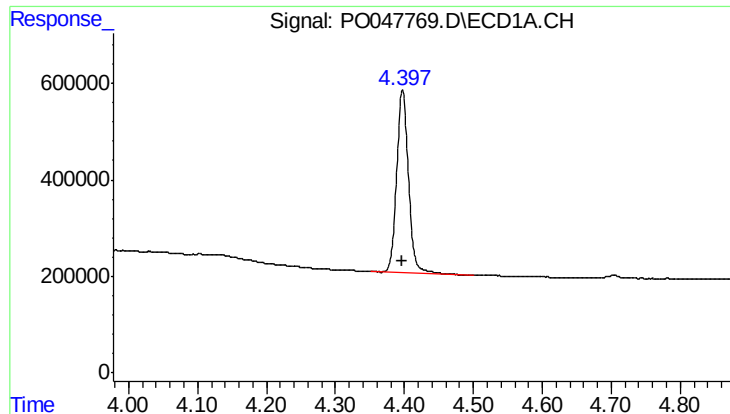


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 4525741
Conc: 22.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-02-007-ABCD


Manual Integrations
APPROVED

Sohil
8/7/2018 3:55:52 PM

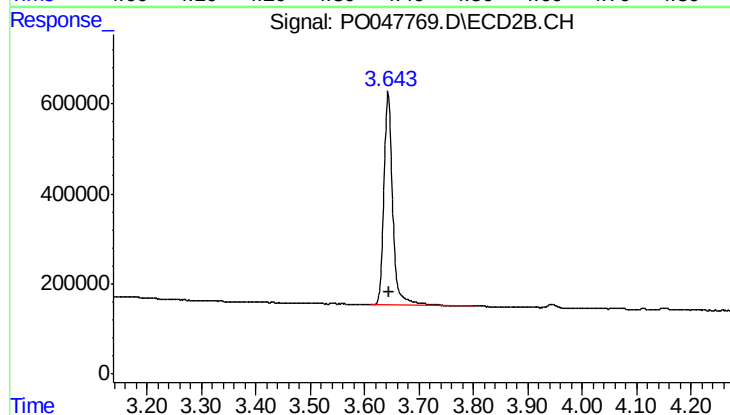


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 5285475
Conc: 21.51 ng/ml

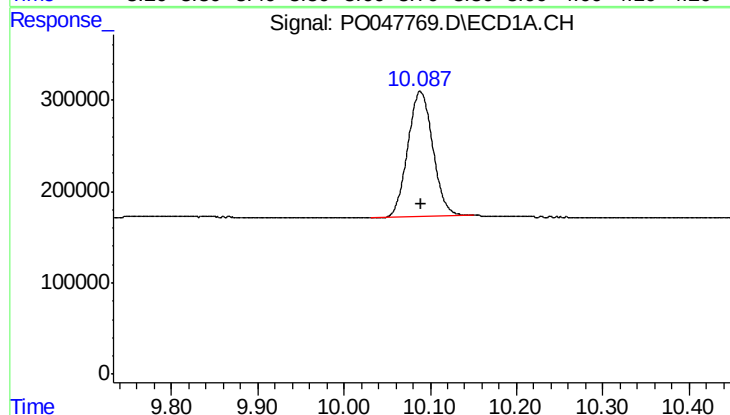

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.001 min
Response: 2769952
Conc: 16.98 ng/ml

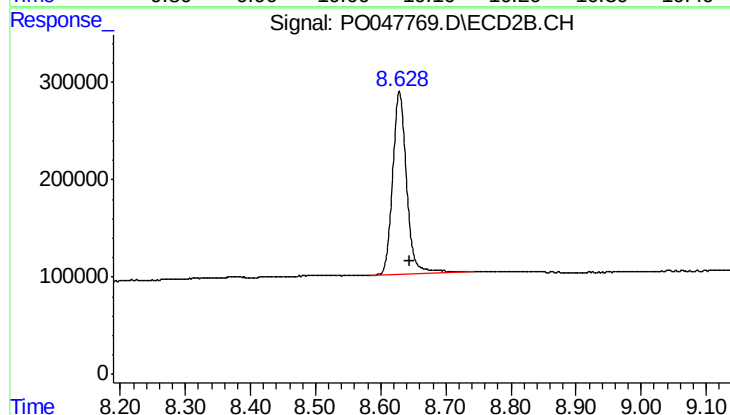

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.016 min
Response: 2824964
Conc: 17.97 ng/ml m