

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080619\
 Data File : P0058922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2019 10:40
 Operator : SM/AJ
 Sample : K4114-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-TEST-PITRE

Manual Integrations
 APPROVED

Ankita
 8/7/2019 5:50:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 13:14:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.157	3.516	479278	392514	11.357	9.825
2)	SA Decachlor...	9.666	8.397	368323	291278	6.801m	7.379
Target Compounds							
31)	L7 AR-1260-1	6.894	6.023	209517	182935	72.770m	76.862
32)	L7 AR-1260-2	7.149	6.212	619996	537472	149.036m	177.424
33)	L7 AR-1260-3	7.505	6.359	345697	157446	92.830m	58.317m#
34)	L7 AR-1260-4	7.732	6.824	260066	198048	76.315m	87.650
35)	L7 AR-1260-5	8.040	7.067	814620	660392	110.761m	122.628

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080619\
Data File : PO058922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2019 10:40
Operator : SM/AJ
Sample : K4114-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CS-TEST-PITRE


Manual Integrations
APPROVED

Ankita
8/7/2019 5:50:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 13:14:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

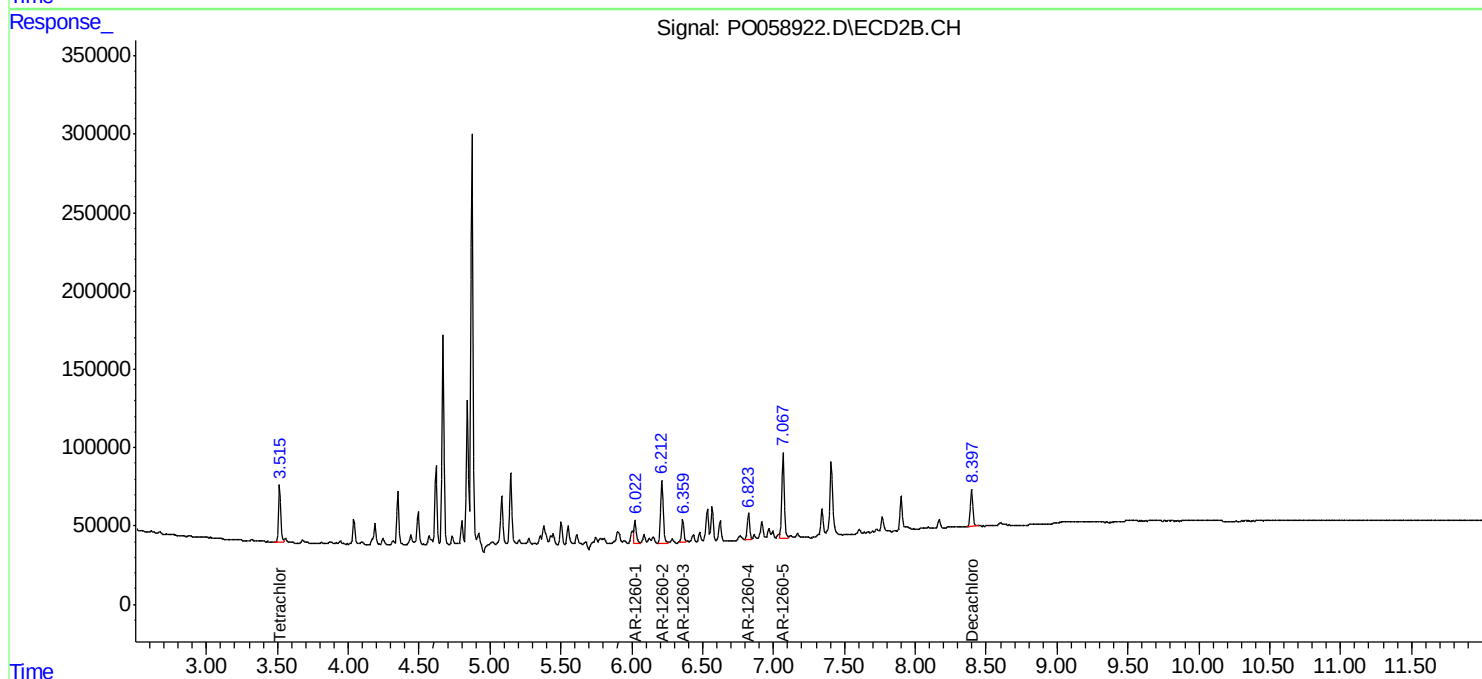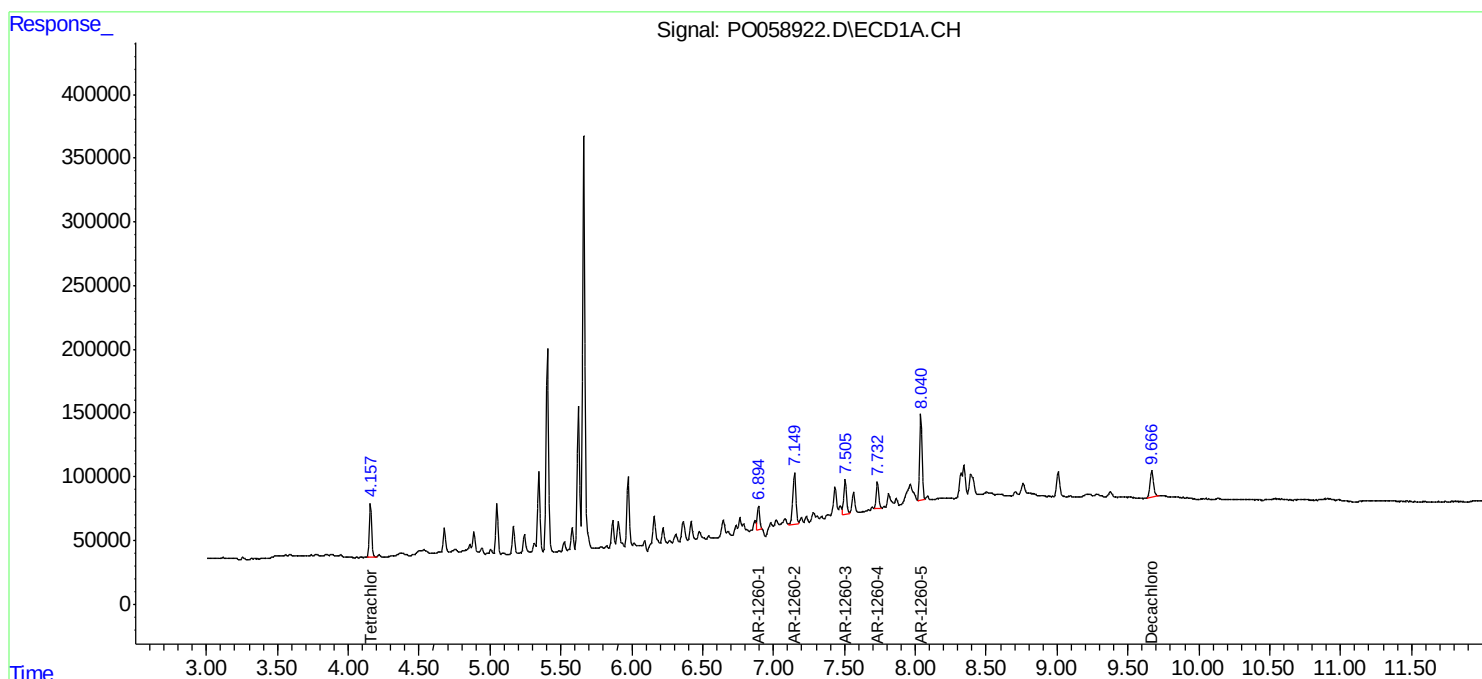

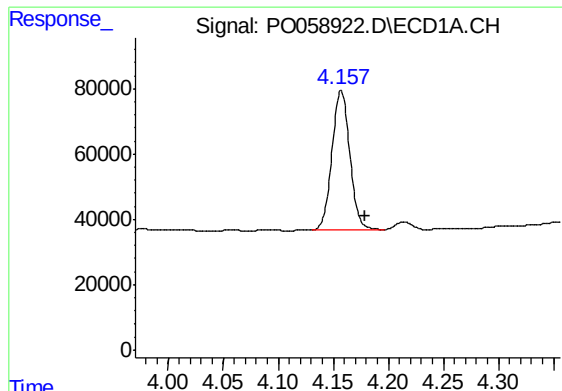


#1 Tetrachloro-m-xylene

R.T.: 4.157 min
Delta R.T.: -0.022 min
Response: 479278
Conc: 11.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PITRE


Manual Integrations
APPROVED

Ankita
8/7/2019 5:50:14 PM

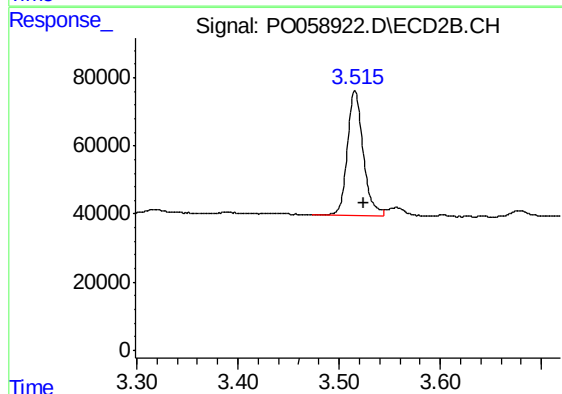


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 392514
Conc: 9.83 ng/ml

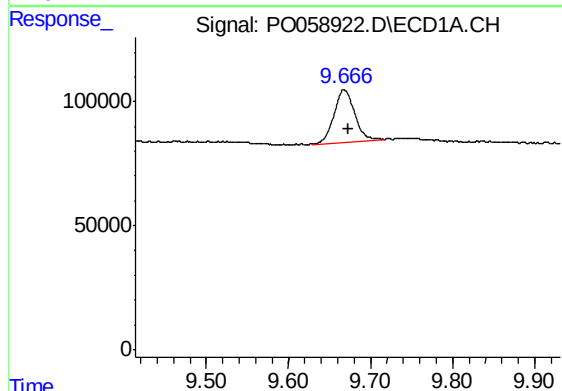


#2 Decachlorobiphenyl

R.T.: 9.666 min
Delta R.T.: -0.006 min
Response: 368323
Conc: 6.80 ng/ml m

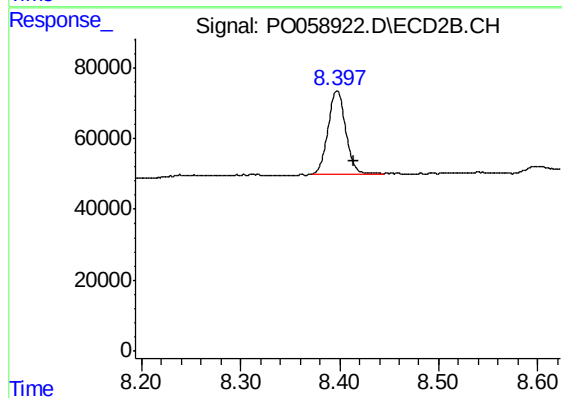

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.017 min
Response: 291278
Conc: 7.38 ng/ml

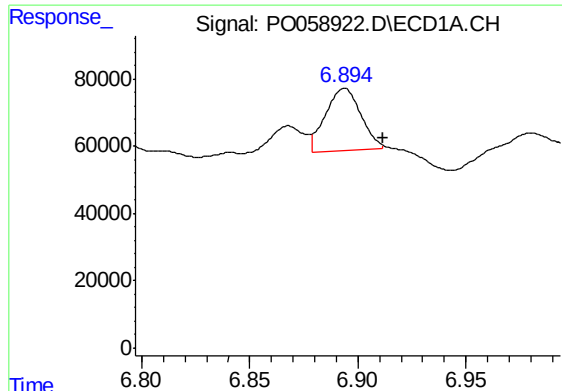


#31 AR-1260-1

R.T.: 6.894 min
Delta R.T.: -0.018 min
Response: 209517
Conc: 72.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PITRE


Manual Integrations
APPROVED

Ankita
8/7/2019 5:50:14 PM

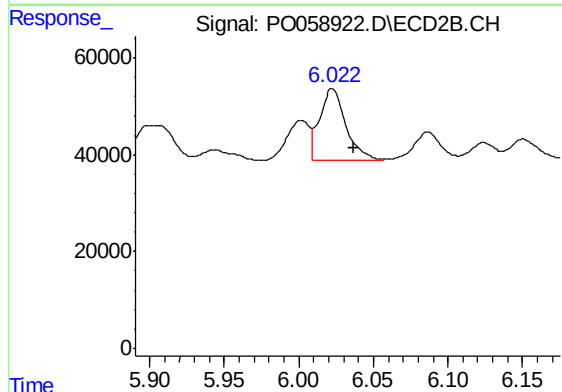


#31 AR-1260-1

R.T.: 6.023 min
Delta R.T.: -0.014 min
Response: 182935
Conc: 76.86 ng/ml

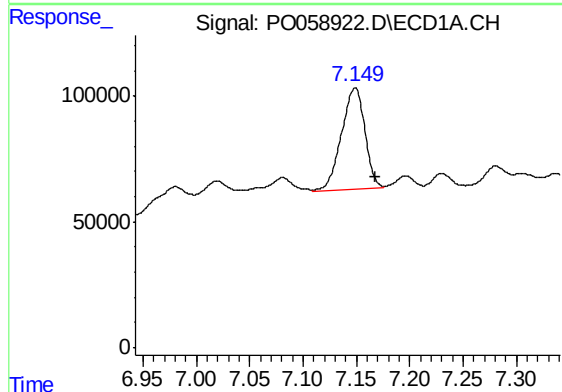


#32 AR-1260-2

R.T.: 7.149 min
Delta R.T.: -0.019 min
Response: 619996
Conc: 149.04 ng/ml m

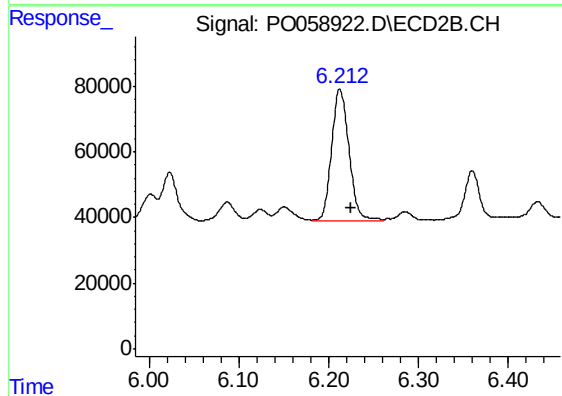

#32 AR-1260-2

R.T.: 6.212 min
Delta R.T.: -0.012 min
Response: 537472
Conc: 177.42 ng/ml

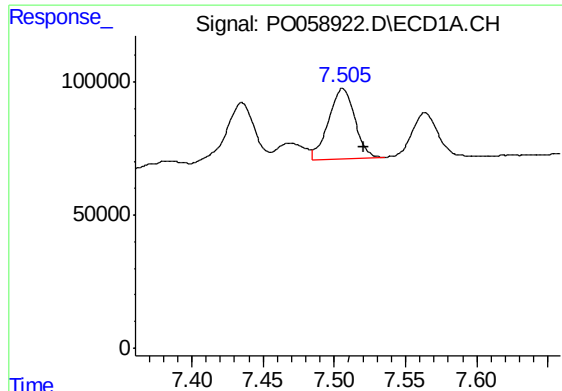


#33 AR-1260-3

R.T.: 7.505 min
Delta R.T.: -0.015 min
Response: 345697
Conc: 92.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PITRE


Manual Integrations
APPROVED

Ankita
8/7/2019 5:50:14 PM

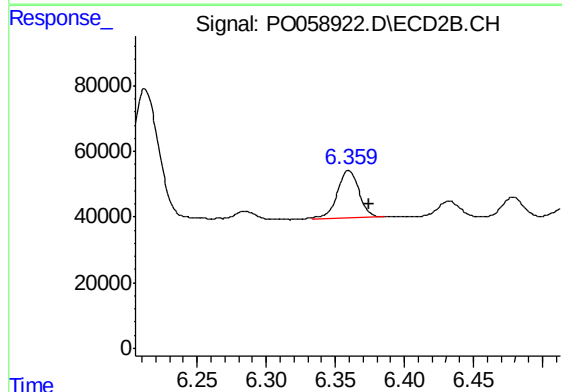


#33 AR-1260-3

R.T.: 6.359 min
Delta R.T.: -0.015 min
Response: 157446
Conc: 58.32 ng/ml m

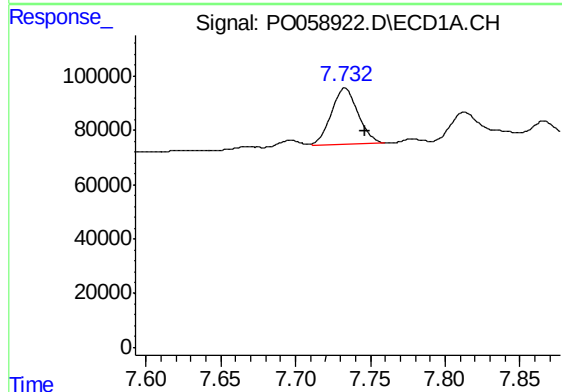


#34 AR-1260-4

R.T.: 7.732 min
Delta R.T.: -0.014 min
Response: 260066
Conc: 76.32 ng/ml m

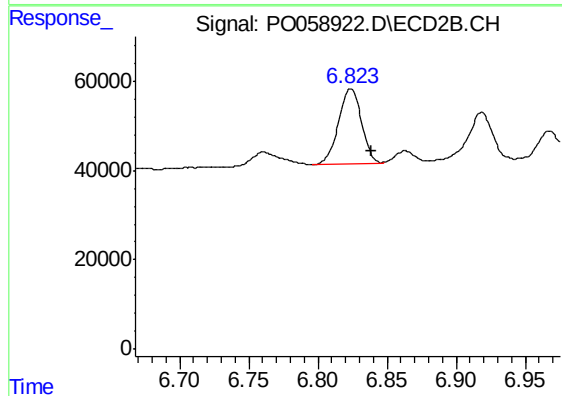

#34 AR-1260-4

R.T.: 6.824 min
Delta R.T.: -0.015 min
Response: 198048
Conc: 87.65 ng/ml

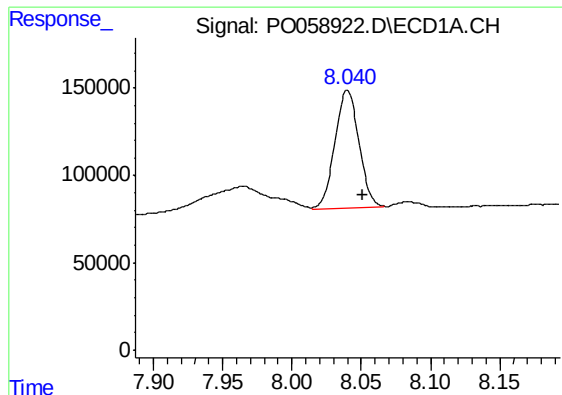


#35 AR-1260-5

R.T.: 8.040 min
Delta R.T.: -0.012 min
Response: 814620
Conc: 110.76 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CS-TEST-PITRE

Manual Integrations
APPROVED

Ankita
8/7/2019 5:50:14 PM

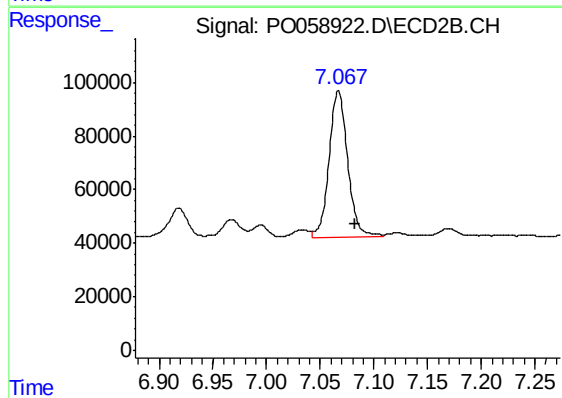

#35 AR-1260-5

R.T.: 7.067 min
Delta R.T.: -0.015 min
Response: 660392
Conc: 122.63 ng/ml