

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080619\
Data File : P0058943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2019 18:13
Operator : SM/AJ
Sample : K4154-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PS-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 02:08:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.160	3.516	566643	532664	13.427	13.333
2)	SA Decachlor...	9.677	8.399	511871	345856	9.452	8.762

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080619\
Data File : PO058943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2019 18:13
Operator : SM/AJ
Sample : K4154-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
PS-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 02:08:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

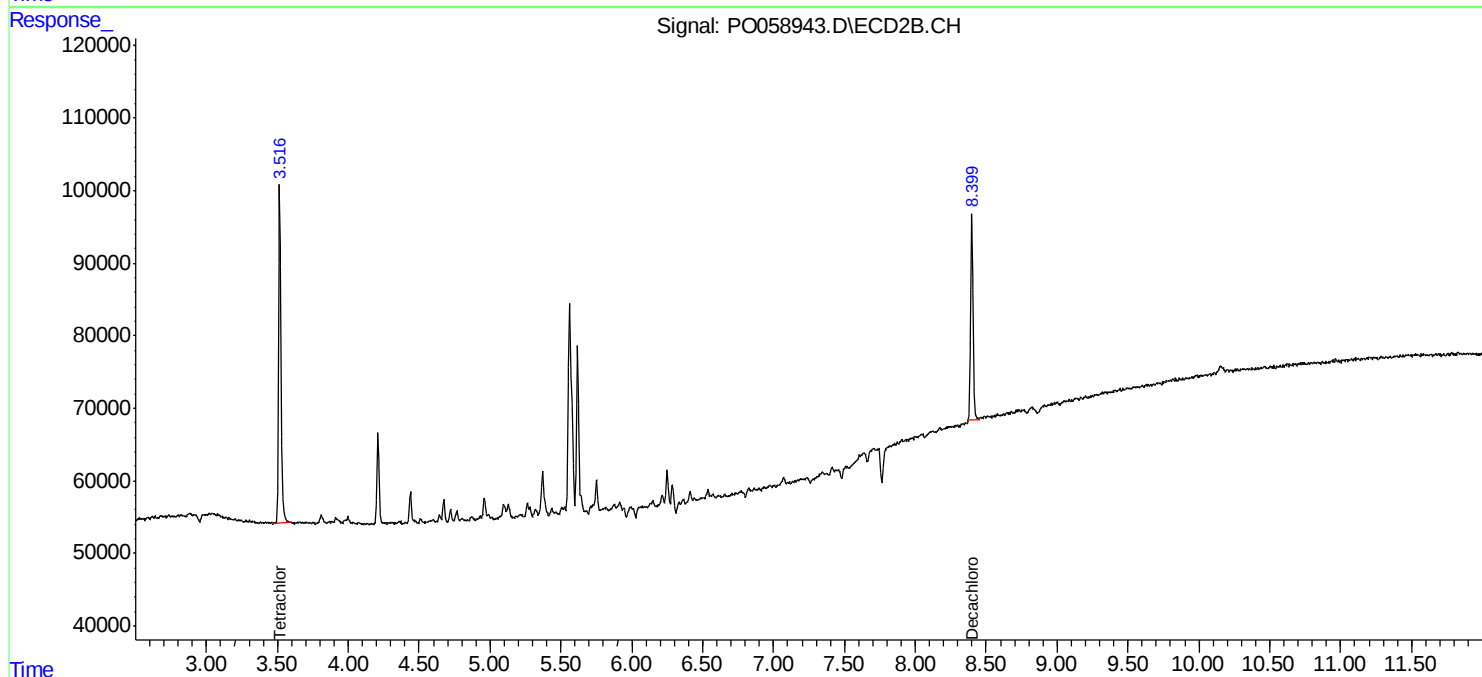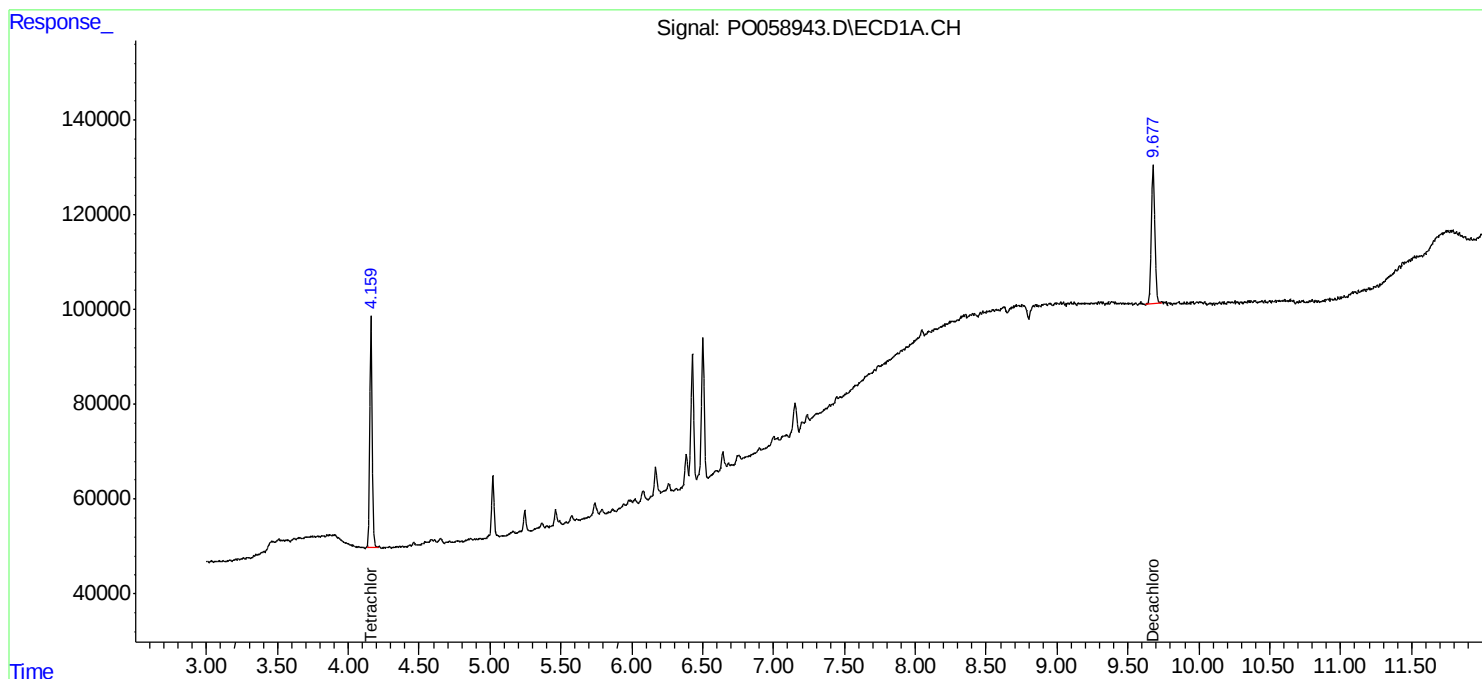


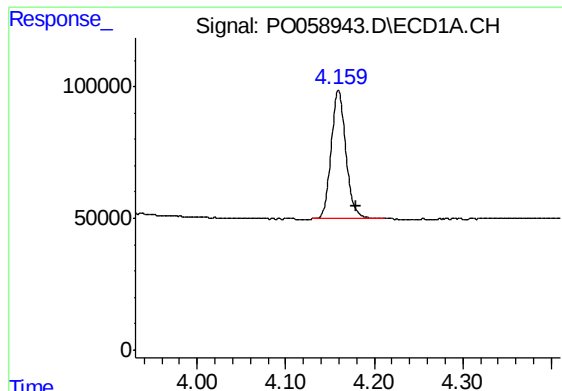

#1 Tetrachloro-m-xylene


R.T.: 4.160 min
Delta R.T.: -0.019 min
Response: 566643
Conc: 13.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
PS-3

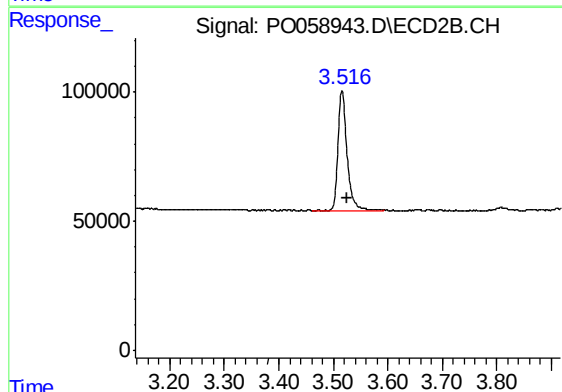


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 532664
Conc: 13.33 ng/ml

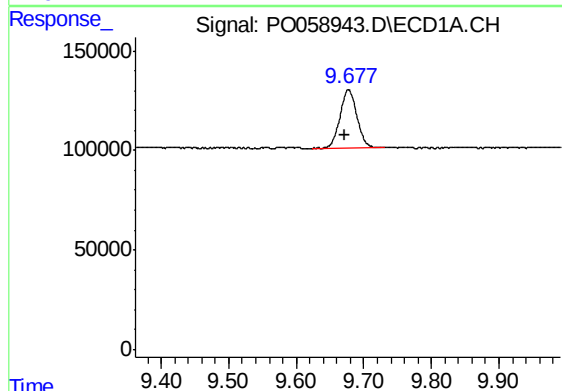

#2 Decachlorobiphenyl

R.T.: 9.677 min
Delta R.T.: 0.005 min
Response: 511871
Conc: 9.45 ng/ml

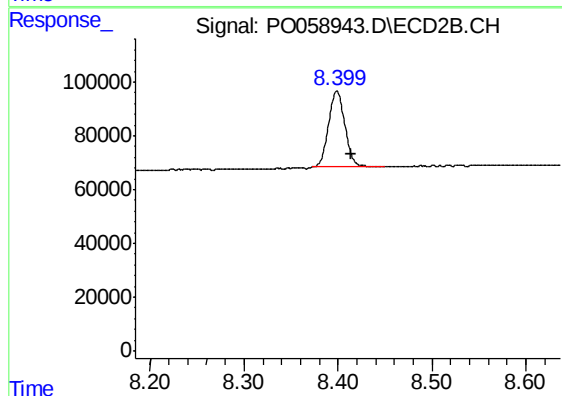

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.015 min
Response: 345856
Conc: 8.76 ng/ml