

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080619\
 Data File : P0058967.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Aug 2019 1:08
 Operator : SM/AJ
 Sample : K4104-18RE
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-3-WATERRE

Manual Integrations
 APPROVED

Ankita
 8/7/2019 5:53:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 02:24:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.155	3.517	456439	404953	10.815m	10.136m
2)	SA Decachlor...	9.666	8.399	304292	200110	5.619	5.070

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080619\
Data File : PO058967.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Aug 2019 1:08
Operator : SM/AJ
Sample : K4104-18RE
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-3-WATERRE


Manual Integrations
APPROVED

Ankita
8/7/2019 5:53:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 02:24:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

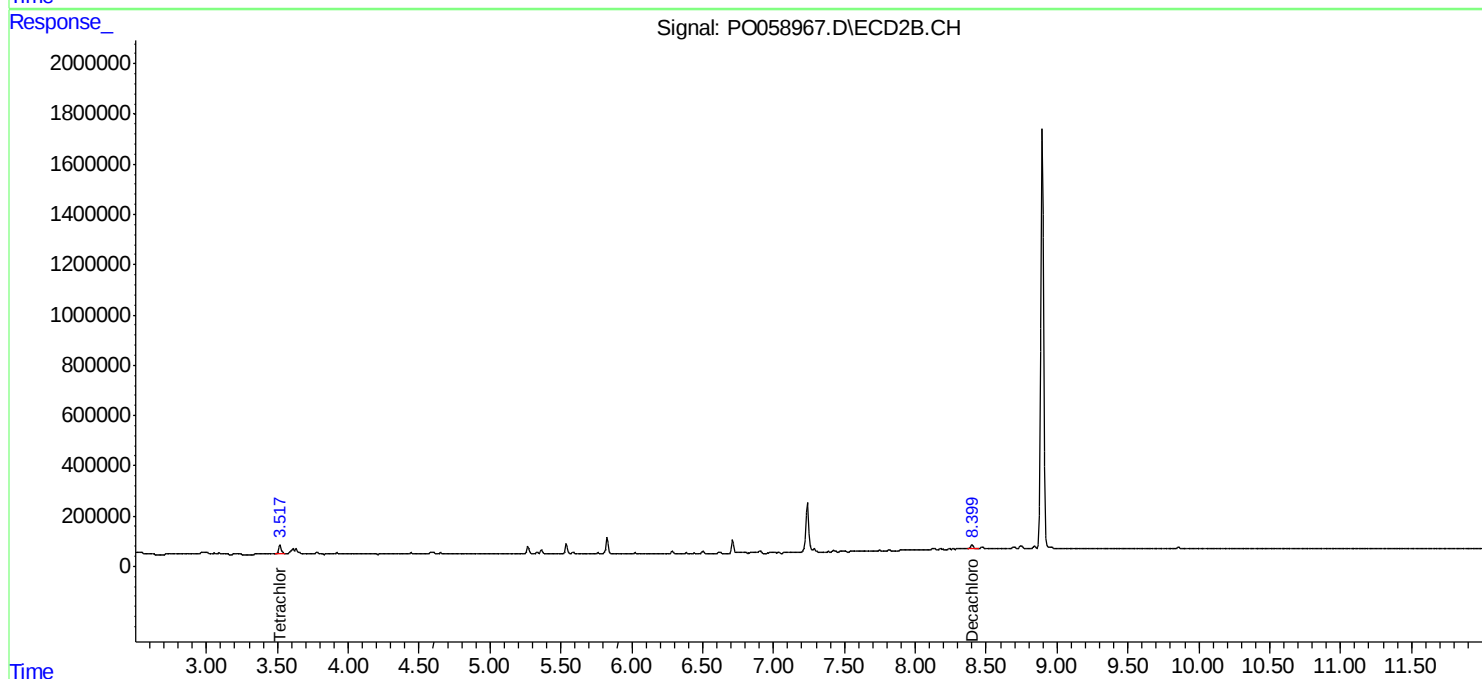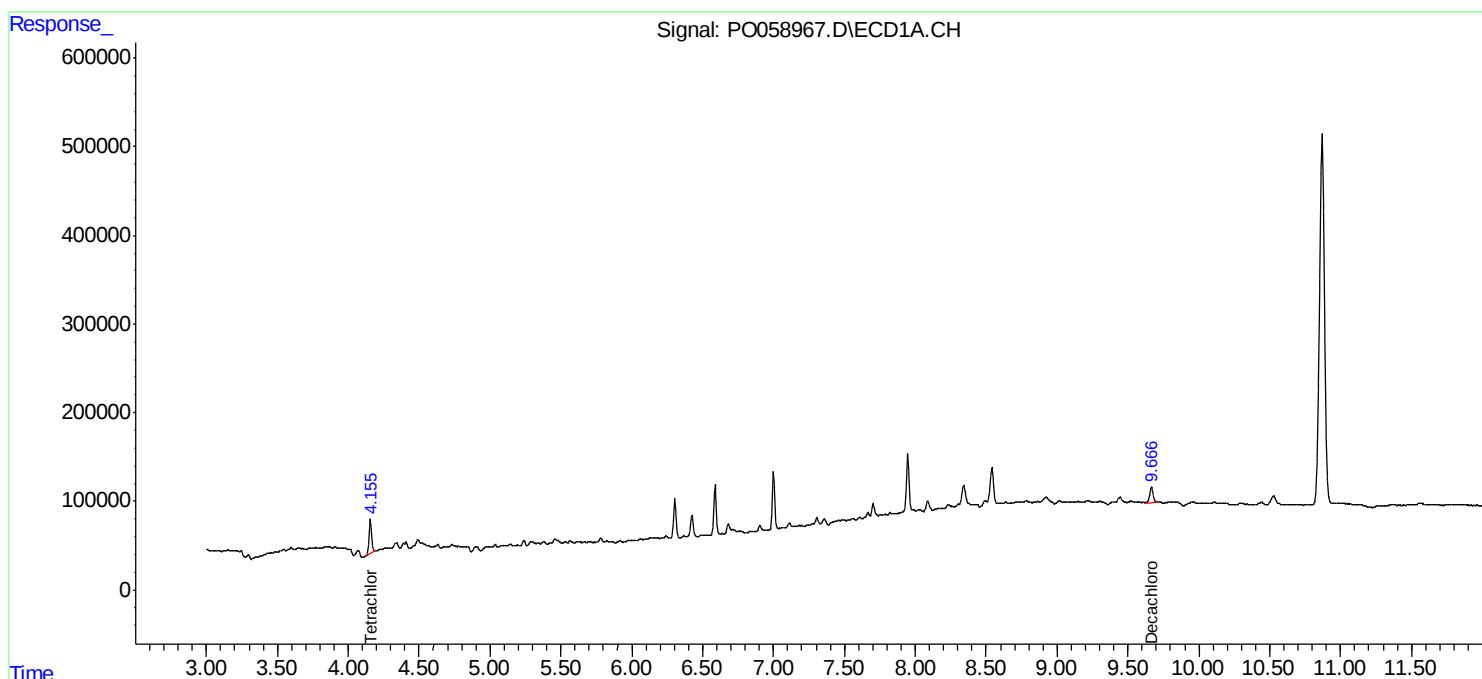

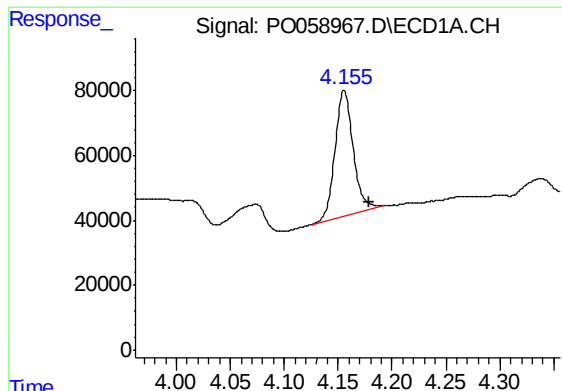


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: -0.024 min
Response: 456439
Conc: 10.82 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-3-WATERRE


Manual Integrations
APPROVED

Ankita
8/7/2019 5:53:01 PM

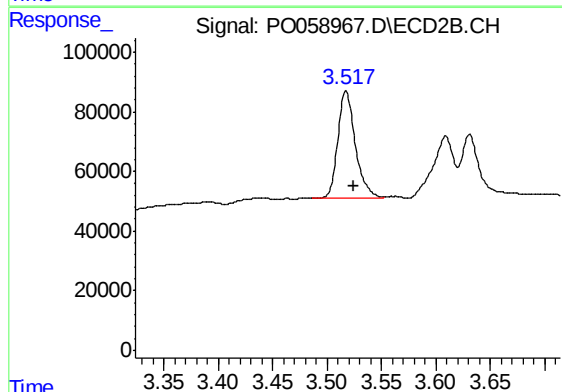


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: -0.008 min
Response: 404953
Conc: 10.14 ng/ml m

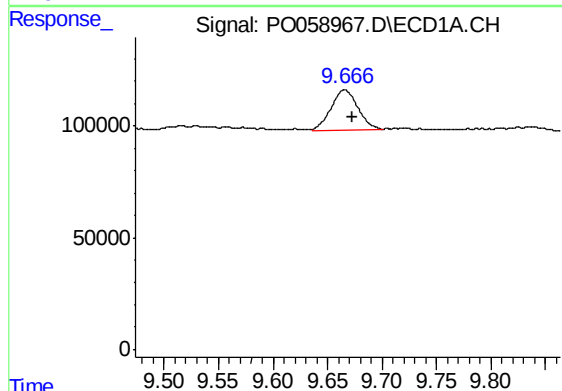

#2 Decachlorobiphenyl

R.T.: 9.666 min
Delta R.T.: -0.007 min
Response: 304292
Conc: 5.62 ng/ml

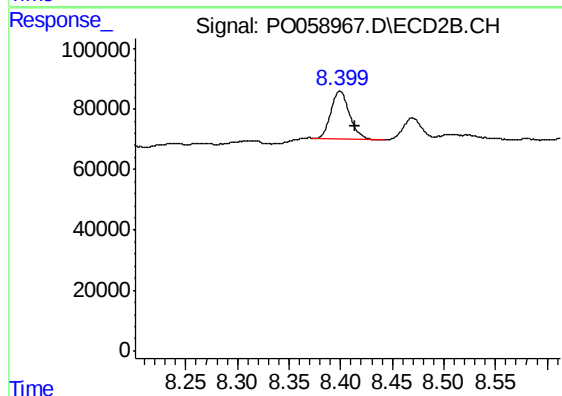

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.015 min
Response: 200110
Conc: 5.07 ng/ml