

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
 Data File : P0070298.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2020 9:04
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 14:44:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.375	3.559	1216624	813623	18.399	18.467
2)	SA Decachlor...	10.004	8.751	1719890	1070716	20.086	19.289
Target Compounds							
9)	L2 AR-1221-2	4.716	0.000	24279	0	38.593	N.D. #
12)	L3 AR-1232-2	5.395	0.000	3363	0	4.088	N.D. #
20)	L4 AR-1242-5	6.629	0.000	101319	0	49.189	N.D. #
24)	L5 AR-1248-4	6.604	0.000	14484	0	4.257	N.D. #
25)	L5 AR-1248-5	6.629	0.000	101319	0	31.853	N.D. #
26)	L6 AR-1254-1	6.586f	0.000	85140	0	23.926	N.D. #
35)	L7 AR-1260-5	8.508	0.000	5457	0	0.490	N.D. #
37)	L8 AR-1262-2	8.496	0.000	8444	0	0.670	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
Data File : P0070298.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2020 9:04
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 14:44:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

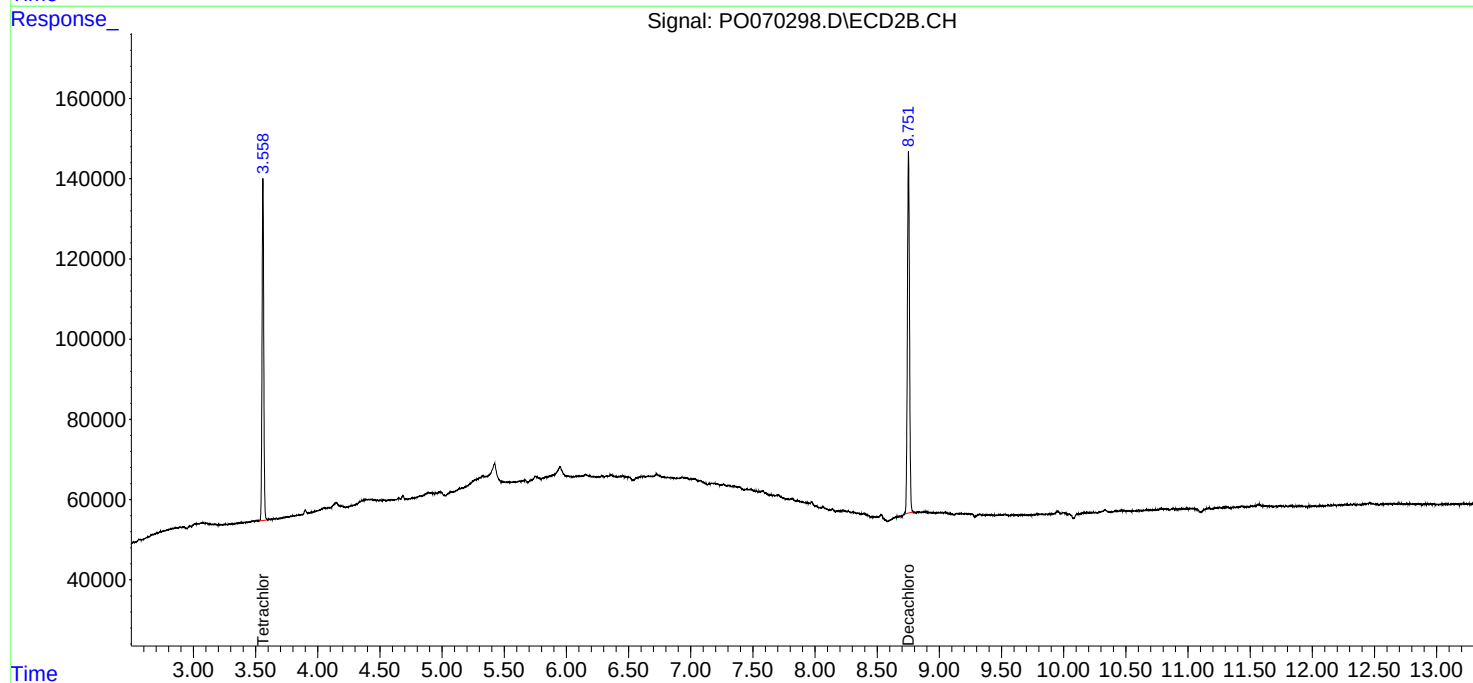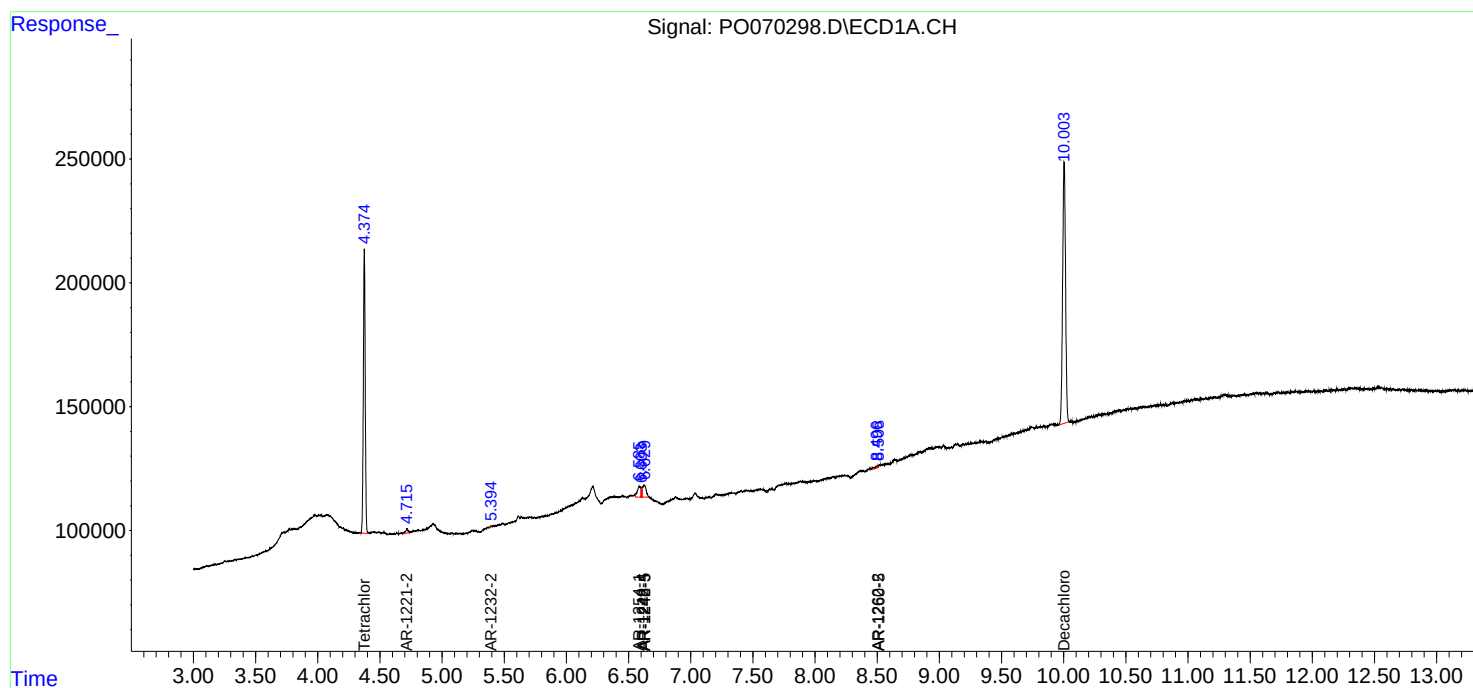


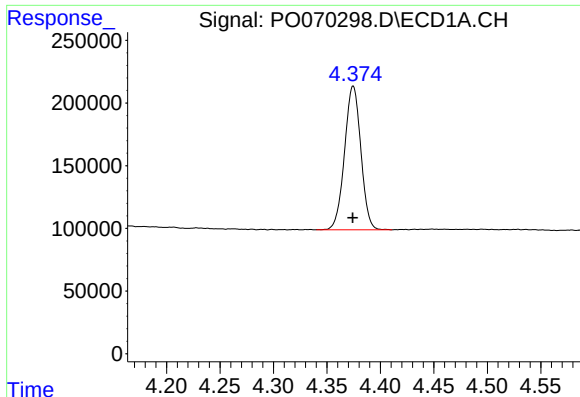

#1 Tetrachloro-m-xylene


R.T.: 4.375 min
Delta R.T.: 0.000 min
Response: 1216624
Conc: 18.40 ng/ml

Instrument :
ECD_O
ClientSampleId :

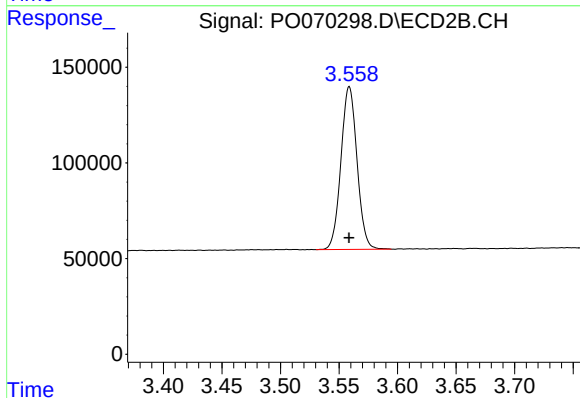


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: 0.000 min
Response: 813623
Conc: 18.47 ng/ml

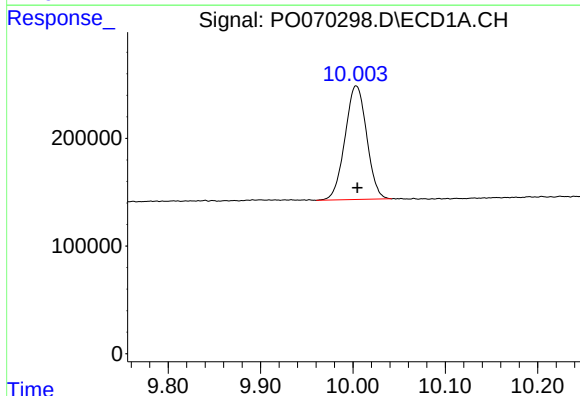


#2 Decachlorobiphenyl

R.T.: 10.004 min
Delta R.T.: -0.001 min
Response: 1719890
Conc: 20.09 ng/ml

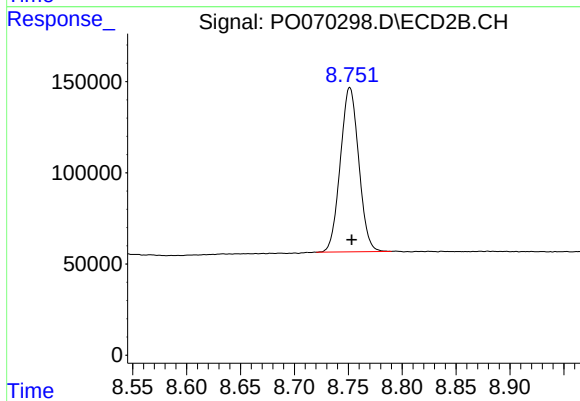

#2 Decachlorobiphenyl


R.T.: 8.751 min
Delta R.T.: -0.002 min
Response: 1070716
Conc: 19.29 ng/ml

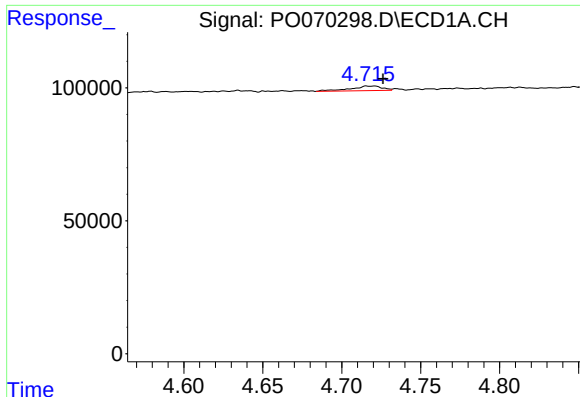

#9 AR-1221-2


R.T.: 4.716 min
Delta R.T.: -0.011 min
Response: 24279
Conc: 38.59 ng/ml

Instrument :
ECD_O
ClientSampleId :

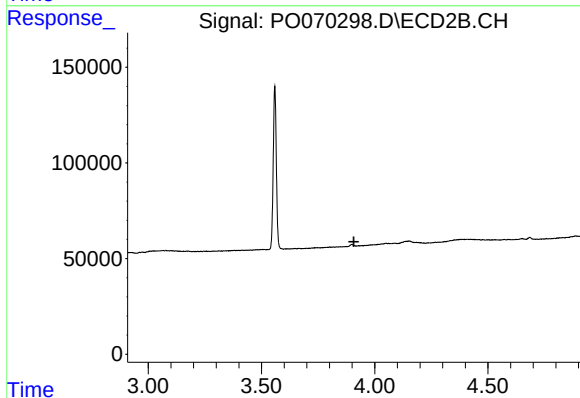


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

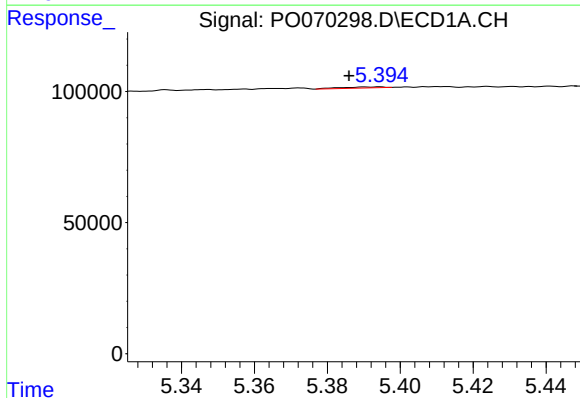


#12 AR-1232-2

R.T.: 5.395 min
Delta R.T.: 0.009 min
Response: 3363
Conc: 4.09 ng/ml

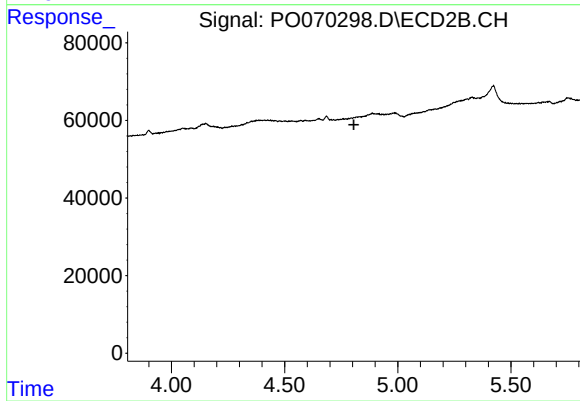

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.806 min
Response: 0
Conc: N.D.

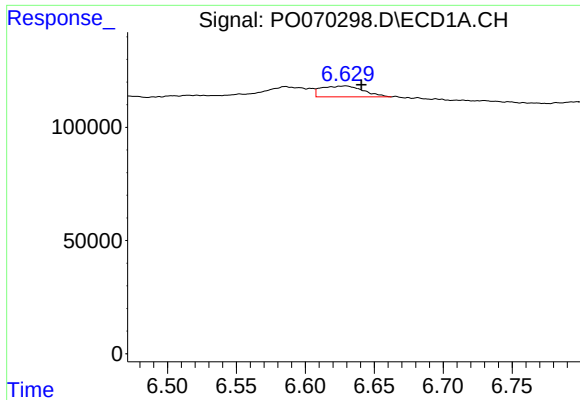

#20 AR-1242-5


R.T.: 6.629 min
Delta R.T.: -0.011 min
Response: 101319
Conc: 49.19 ng/ml

Instrument :
ECD_O
ClientSampleId :

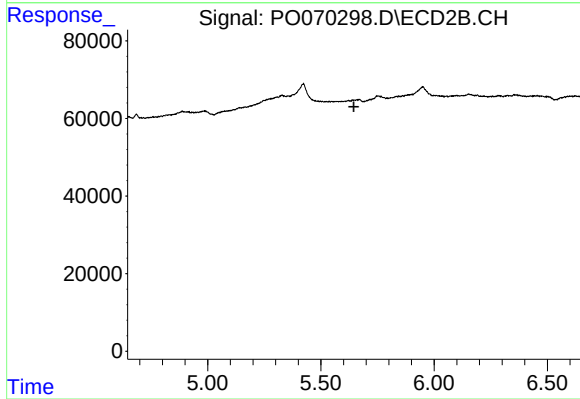


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.645 min
Response: 0
Conc: N.D.

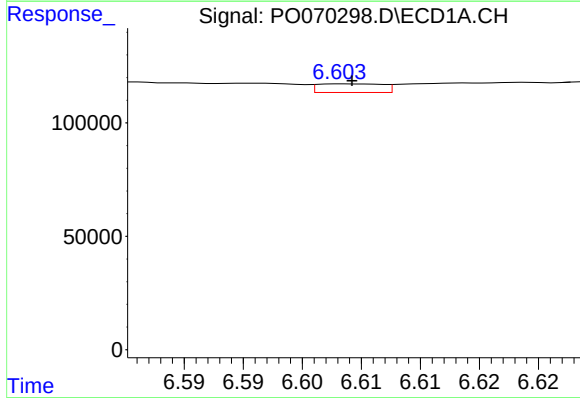


#24 AR-1248-4

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 14484
Conc: 4.26 ng/ml

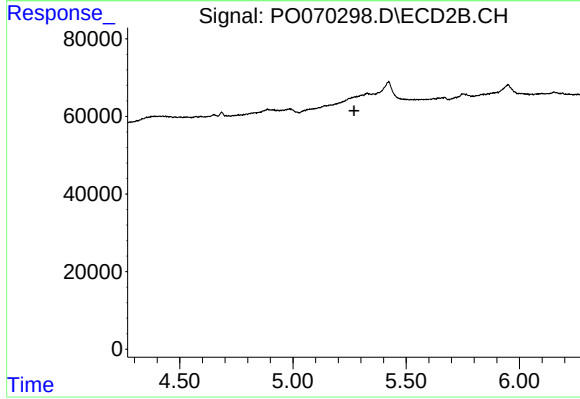

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.269 min
Response: 0
Conc: N.D.

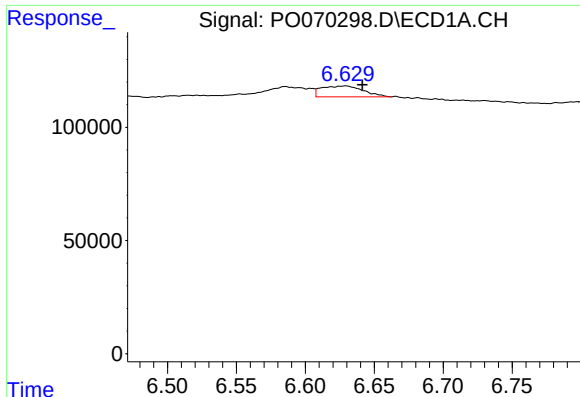

#25 AR-1248-5


R.T.: 6.629 min
Delta R.T.: -0.012 min
Response: 101319
Conc: 31.85 ng/ml

Instrument :
ECD_O
ClientSampleId :

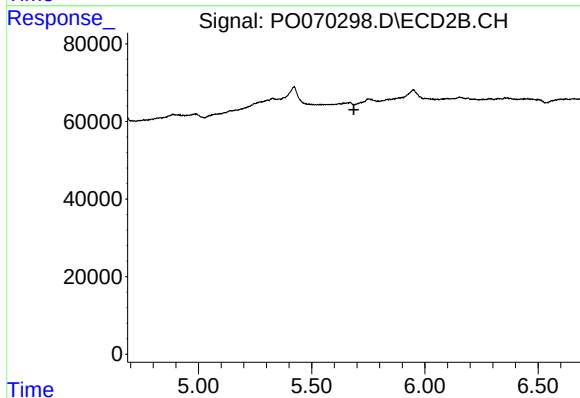


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.687 min
Response: 0
Conc: N.D.

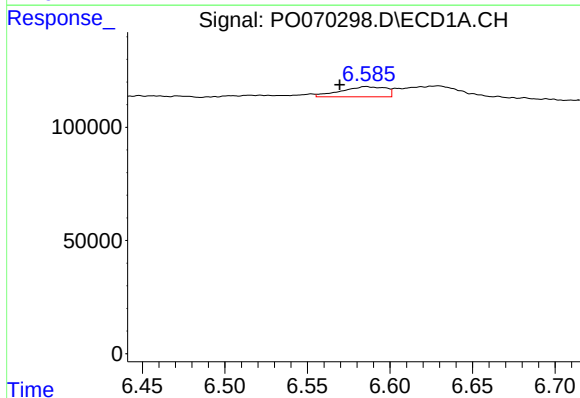


#26 AR-1254-1

R.T.: 6.586 min
Delta R.T.: 0.016 min
Response: 85140
Conc: 23.93 ng/ml

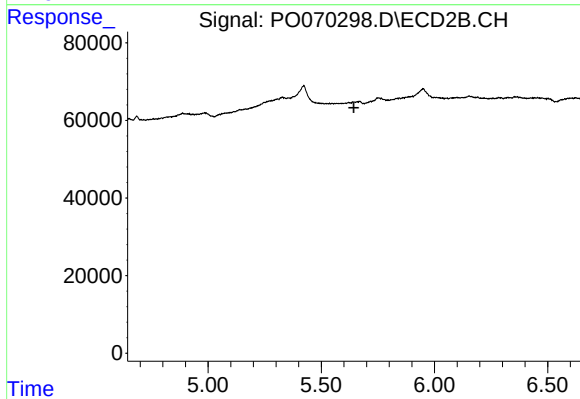

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

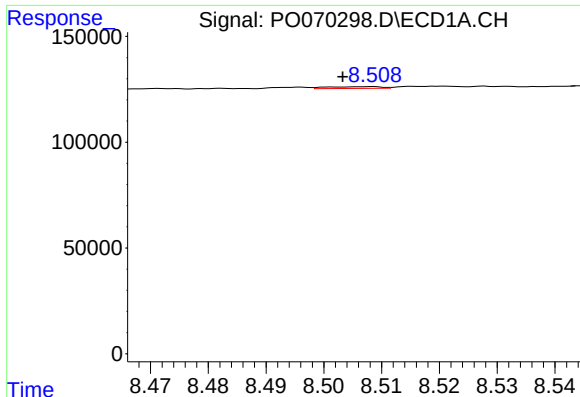

#35 AR-1260-5


R.T.: 8.508 min
Delta R.T.: 0.005 min
Response: 5457
Conc: 0.49 ng/ml

Instrument :
ECD_O
ClientSampleId :

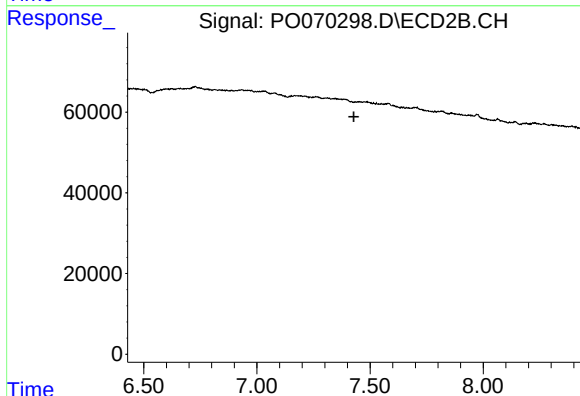


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.429 min
Response: 0
Conc: N.D.

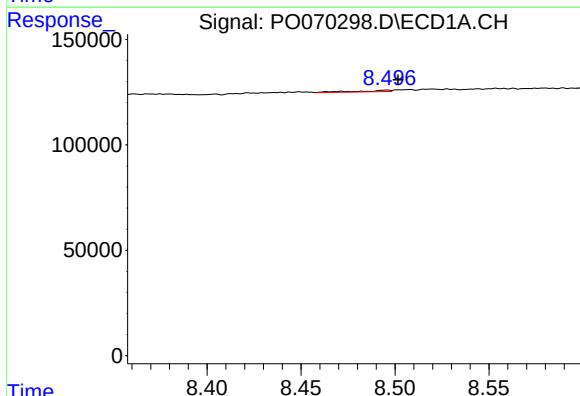

#37 AR-1262-2

R.T.: 8.496 min
Delta R.T.: -0.006 min
Response: 8444
Conc: 0.67 ng/ml

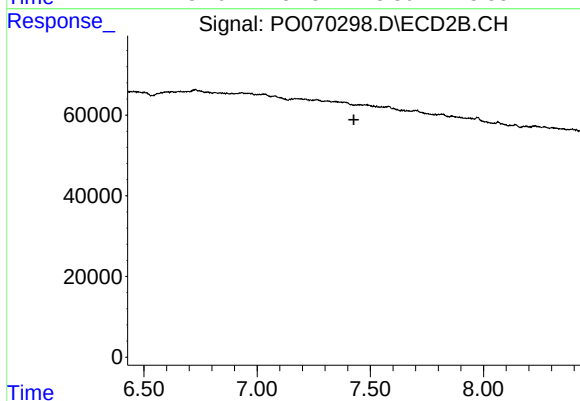

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.