

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
 Data File : P0070319.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2020 15:36
 Operator : DD\AJ
 Sample : L3512-04RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER-1493RE

Manual Integrations
 APPROVED

Ankita
 8/7/2020 1:14:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 17:05:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.561	471858	323779	7.136m	7.349
2) SA Decachlor...	10.002	8.753	242570	329297	2.833	5.932 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
Data File : P0070319.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2020 15:36
Operator : DD\AJ
Sample : L3512-04RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER-1493RE


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 17:05:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

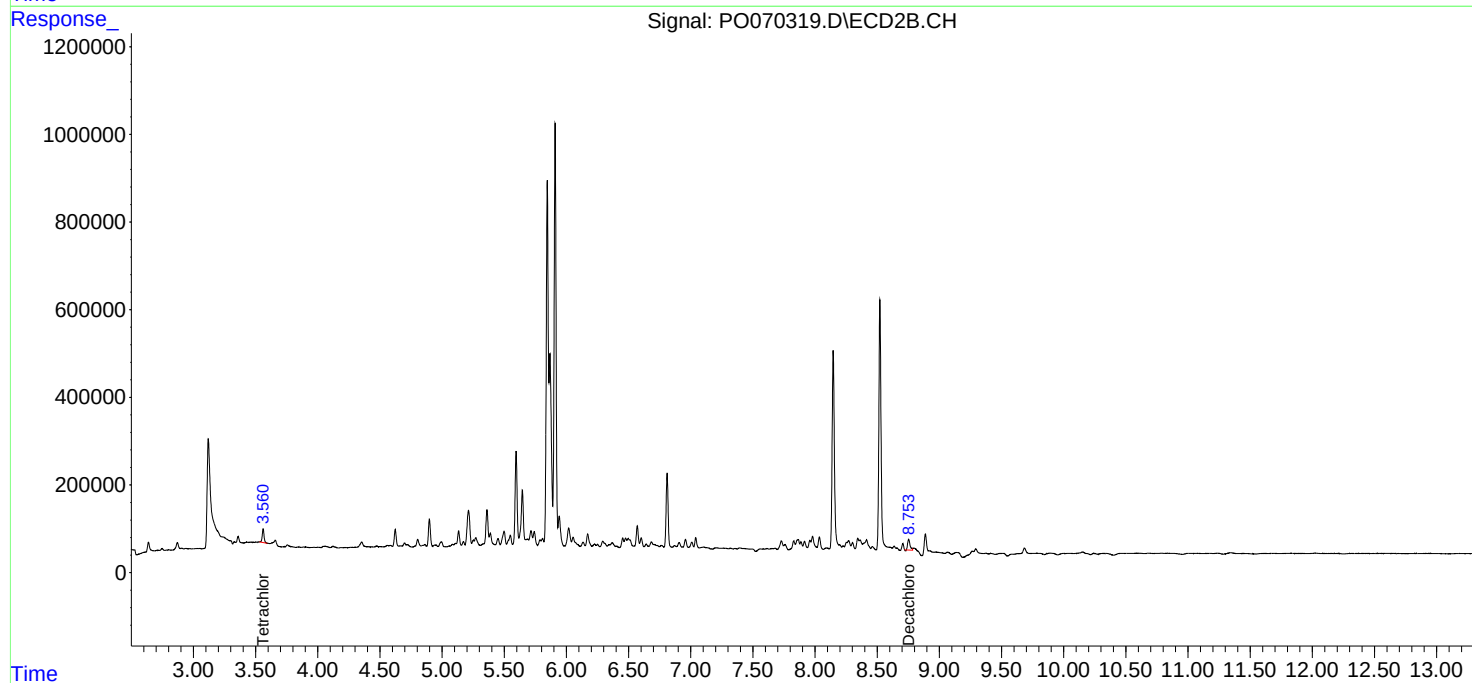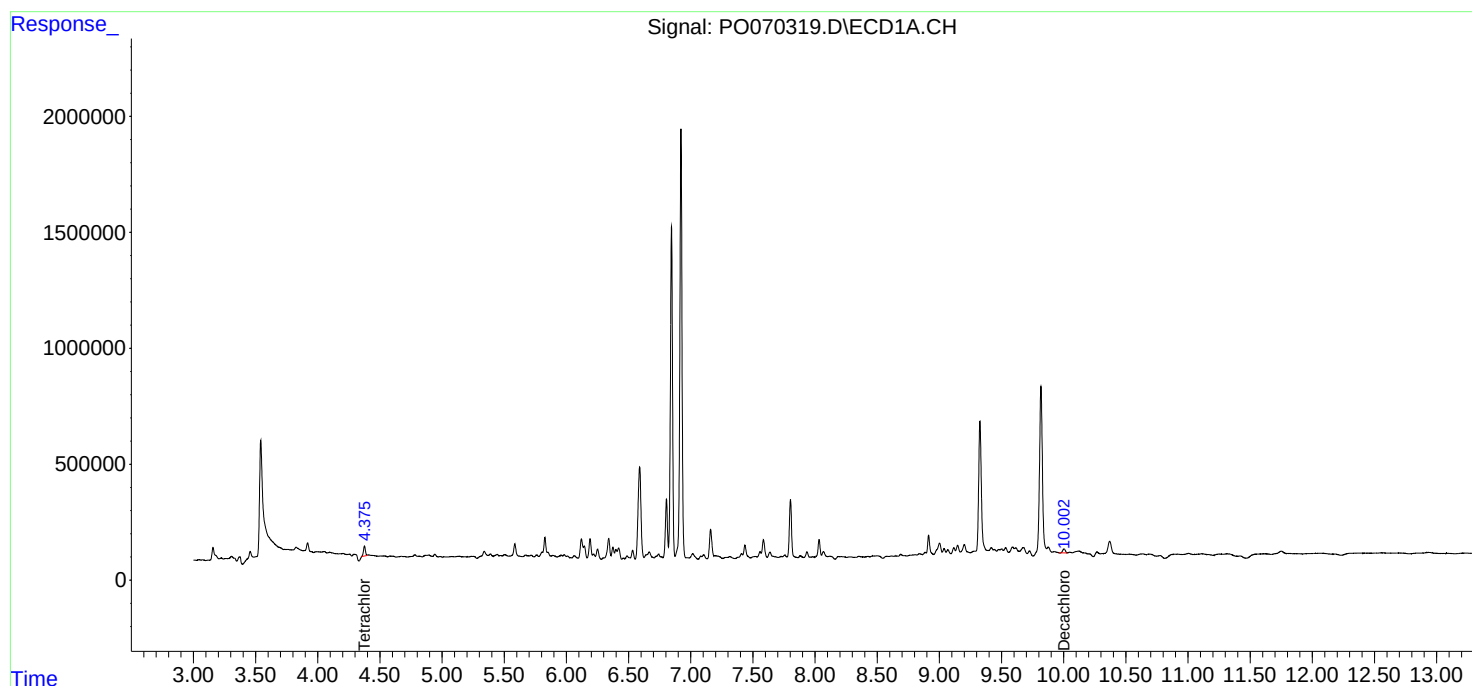

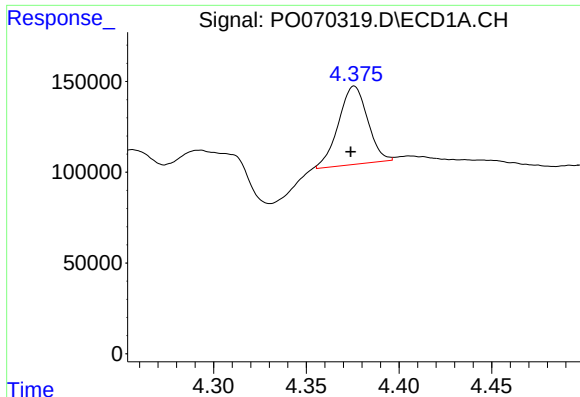


#1 Tetrachloro-m-xylene

R.T.: 4.375 min
Delta R.T.: 0.001 min
Response: 471858
Conc: 7.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OILY-WATER-1493RE


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:04 PM

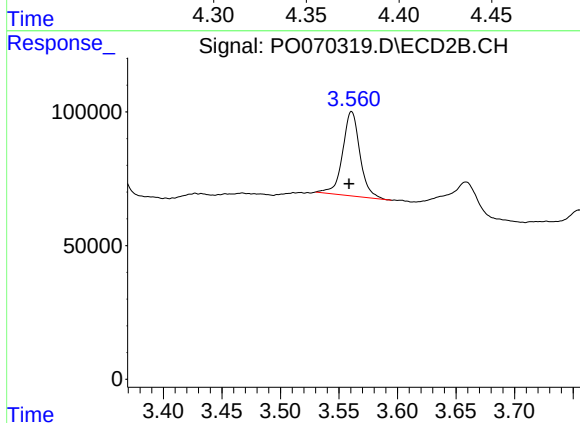


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.002 min
Response: 323779
Conc: 7.35 ng/ml

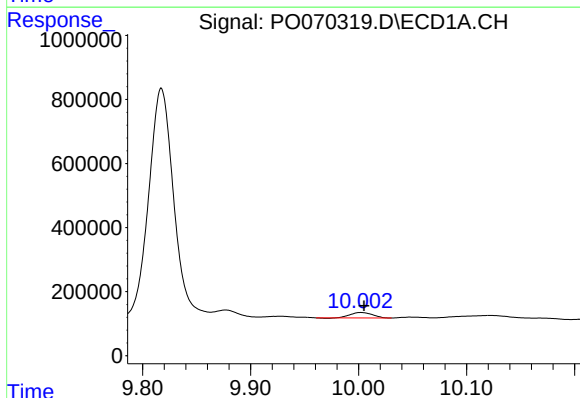

#2 Decachlorobiphenyl

R.T.: 10.002 min
Delta R.T.: -0.003 min
Response: 242570
Conc: 2.83 ng/ml

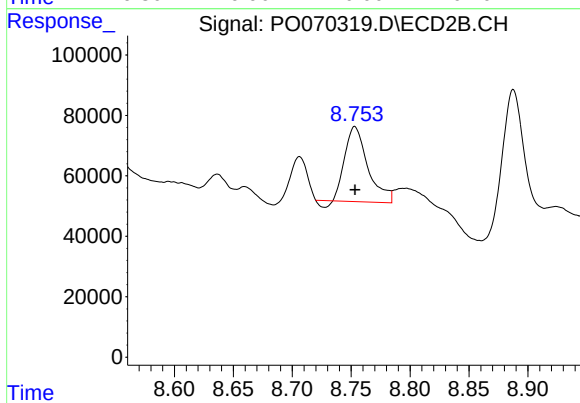

#2 Decachlorobiphenyl

R.T.: 8.753 min
Delta R.T.: 0.000 min
Response: 329297
Conc: 5.93 ng/ml