

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
 Data File : P0070332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2020 19:38
 Operator : DD\AJ
 Sample : L3548-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CRT-004

Manual Integrations
 APPROVED

Ankita
 8/7/2020 1:14:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 05:24:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.559	1458226	945516	22.052	21.460
2) SA Decachlor...	10.004	8.752	1925531	1303550	22.488	23.484
Target Compounds						
31) L7 AR-1260-1	7.335	6.353	55795	20954	13.415m	6.489m#
32) L7 AR-1260-2	7.606	6.551	143669	106773	23.927	24.814
33) L7 AR-1260-3	7.960	6.701	95235	66546	18.504	18.175m
34) L7 AR-1260-4	8.185	7.175	135837	48678	27.935	15.615 #
35) L7 AR-1260-5	8.502	7.427	129671	108215	11.634	13.393

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
Data File : P0070332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2020 19:38
Operator : DD\AJ
Sample : L3548-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CRT-004


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 05:24:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

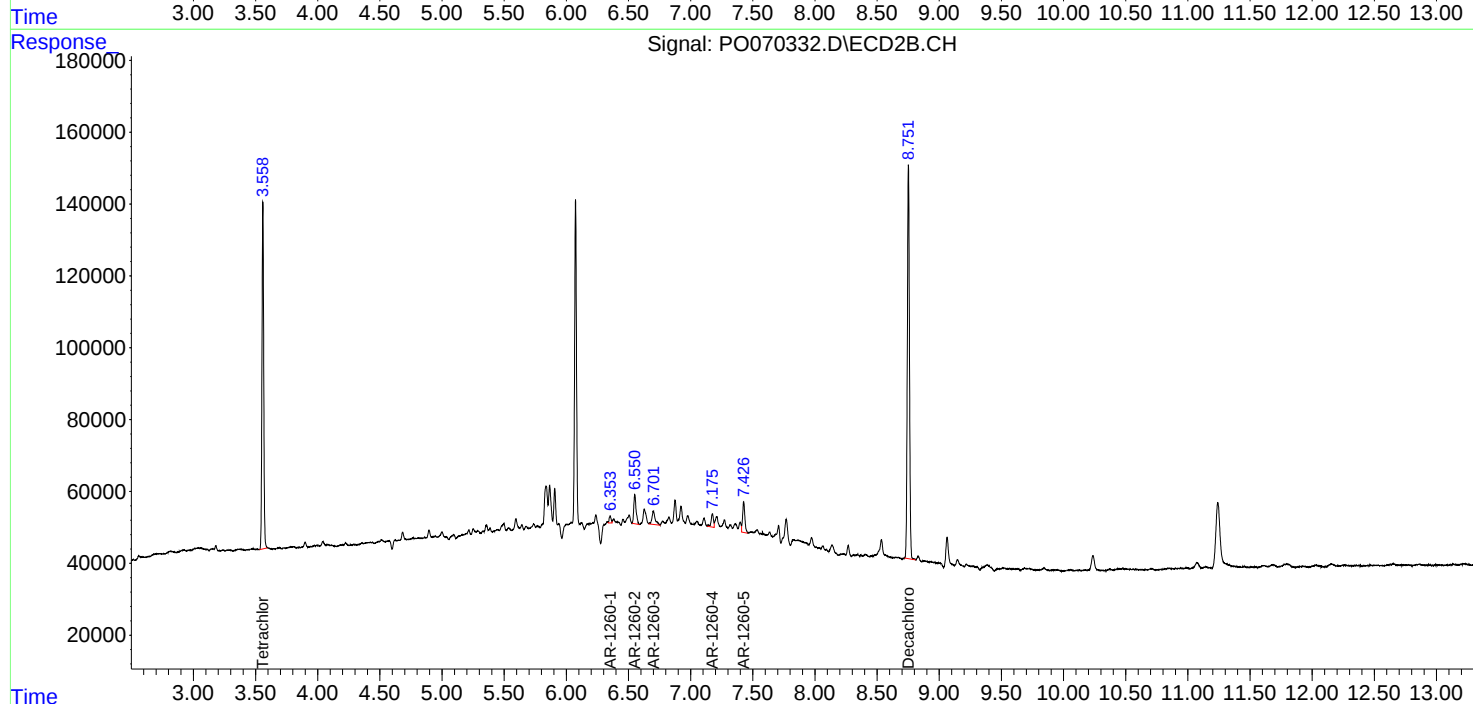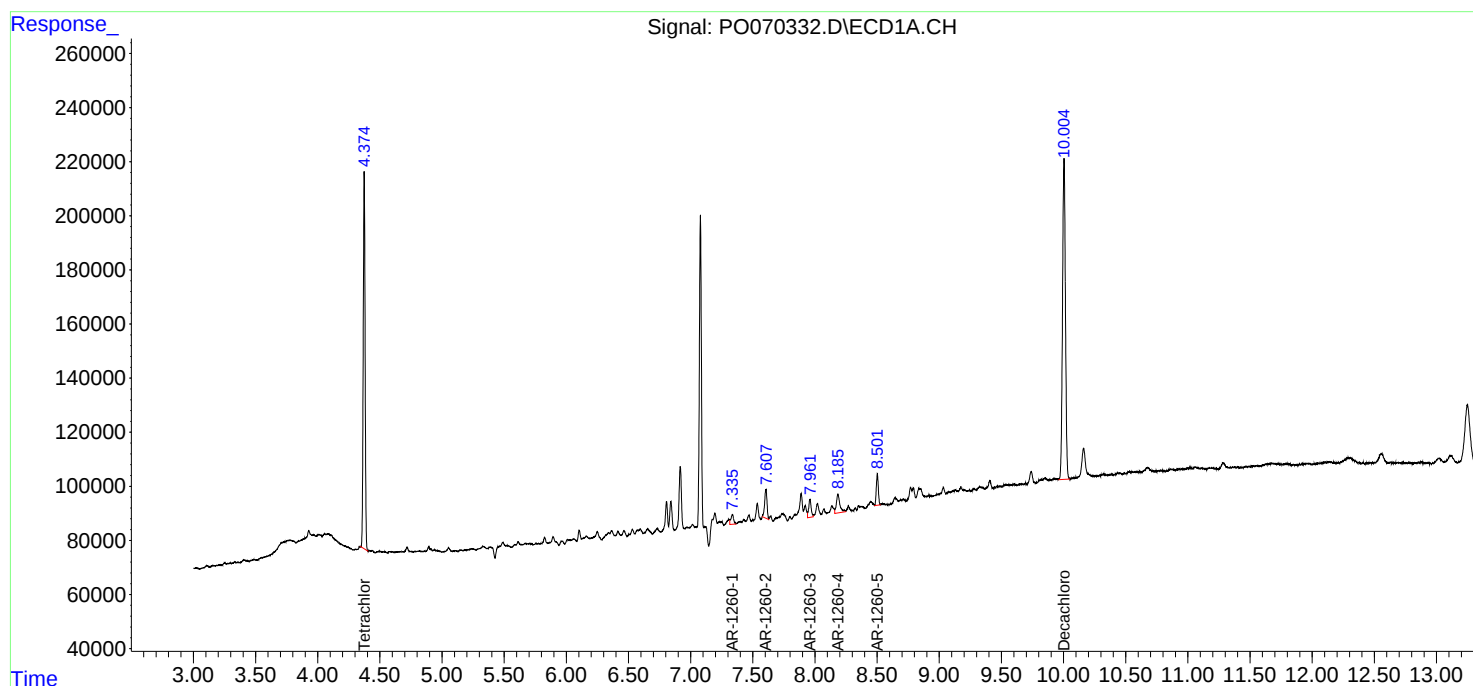

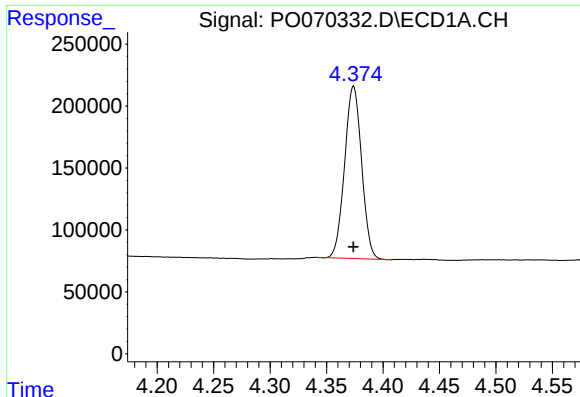


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: 0.000 min
Response: 1458226
Conc: 22.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-004


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:07 PM

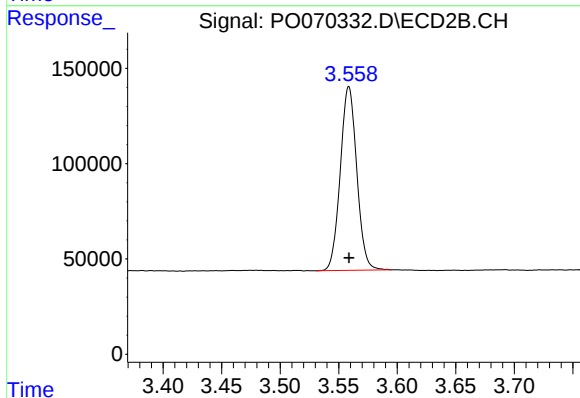


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: 0.000 min
Response: 945516
Conc: 21.46 ng/ml

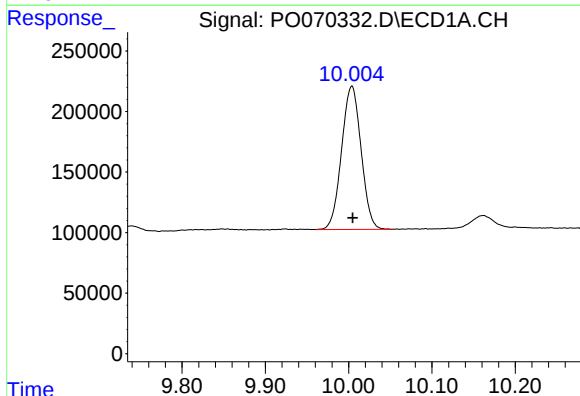


#2 Decachlorobiphenyl

R.T.: 10.004 min
Delta R.T.: -0.001 min
Response: 1925531
Conc: 22.49 ng/ml

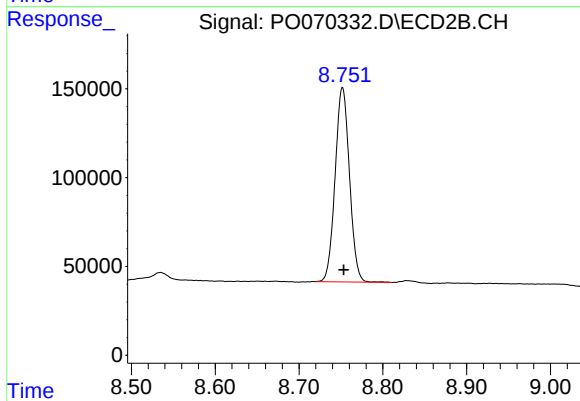

#2 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: -0.001 min
Response: 1303550
Conc: 23.48 ng/ml

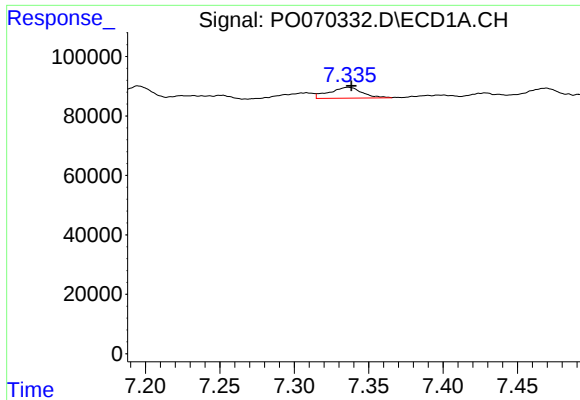


#31 AR-1260-1

R.T.: 7.335 min
Delta R.T.: -0.003 min
Response: 55795
Conc: 13.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CRT-004


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:07 PM

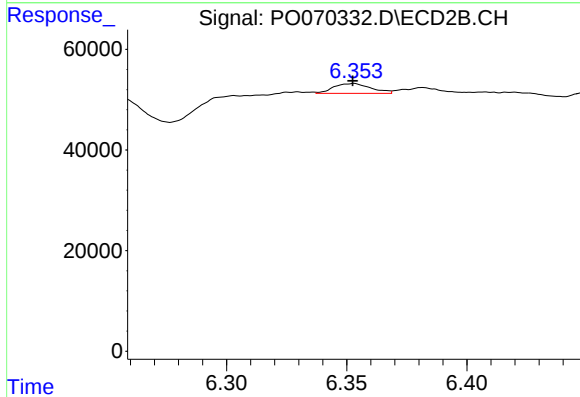


#31 AR-1260-1

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 20954
Conc: 6.49 ng/ml m

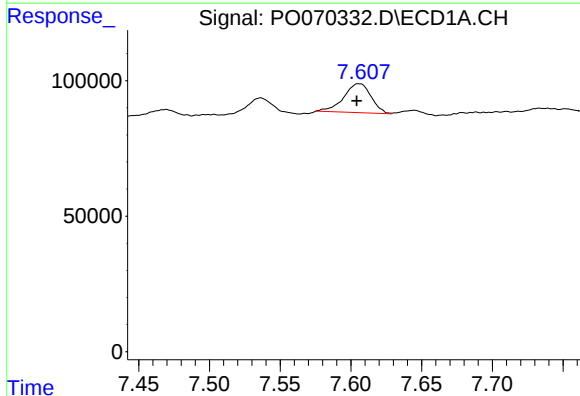


#32 AR-1260-2

R.T.: 7.606 min
Delta R.T.: 0.002 min
Response: 143669
Conc: 23.93 ng/ml

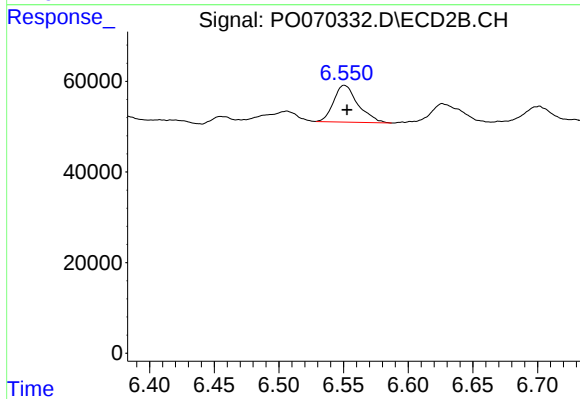

#32 AR-1260-2

R.T.: 6.551 min
Delta R.T.: -0.002 min
Response: 106773
Conc: 24.81 ng/ml

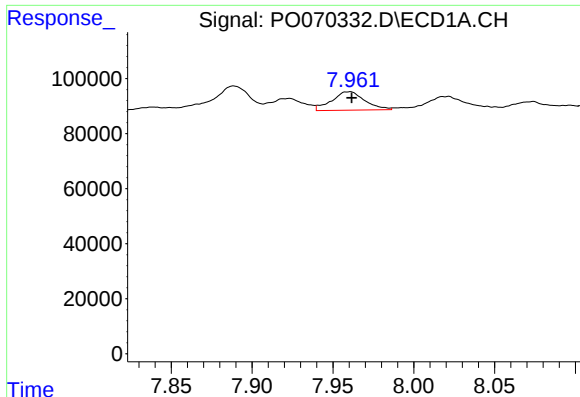


#33 AR-1260-3

R.T.: 7.960 min
Delta R.T.: -0.001 min
Response: 95235
Conc: 18.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-004


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:07 PM

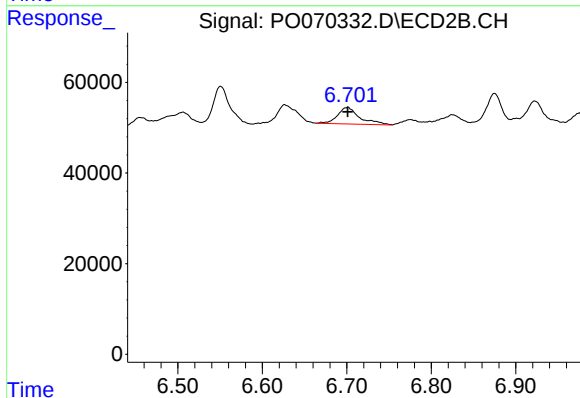


#33 AR-1260-3

R.T.: 6.701 min
Delta R.T.: 0.000 min
Response: 66546
Conc: 18.18 ng/ml m

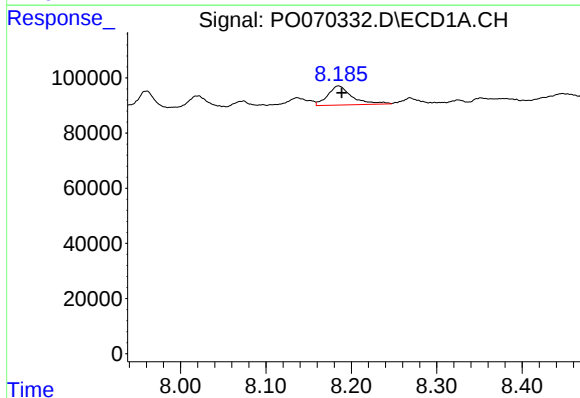


#34 AR-1260-4

R.T.: 8.185 min
Delta R.T.: -0.004 min
Response: 135837
Conc: 27.93 ng/ml

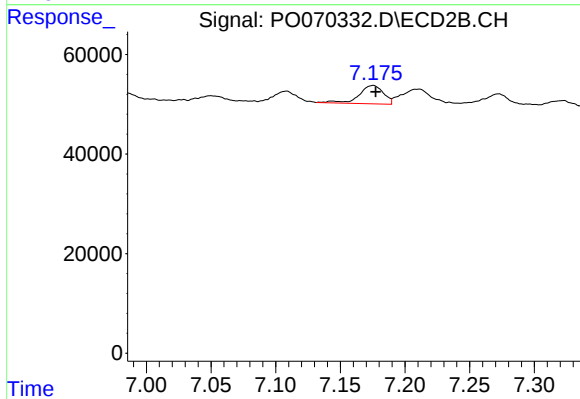

#34 AR-1260-4

R.T.: 7.175 min
Delta R.T.: -0.002 min
Response: 48678
Conc: 15.61 ng/ml

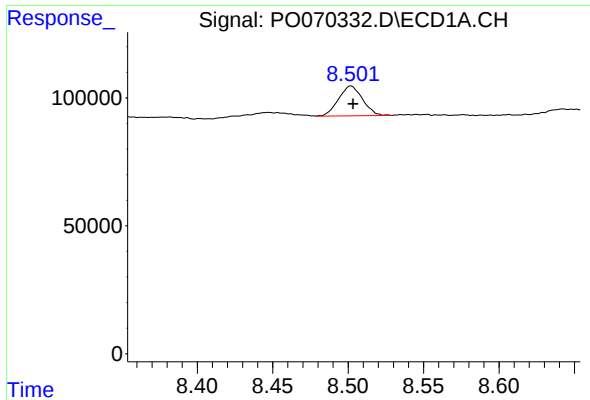


#35 AR-1260-5

R.T.: 8.502 min
Delta R.T.: -0.001 min
Response: 129671
Conc: 11.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-004

Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:07 PM

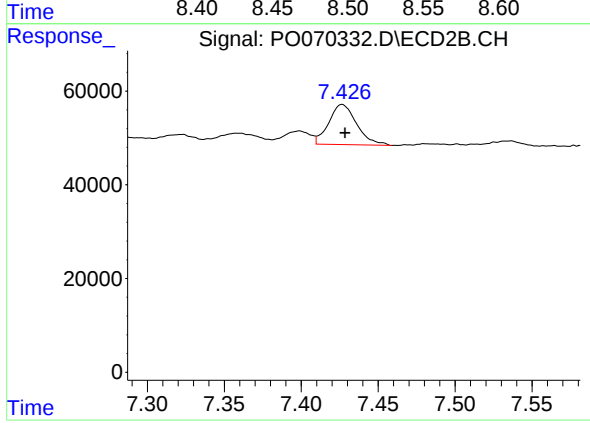

#35 AR-1260-5

R.T.: 7.427 min
Delta R.T.: -0.002 min
Response: 108215
Conc: 13.39 ng/ml