

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
 Data File : P0070345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Aug 2020 23:38
 Operator : DD\AJ
 Sample : L3563-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-30860

Manual Integrations
 APPROVED

Ankita
 8/7/2020 1:14:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 05:30:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.379	3.566	1560334	1113174	23.596	25.265
2) SA Decachlor...	10.044f	8.794f	1625705	883660	18.986m	15.919m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080620\
Data File : P0070345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Aug 2020 23:38
Operator : DD\AJ
Sample : L3563-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-30860


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 05:30:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

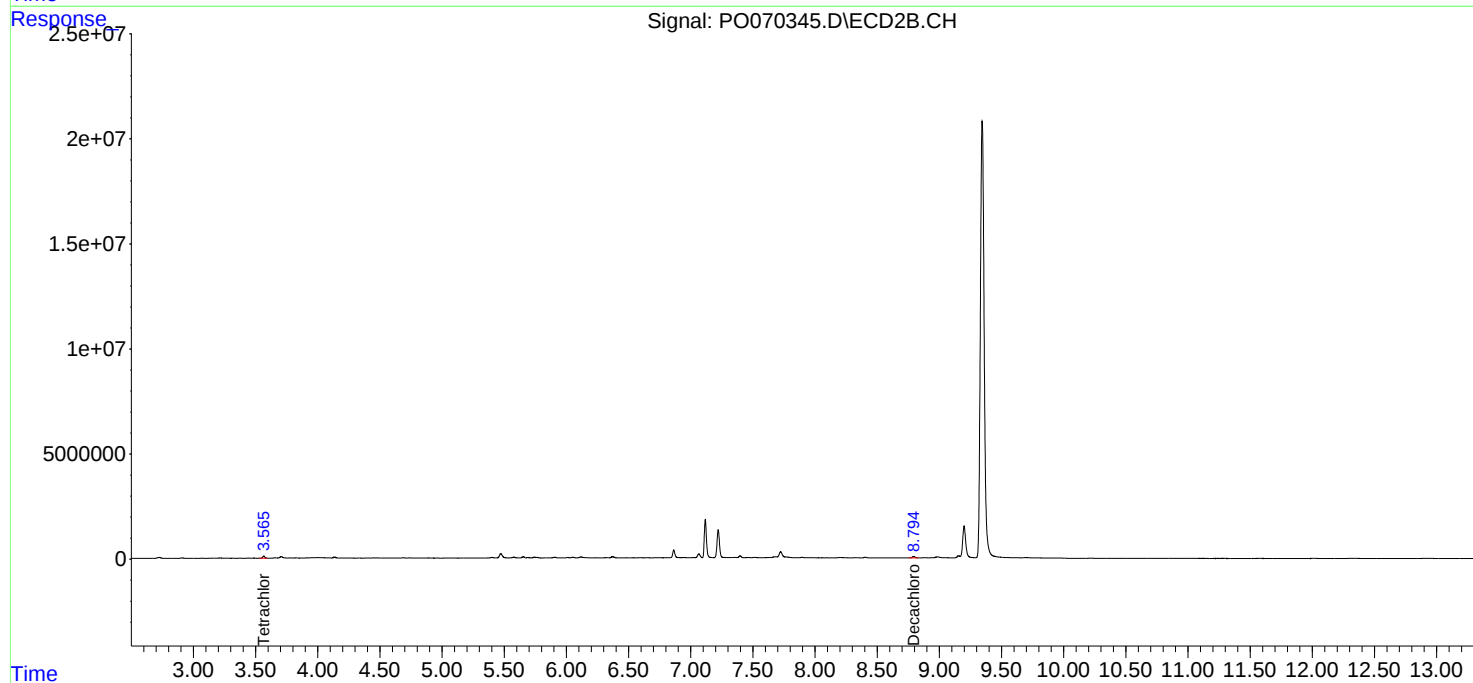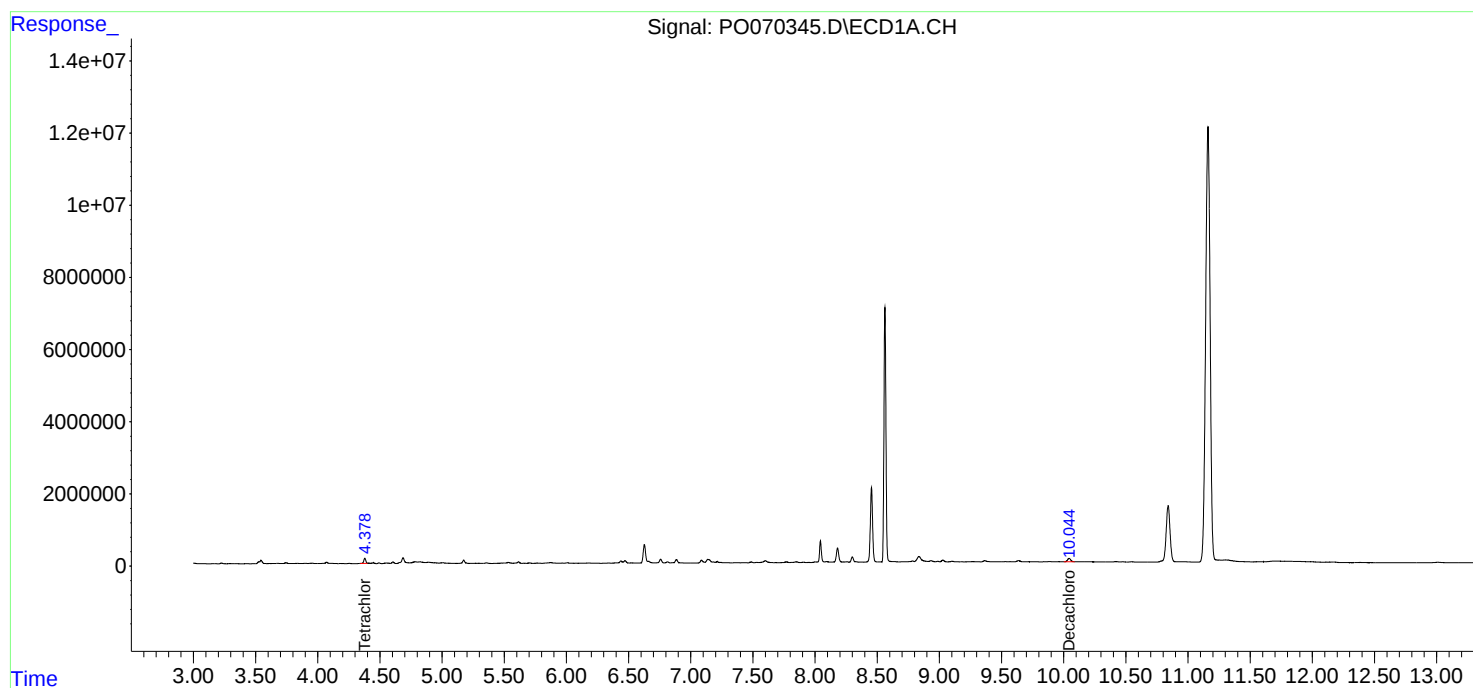

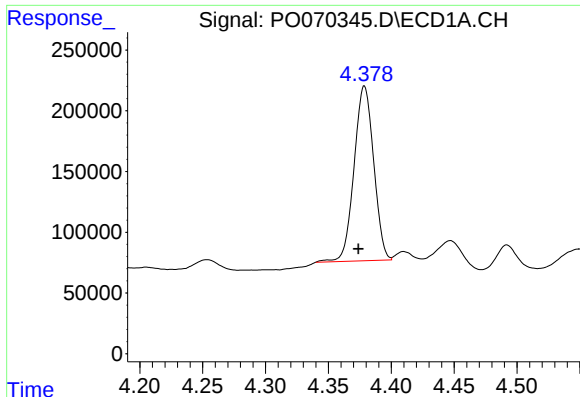


#1 Tetrachloro-m-xylene

R.T.: 4.379 min
Delta R.T.: 0.005 min
Response: 1560334
Conc: 23.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-30860


Manual Integrations
APPROVED

Ankita
8/7/2020 1:14:18 PM

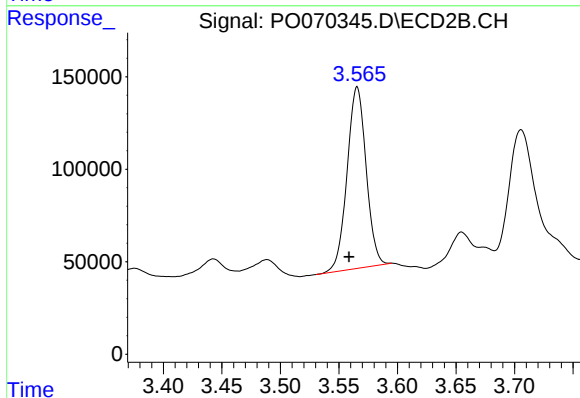


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.007 min
Response: 1113174
Conc: 25.27 ng/ml

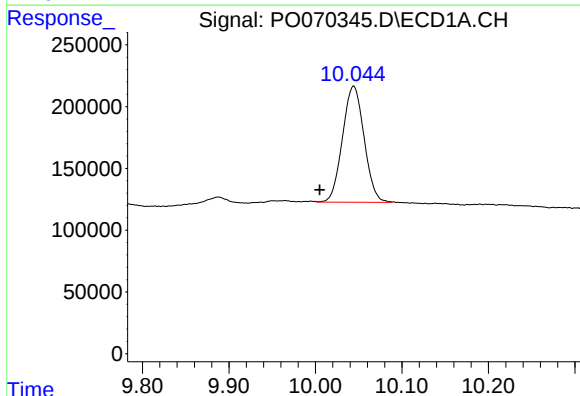

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: 0.039 min
Response: 1625705
Conc: 18.99 ng/ml m

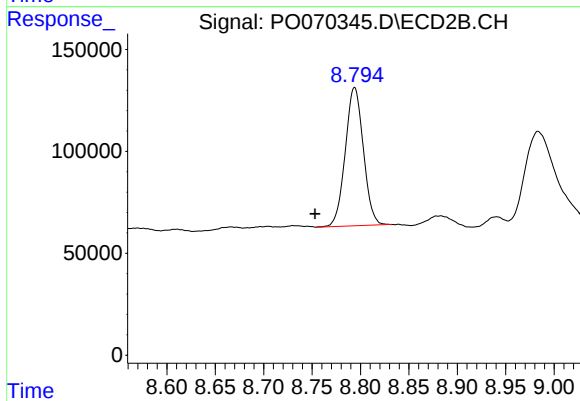

#2 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: 0.040 min
Response: 883660
Conc: 15.92 ng/ml m